

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB050622\
 Data File : FB027121.D
 Signal(s) : FID2B.CH
 Acq On : 6 May 2022 13:22
 Operator : AJ/MA
 Sample : BSF0506S2
 Misc : 0.57G/5.00 ML WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0506S2

Integration File: Calibration.e
 Quant Time: May 08 22:36:54 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040922.M
 Quant Title :
 QLast Update : Sat Apr 09 04:06:25 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.791	273894	24.227 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.707	540633	28.721 ng/ml
2) t 2,2,4-Trimethylpentane	7.420	540254	27.005 ng/ml
3) t n-Heptane	7.749	192297	9.830 ng/ml
4) t Benzene	7.886	210450	9.536 ng/ml
6) t Toluene	10.619	605363	29.358 ng/ml
7) t Ethylbenzene	13.056	188794	9.881 ng/ml
8) t m-Xylene	13.188	372856	19.739 ng/ml
9) t O-Xylene	13.915	360435	19.898 ng/ml
10) t 1,2,4-Trimethylbenzene	16.191	371118	20.135 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB050622\
Data File : FB027121.D
Signal(s) : FID2B.CH
Acq On : 6 May 2022 13:22
Operator : AJ/MA
Sample : BSF0506S2
Misc : 0.57G/5.00 ML WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0506S2

Integration File: Calibration.e
Quant Time: May 08 22:36:54 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040922.M
Quant Title :
QLast Update : Sat Apr 09 04:06:25 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

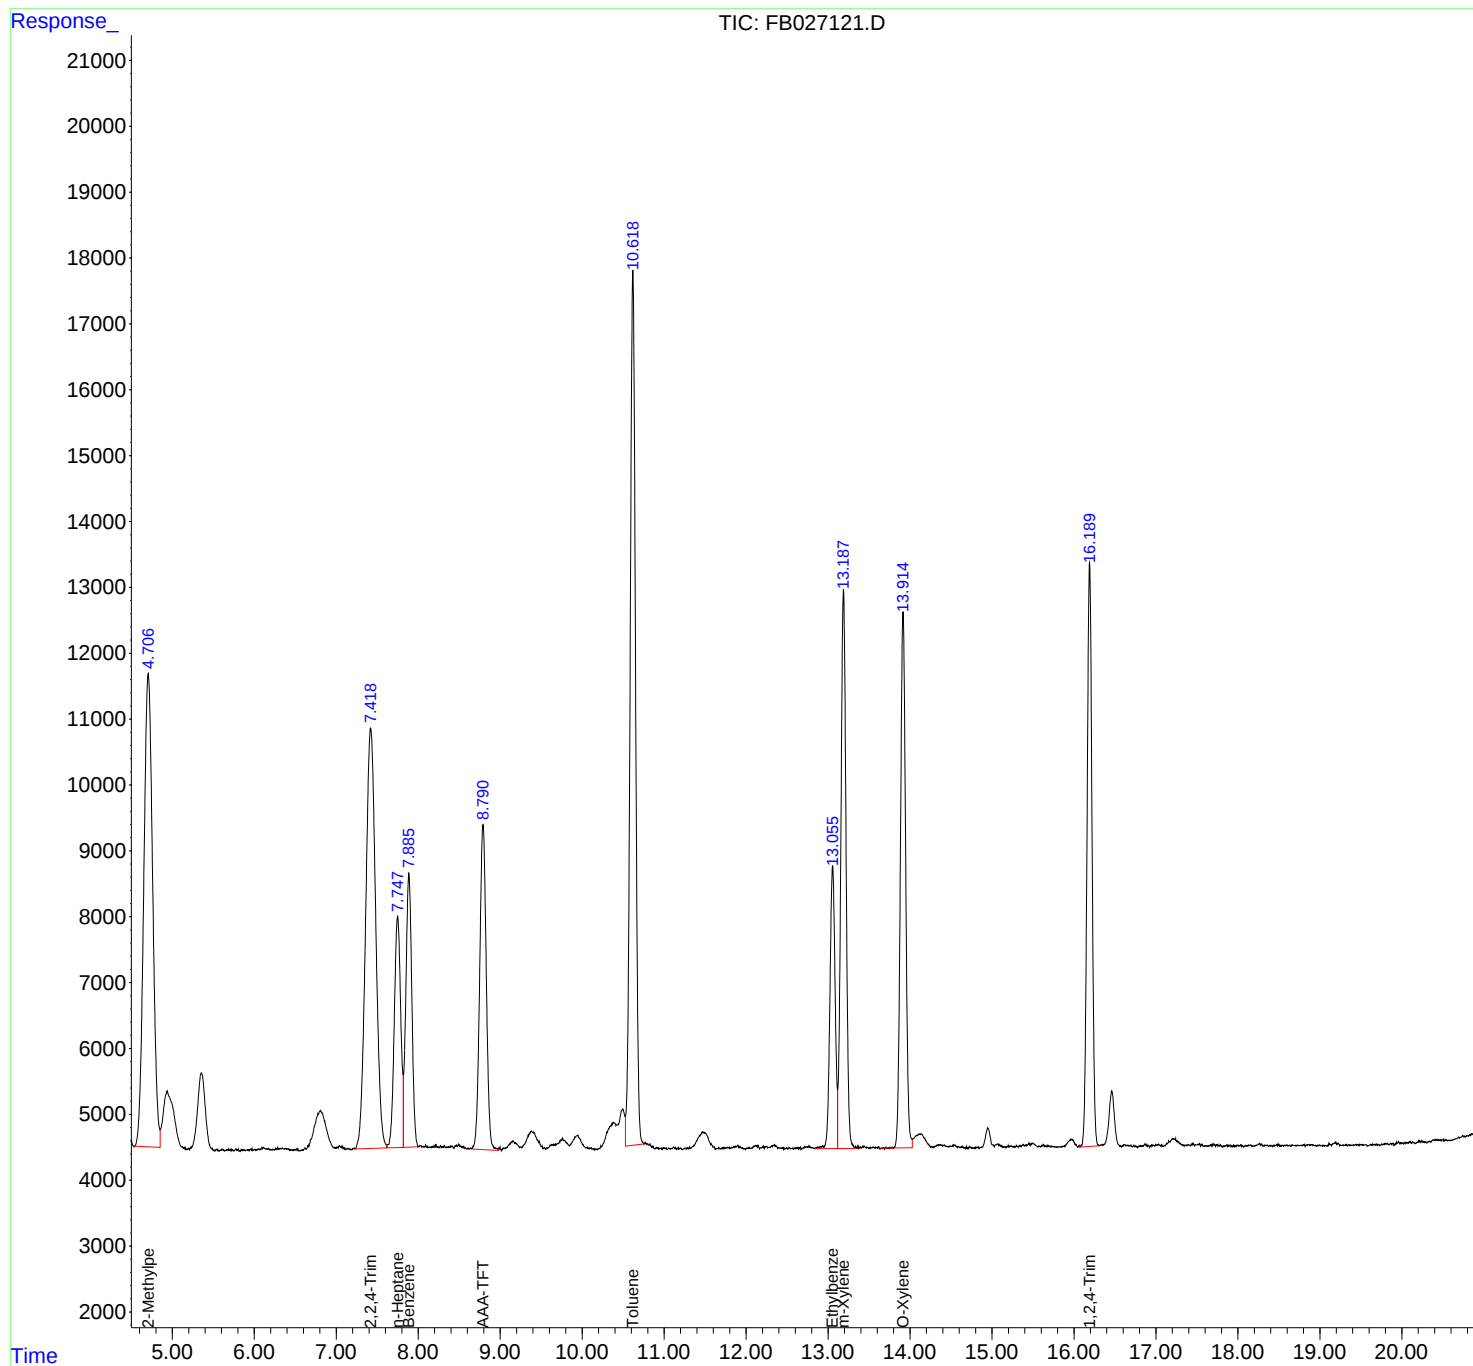


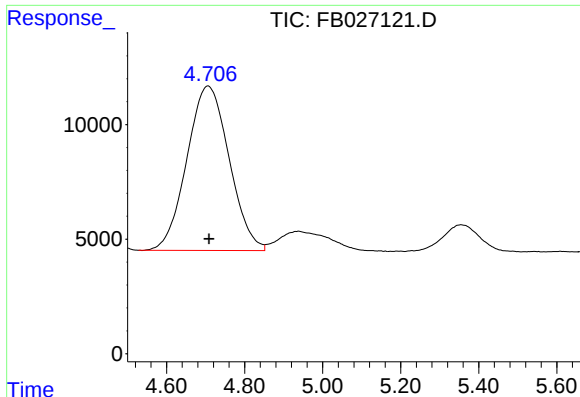

#1 2-Methylpentane


R.T.: 4.707 min
Delta R.T.: -0.002 min
Response: 540633
Conc: 28.72 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0506S2

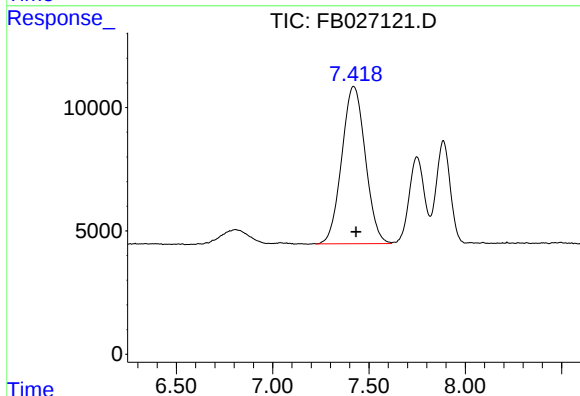


#2 2,2,4-Trimethylpentane

R.T.: 7.420 min
Delta R.T.: -0.014 min
Response: 540254
Conc: 27.01 ng/ml

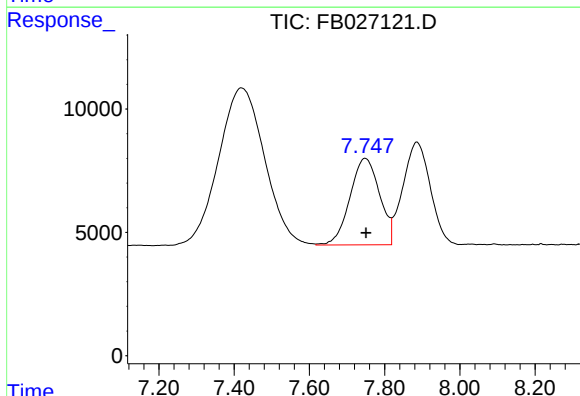


#3 n-Heptane

R.T.: 7.749 min
Delta R.T.: -0.002 min
Response: 192297
Conc: 9.83 ng/ml

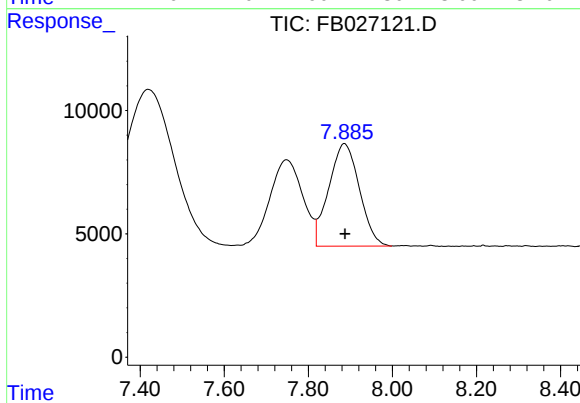

#4 Benzene


R.T.: 7.886 min
Delta R.T.: 0.000 min
Response: 210450
Conc: 9.54 ng/ml

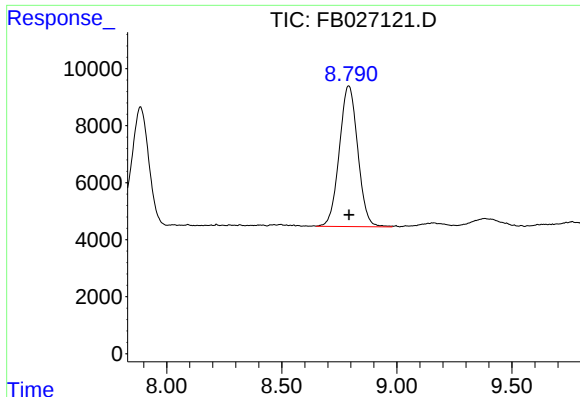

#5 AAA-TFT


R.T.: 8.791 min
Delta R.T.: 0.000 min
Response: 273894
Conc: 24.23 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0506S2

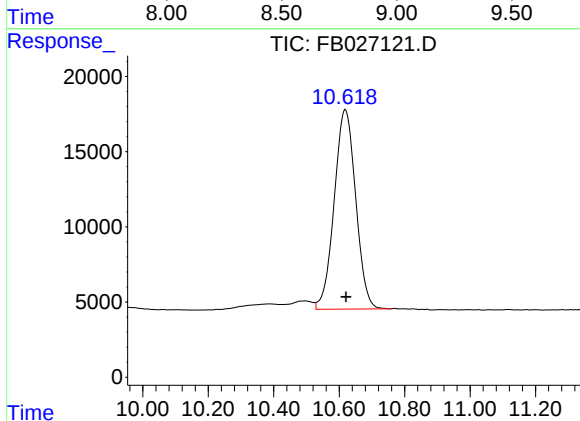


#6 Toluene

R.T.: 10.619 min
Delta R.T.: -0.002 min
Response: 605363
Conc: 29.36 ng/ml

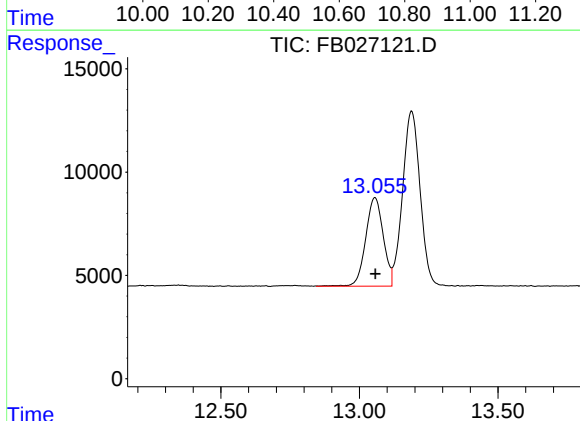


#7 Ethylbenzene

R.T.: 13.056 min
Delta R.T.: -0.002 min
Response: 188794
Conc: 9.88 ng/ml

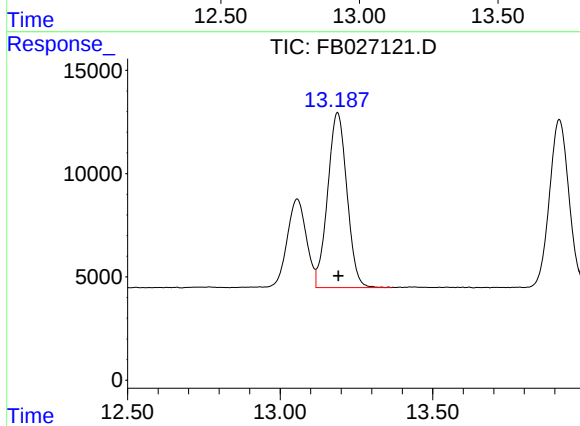

#8 m-Xylene


R.T.: 13.188 min
Delta R.T.: -0.003 min
Response: 372856
Conc: 19.74 ng/ml

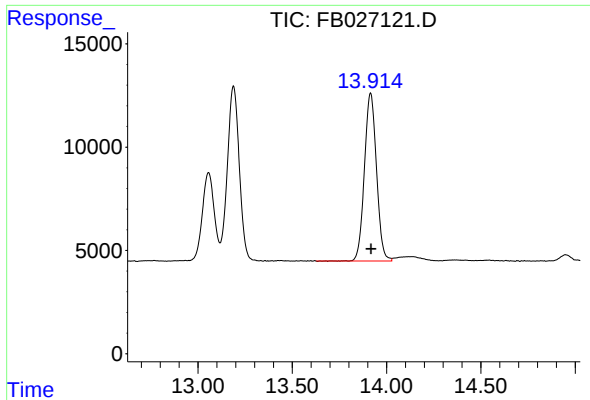

#9 O-Xylene

R.T.: 13.915 min
Delta R.T.: -0.003 min
Response: 360435
Conc: 19.90 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0506S2

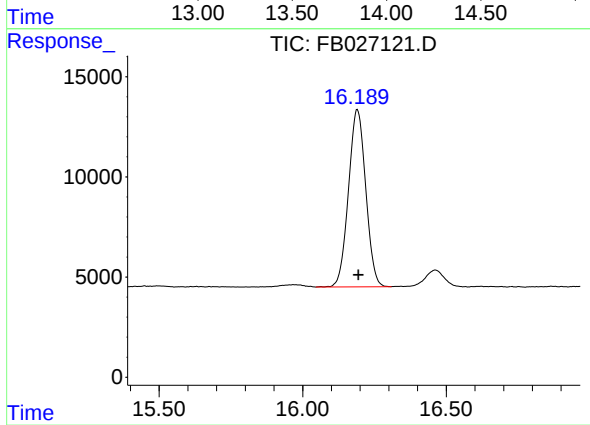

#10 1,2,4-Trimethylbenzene

R.T.: 16.191 min
Delta R.T.: -0.003 min
Response: 371118
Conc: 20.13 ng/ml