

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB050625\
Data File : FB031679.D
Signal(s) : FID2B.CH
Acq On : 6 May 2025 10:29
Operator : YP/AJ
Sample : VBF0506S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: May 07 05:51:32 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB042325.M
Quant Title :
QLast Update : Wed Apr 23 13:48:24 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.793	359879	15.693 ng/ml
Target Compounds			
6) t Toluene	10.622	22314	0.560 ng/ml
7) t Ethylbenzene	13.062	9233	0.258 ng/ml
8) t m-Xylene	13.191	32635	0.835 ng/ml
9) t O-Xylene	13.912	18716	0.508 ng/ml
10) t 1,2,4-Trimethylbenzene	16.193	35470	1.315 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB050625\
Data File : FB031679.D
Signal(s) : FID2B.CH
Acq On : 6 May 2025 10:29
Operator : YP/AJ
Sample : VBF0506S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: May 07 05:51:32 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB042325.M
Quant Title :
QLast Update : Wed Apr 23 13:48:24 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

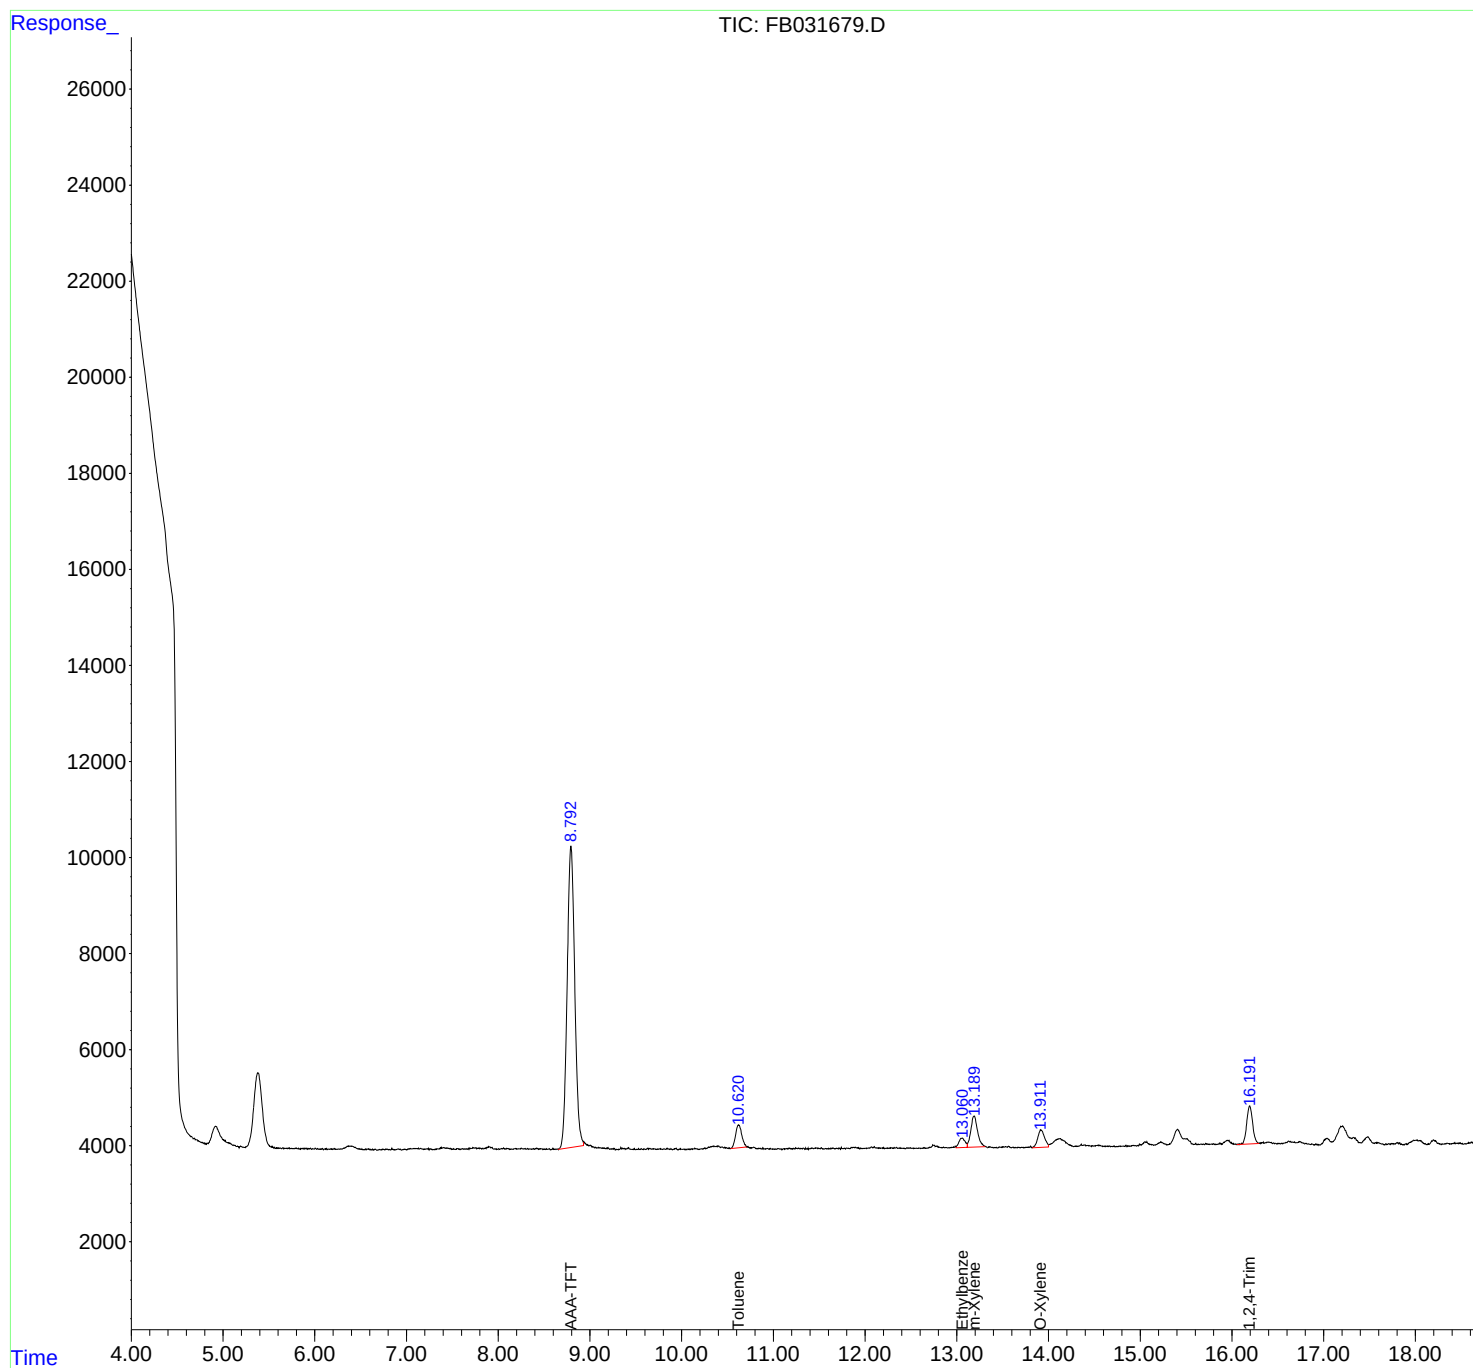


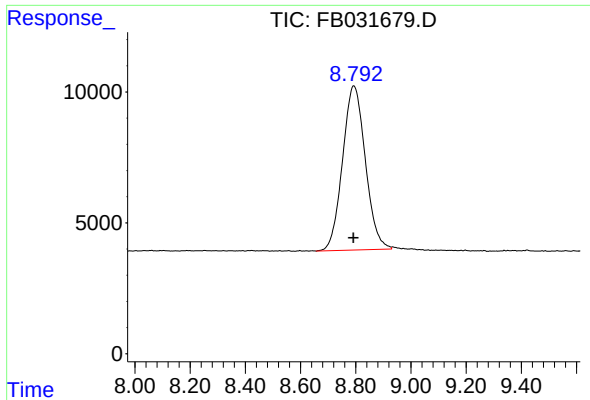

#5 AAA-TFT


R.T.: 8.793 min
Delta R.T.: 0.002 min
Response: 359879
Conc: 15.69 ng/ml

Instrument :
FID_B
ClientSampleId :

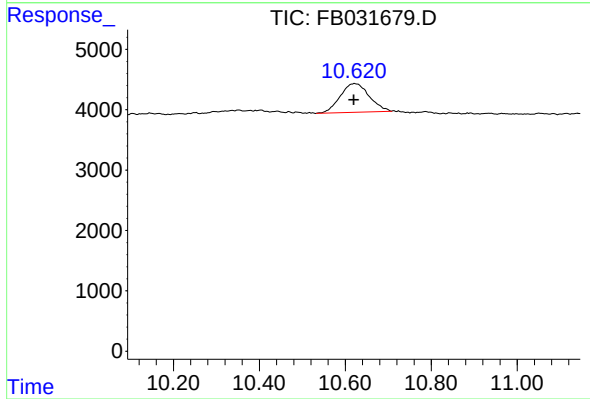


#6 Toluene

R.T.: 10.622 min
Delta R.T.: 0.002 min
Response: 22314
Conc: 0.56 ng/ml

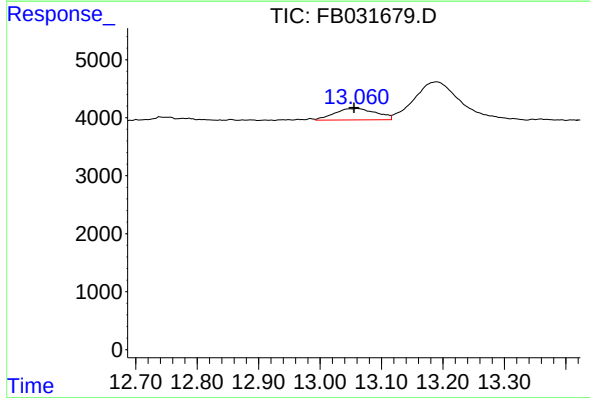


#7 Ethylbenzene

R.T.: 13.062 min
Delta R.T.: 0.006 min
Response: 9233
Conc: 0.26 ng/ml

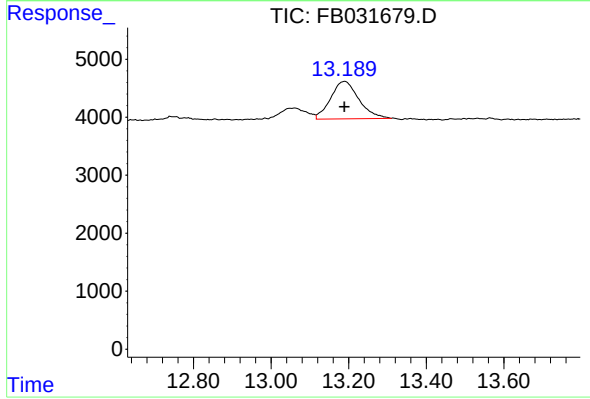

#8 m-Xylene


R.T.: 13.191 min
Delta R.T.: 0.002 min
Response: 32635
Conc: 0.84 ng/ml

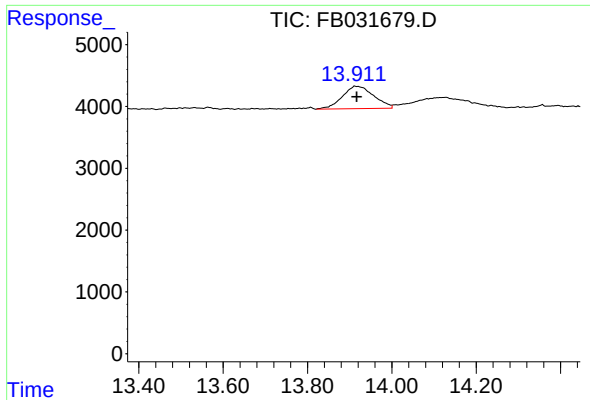

#9 O-Xylene

R.T.: 13.912 min
Delta R.T.: -0.005 min
Response: 18716
Conc: 0.51 ng/ml

Instrument :
FID_B
ClientSampleId :

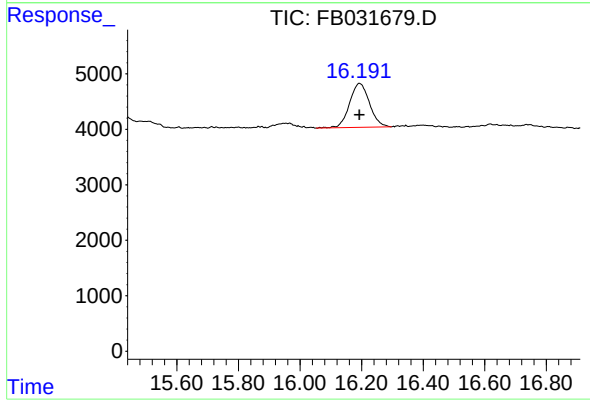

#10 1,2,4-Trimethylbenzene

R.T.: 16.193 min
Delta R.T.: 0.000 min
Response: 35470
Conc: 1.31 ng/ml