

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB050625\
Data File : FB031683.D
Signal(s) : FID2B.CH
Acq On : 6 May 2025 12:48
Operator : YP/AJ
Sample : Q1956-02
Misc : 5.56G/5.00 ML DI WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: May 07 05:52:14 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB042325.M
Quant Title :
QLast Update : Wed Apr 23 13:48:24 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.795	397323	17.325 ng/ml
Target Compounds			
6) t Toluene	10.625	12053	0.303 ng/ml
7) t Ethylbenzene	13.049	2459	0.069 ng/ml
8) t m-Xylene	13.188	14768	0.378 ng/ml
9) t O-Xylene	13.913	5192	0.141 ng/ml
10) t 1,2,4-Trimethylbenzene	16.201	16355	0.606 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB050625\
Data File : FB031683.D
Signal(s) : FID2B.CH
Acq On : 6 May 2025 12:48
Operator : YP/AJ
Sample : Q1956-02
Misc : 5.56G/5.00 ML DI WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: May 07 05:52:14 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB042325.M
Quant Title :
QLast Update : Wed Apr 23 13:48:24 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

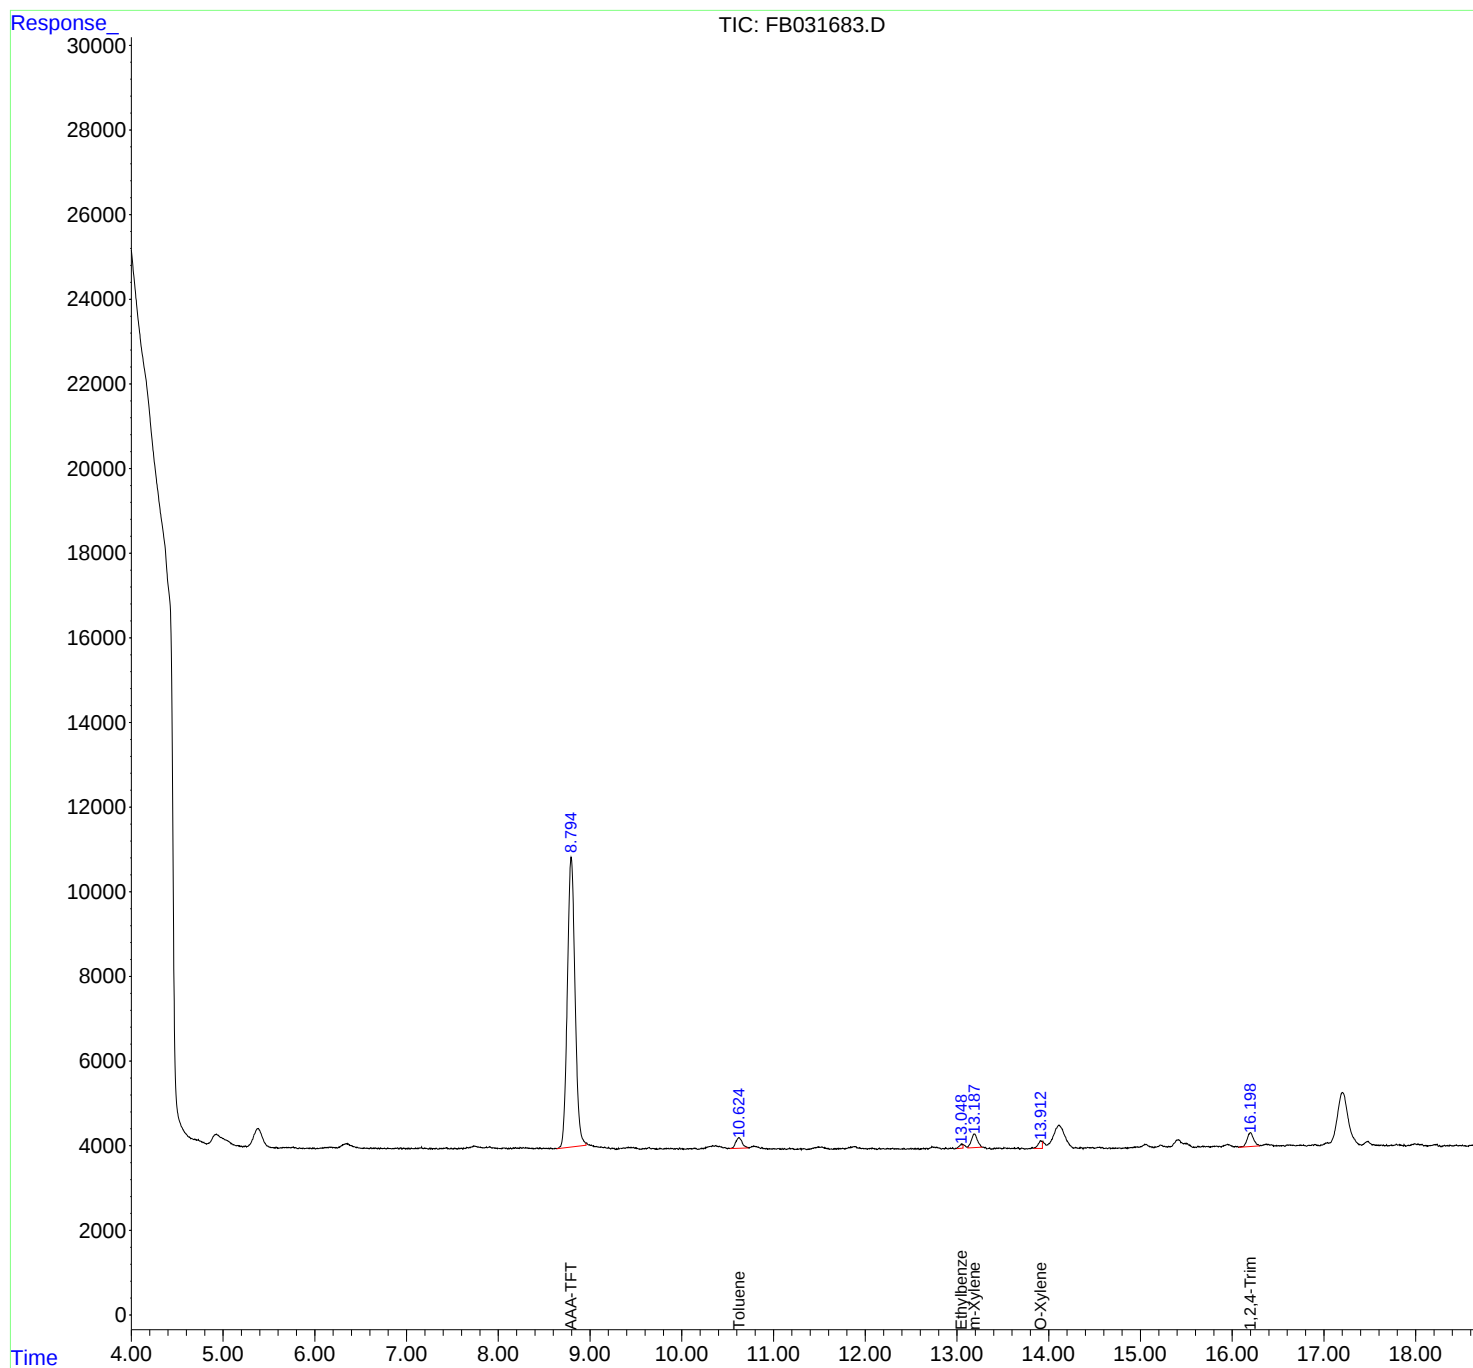


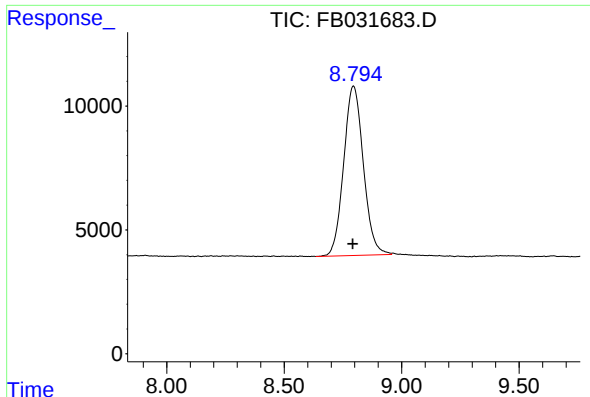

#5 AAA-TFT


R.T.: 8.795 min
Delta R.T.: 0.003 min
Response: 397323
Conc: 17.33 ng/ml

Instrument :
FID_B
ClientSampleId :

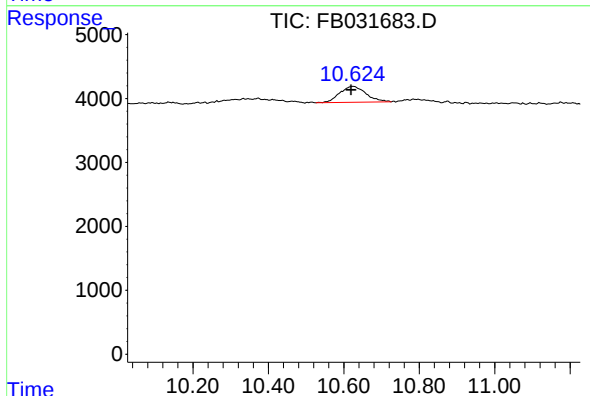


#6 Toluene

R.T.: 10.625 min
Delta R.T.: 0.005 min
Response: 12053
Conc: 0.30 ng/ml

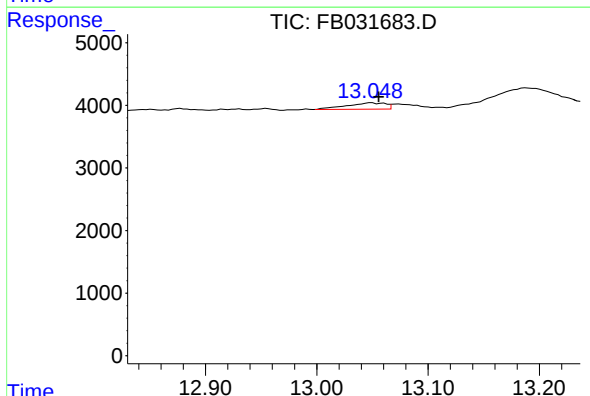


#7 Ethylbenzene

R.T.: 13.049 min
Delta R.T.: -0.006 min
Response: 2459
Conc: 0.07 ng/ml

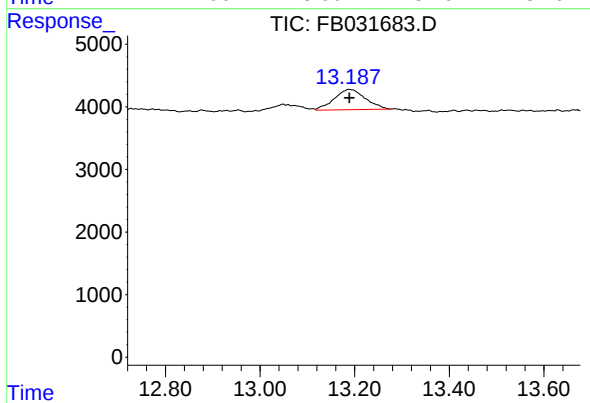

#8 m-Xylene


R.T.: 13.188 min
Delta R.T.: 0.000 min
Response: 14768
Conc: 0.38 ng/ml

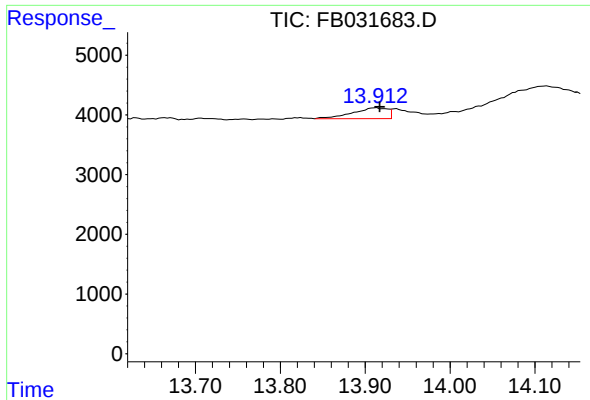

#9 O-Xylene

R.T.: 13.913 min
Delta R.T.: -0.004 min
Response: 5192
Conc: 0.14 ng/ml

Instrument :
FID_B
ClientSampleId :

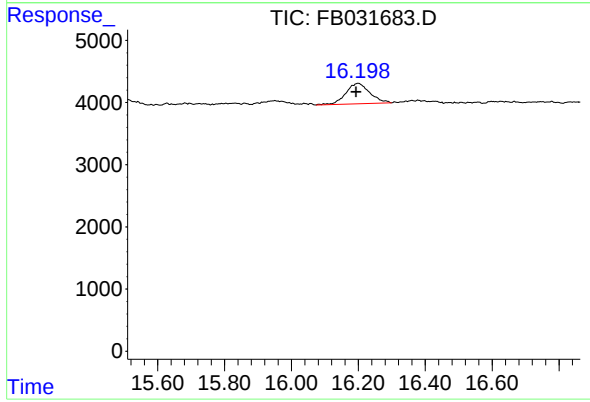

#10 1,2,4-Trimethylbenzene

R.T.: 16.201 min
Delta R.T.: 0.008 min
Response: 16355
Conc: 0.61 ng/ml