

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB050720\
Data File : FB024265.D
Signal(s) : FID2B.CH
Acq On : 7 May 2020 8:38
Operator : DD/AJ
Sample : BSF0507S1
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: May 07 17:32:01 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040820.M
Quant Title :
QLast Update : Wed Apr 08 10:11:26 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.800	537723	21.463 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.692	1041998	31.922 ng/ml
2) t	2,2,4-Trimethylpentane	7.419	1127863	33.049 ng/ml
3) t	n-Heptane	7.759	372998	11.051 ng/ml
4) t	Benzene	7.893	438149	10.856 ng/ml
6) t	Toluene	10.631	1267057	32.231 ng/ml
7) t	Ethylbenzene	13.072	390894	10.723 ng/ml
8) t	m-Xylene	13.204	757102	21.628 ng/ml
9) t	O-Xylene	13.932	738681	21.673 ng/ml
10) t	1,2,4-Trimethylbenzene	16.210	629608	22.174 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB050720\
Data File : FB024265.D
Signal(s) : FID2B.CH
Acq On : 7 May 2020 8:38
Operator : DD/AJ
Sample : BSF0507S1
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: May 07 17:32:01 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040820.M
Quant Title :
QLast Update : Wed Apr 08 10:11:26 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

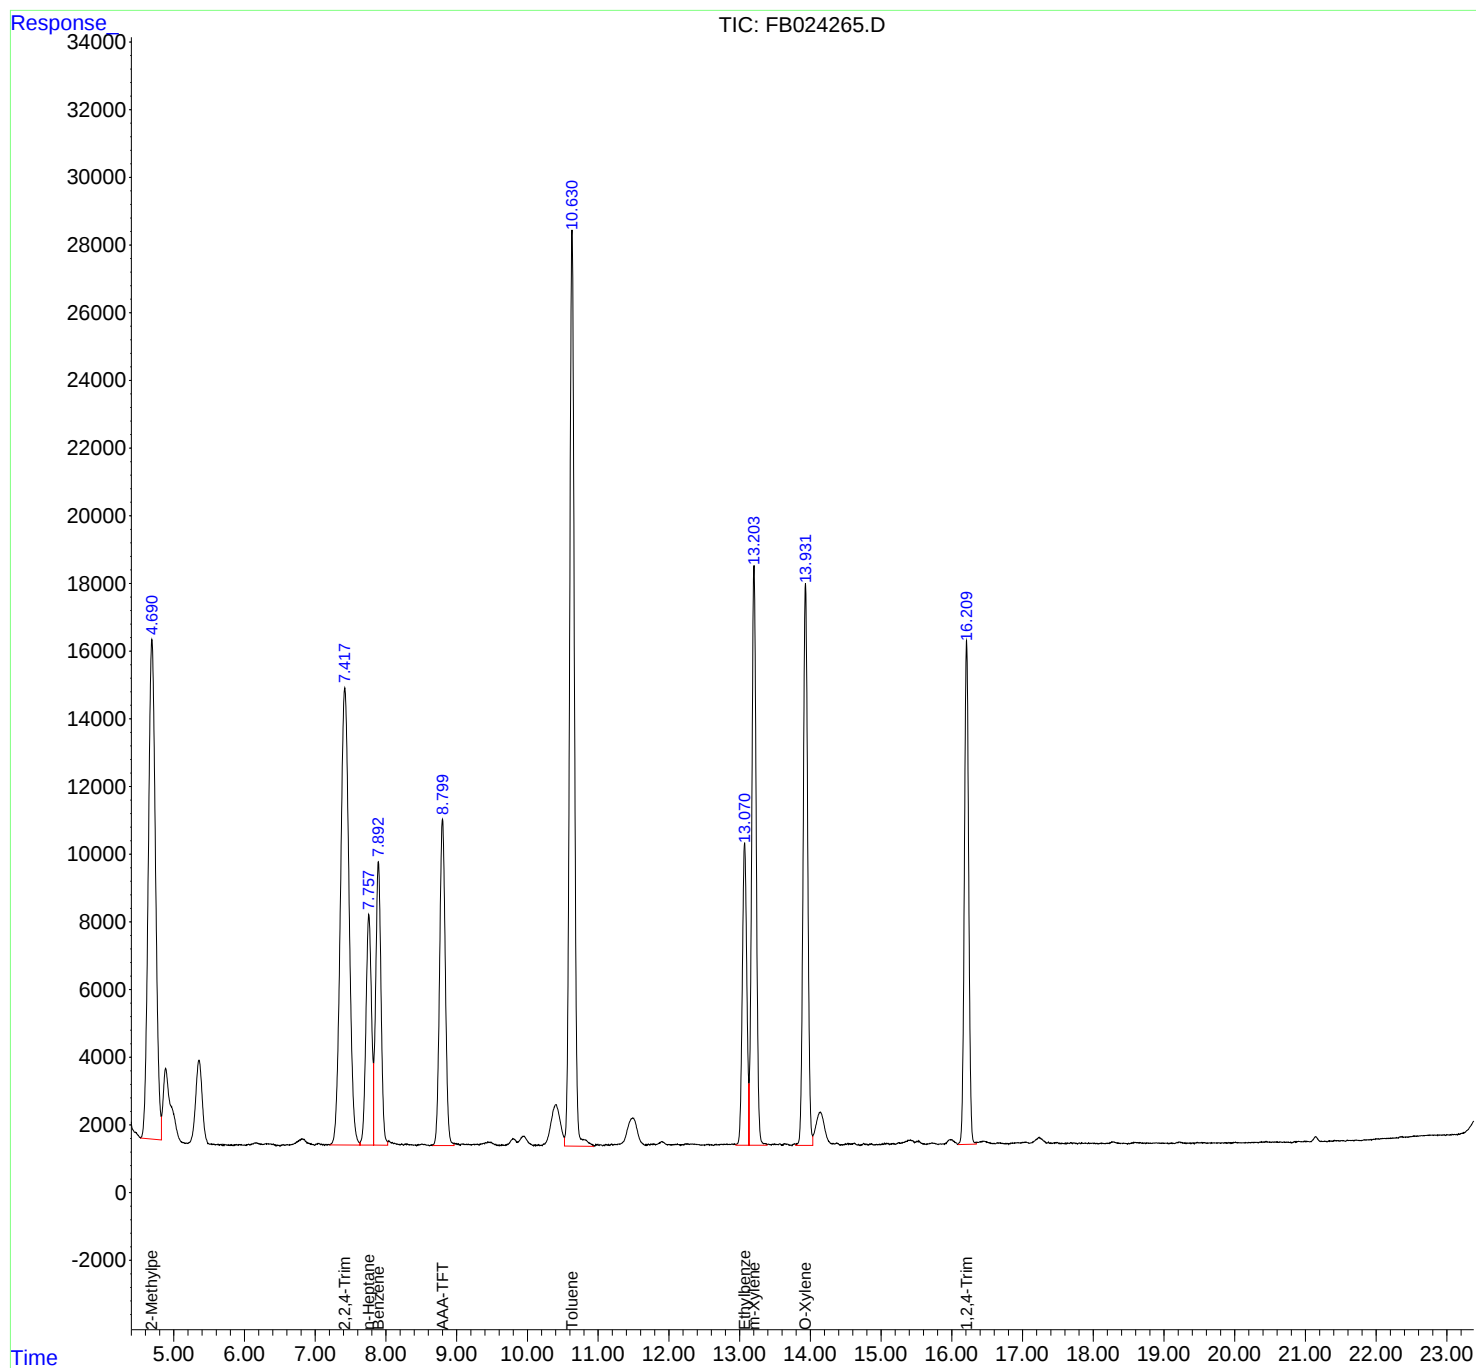

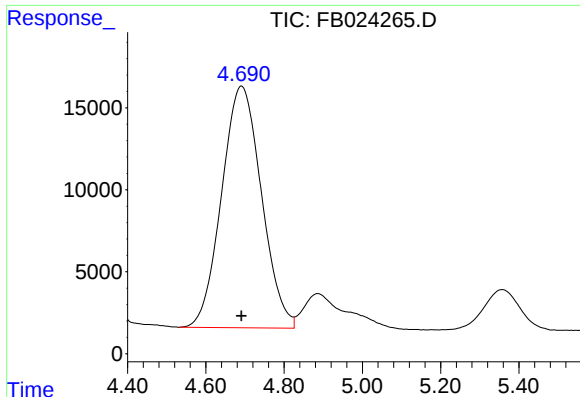


#1 2-Methylpentane

R.T.: 4.692 min
Delta R.T.: 0.000 min
Response: 1041998
Conc: 31.92 ng/ml

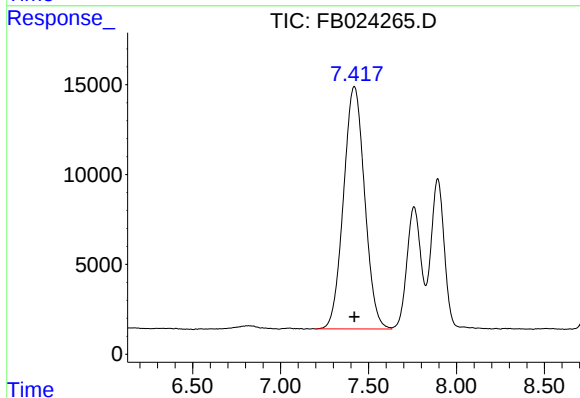


#2 2,2,4-Trimethylpentane

R.T.: 7.419 min
Delta R.T.: 0.000 min
Response: 1127863
Conc: 33.05 ng/ml

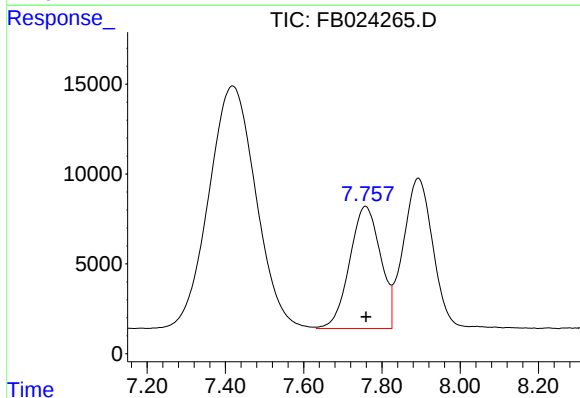


#3 n-Heptane

R.T.: 7.759 min
Delta R.T.: -0.001 min
Response: 372998
Conc: 11.05 ng/ml

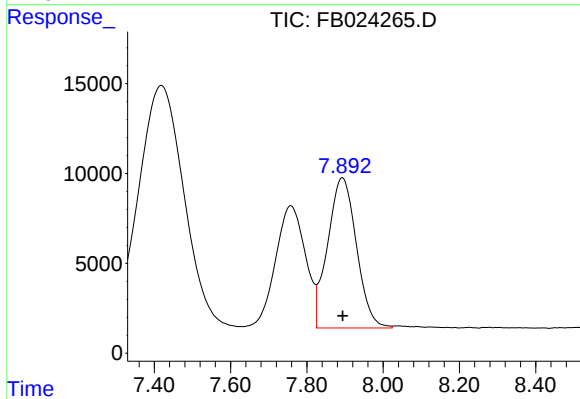


#4 Benzene

R.T.: 7.893 min
Delta R.T.: 0.000 min
Response: 438149
Conc: 10.86 ng/ml

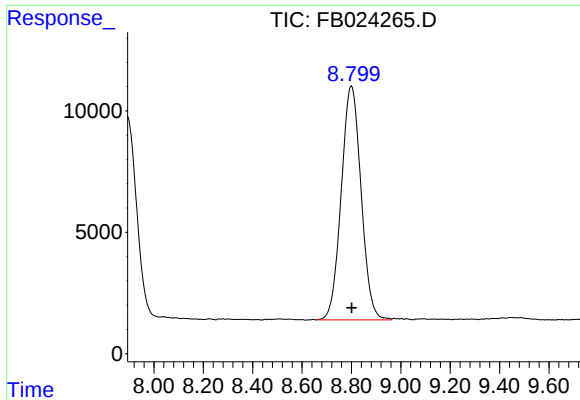


#5 AAA-TFT

R.T.: 8.800 min
 Delta R.T.: 0.000 min
 Response: 537723
 Conc: 21.46 ng/ml

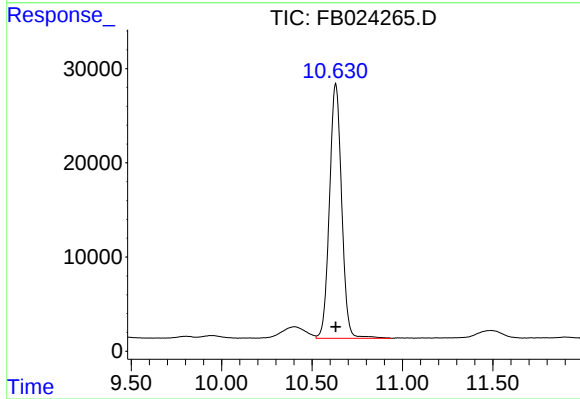


#6 Toluene

R.T.: 10.631 min
 Delta R.T.: 0.000 min
 Response: 1267057
 Conc: 32.23 ng/ml

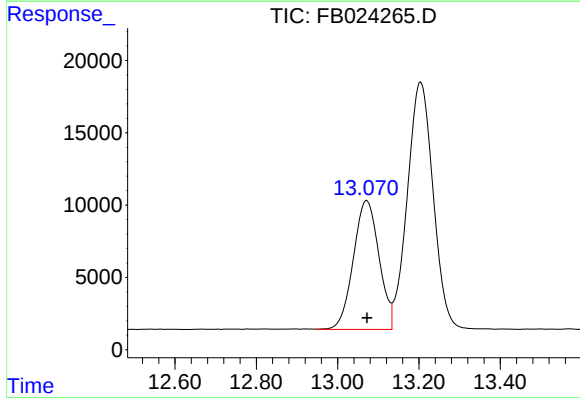


#7 Ethylbenzene

R.T.: 13.072 min
 Delta R.T.: 0.000 min
 Response: 390894
 Conc: 10.72 ng/ml

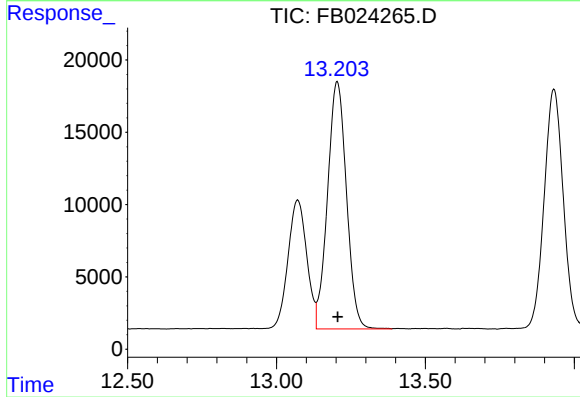


#8 m-Xylene

R.T.: 13.204 min
 Delta R.T.: -0.001 min
 Response: 757102
 Conc: 21.63 ng/ml

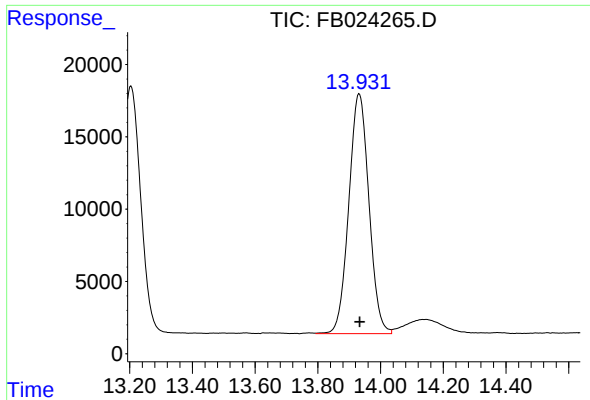

#9 O-Xylene

R.T.: 13.932 min
Delta R.T.: -0.001 min
Response: 738681
Conc: 21.67 ng/ml

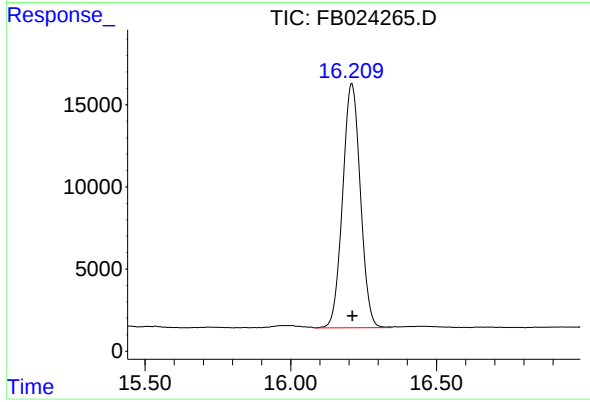

#10 1,2,4-Trimethylbenzene

R.T.: 16.210 min
Delta R.T.: -0.002 min
Response: 629608
Conc: 22.17 ng/ml