

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB050721\
 Data File : FB025730.D
 Signal(s) : FID2B.CH
 Acq On : 7 May 2021 15:08
 Operator : DD/AJ
 Sample : M2265-01MSD
 Misc : 5.03g/5.00ml dI WATER
 ALS Vial : 13 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: May 07 15:31:42 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB050521.M
 Quant Title :
 QLast Update : Thu May 06 15:01:51 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.272	403895	18.817 ng/ml
Target Compounds			
2) t 2,2,4-Trimethylpentane	7.951	662238	30.773 ng/ml
3) t n-Heptane	8.263	306910	10.149 ng/ml
4) t Benzene	8.415	384342	10.048 ng/ml
6) t Toluene	11.077	1113173	29.754 ng/ml
7) t Ethylbenzene	13.471	354098	9.782 ng/ml
8) t m-Xylene	13.601	710292	19.534 ng/ml
9) t O-Xylene	14.322	681002	19.727 ng/ml
10) t 1,2,4-Trimethylbenzene	16.571	552963	19.462 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB050721\
Data File : FB025730.D
Signal(s) : FID2B.CH
Acq On : 7 May 2021 15:08
Operator : DD/AJ
Sample : M2265-01MSD
Misc : 5.03g/5.00ml dI WATER
ALS Vial : 13 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: May 07 15:31:42 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB050521.M
Quant Title :
QLast Update : Thu May 06 15:01:51 2021
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

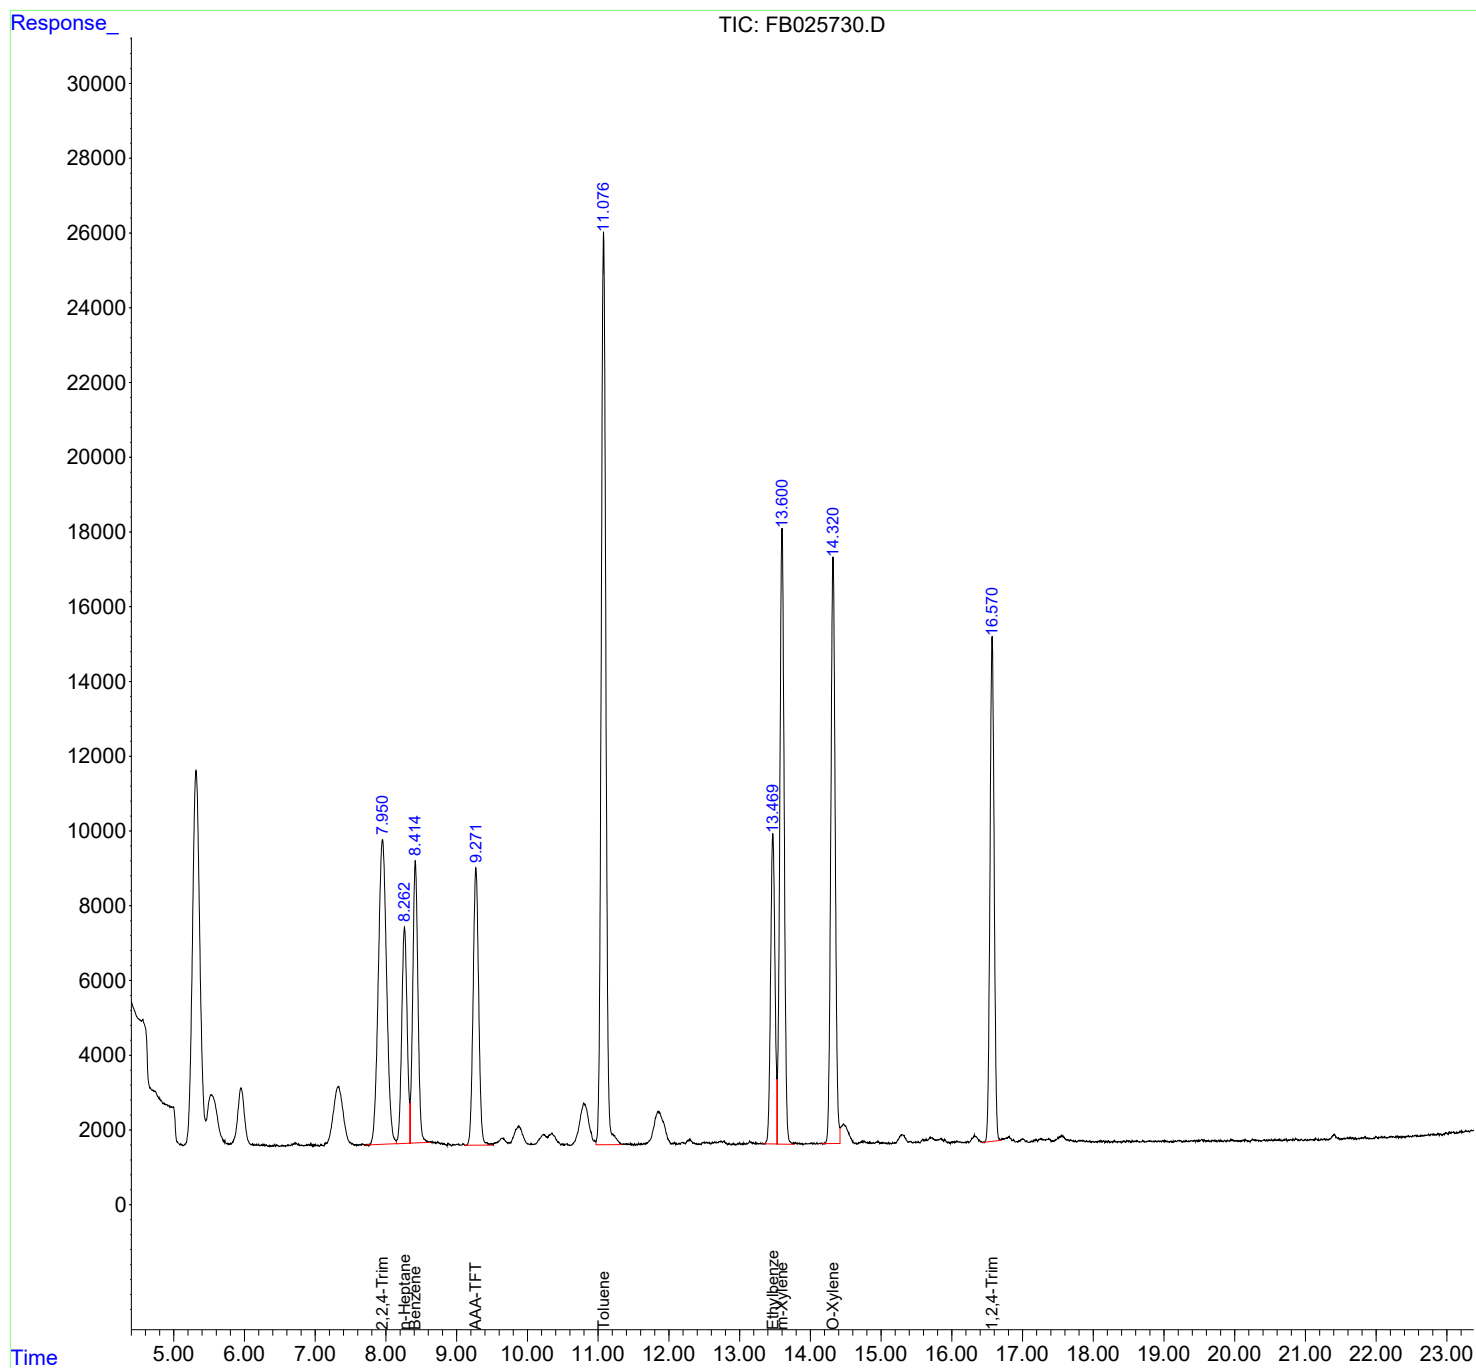

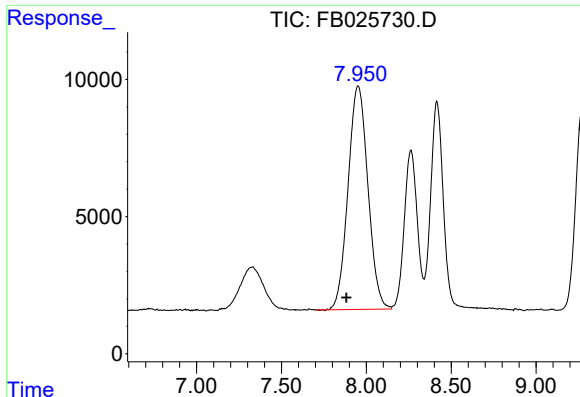


#2 2,2,4-Trimethylpentane

R.T.: 7.951 min
Delta R.T.: 0.068 min
Response: 662238
Conc: 30.77 ng/ml

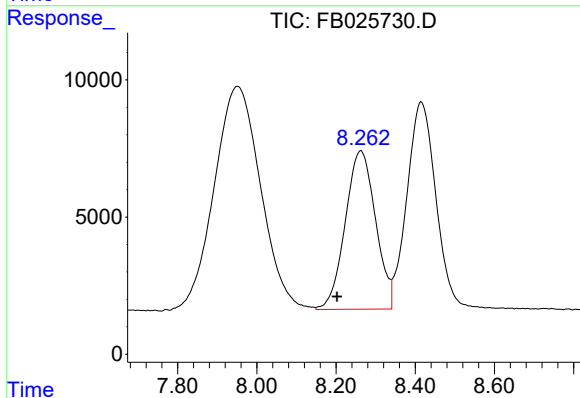


#3 n-Heptane

R.T.: 8.263 min
Delta R.T.: 0.060 min
Response: 306910
Conc: 10.15 ng/ml

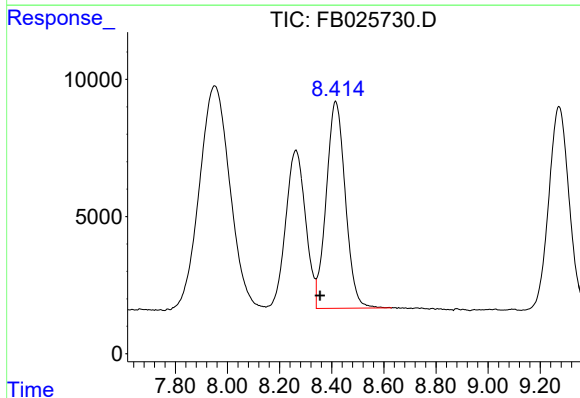


#4 Benzene

R.T.: 8.415 min
Delta R.T.: 0.061 min
Response: 384342
Conc: 10.05 ng/ml

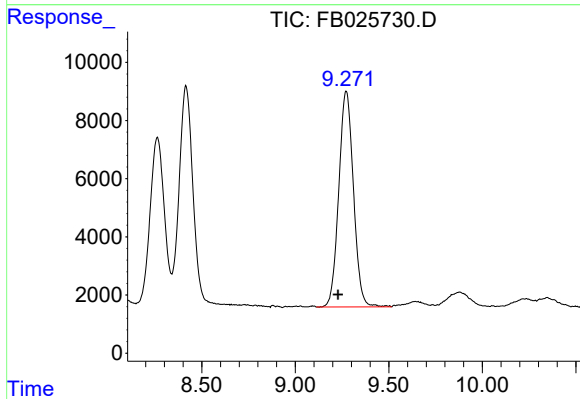


#5 AAA-TFT

R.T.: 9.272 min
Delta R.T.: 0.043 min
Response: 403895
Conc: 18.82 ng/ml

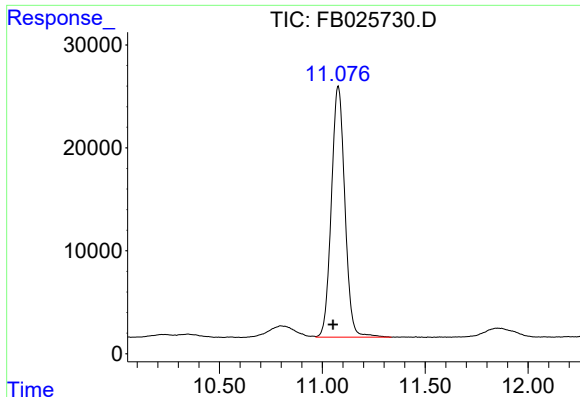


#6 Toluene

R.T.: 11.077 min
Delta R.T.: 0.026 min
Response: 1113173
Conc: 29.75 ng/ml

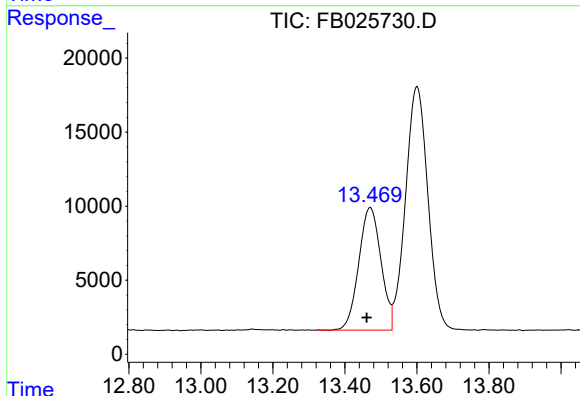


#7 Ethylbenzene

R.T.: 13.471 min
Delta R.T.: 0.010 min
Response: 354098
Conc: 9.78 ng/ml

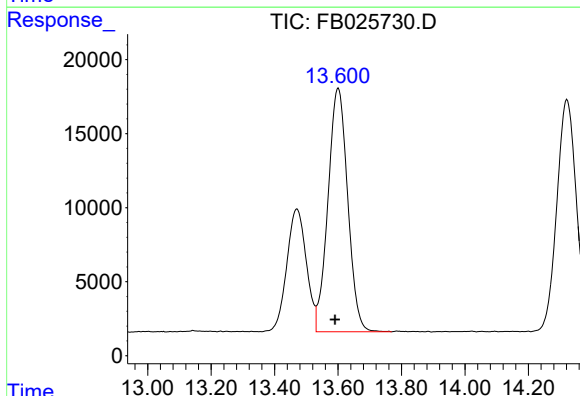


#8 m-Xylene

R.T.: 13.601 min
Delta R.T.: 0.010 min
Response: 710292
Conc: 19.53 ng/ml

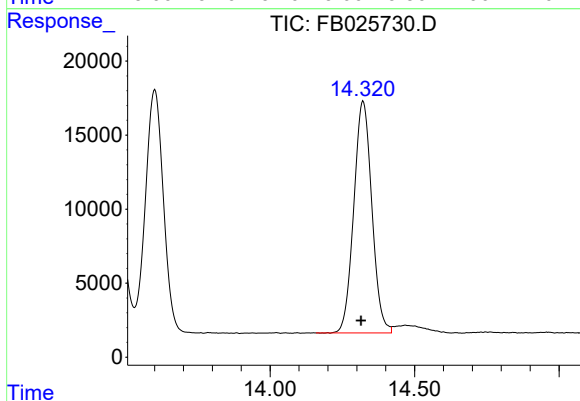

#9 O-Xylene

R.T.: 14.322 min
Delta R.T.: 0.007 min
Response: 681002
Conc: 19.73 ng/ml

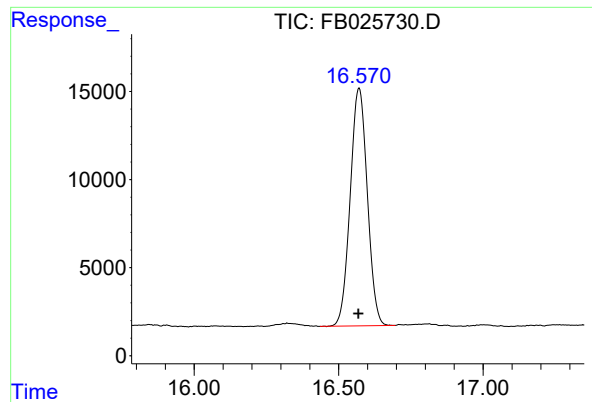

#10 1,2,4-Trimethylbenzene

R.T.: 16.571 min
Delta R.T.: 0.002 min
Response: 552963
Conc: 19.46 ng/ml