

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB050819\
 Data File : FB020985.D
 Signal(s) : FID2B.CH
 Acq On : 8 May 2019 11:13
 Operator : MJ/SJ
 Sample : K2643-01MSD
 Misc : 5.05g/5.00ml DI WATER
 ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: May 09 00:54:11 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB042919.M
 Quant Title :
 QLast Update : Mon Apr 29 15:53:58 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.994	393033	21.909 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.856	1010042	22.391 ng/ml
2) t	2,2,4-Trimethylpentane	7.610	892438	21.410 ng/ml
3) t	n-Heptane	7.950	269281	6.802 ng/ml
4) t	Benzene	8.086	366010	8.749 ng/ml
6) t	Toluene	10.838	700533	25.289 ng/ml
7) t	Ethylbenzene	13.288	224876	8.018 ng/ml
8) t	m-Xylene	13.422	467222	15.721 ng/ml
9) t	O-Xylene	14.152	501994	16.195 ng/ml
10) t	1,2,4-Trimethylbenzene	16.436	438661	14.144 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB050819\
Data File : FB020985.D
Signal(s) : FID2B.CH
Acq On : 8 May 2019 11:13
Operator : MJ/SJ
Sample : K2643-01MSD
Misc : 5.05g/5.00ml DI WATER
ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: May 09 00:54:11 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB042919.M
Quant Title :
QLast Update : Mon Apr 29 15:53:58 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

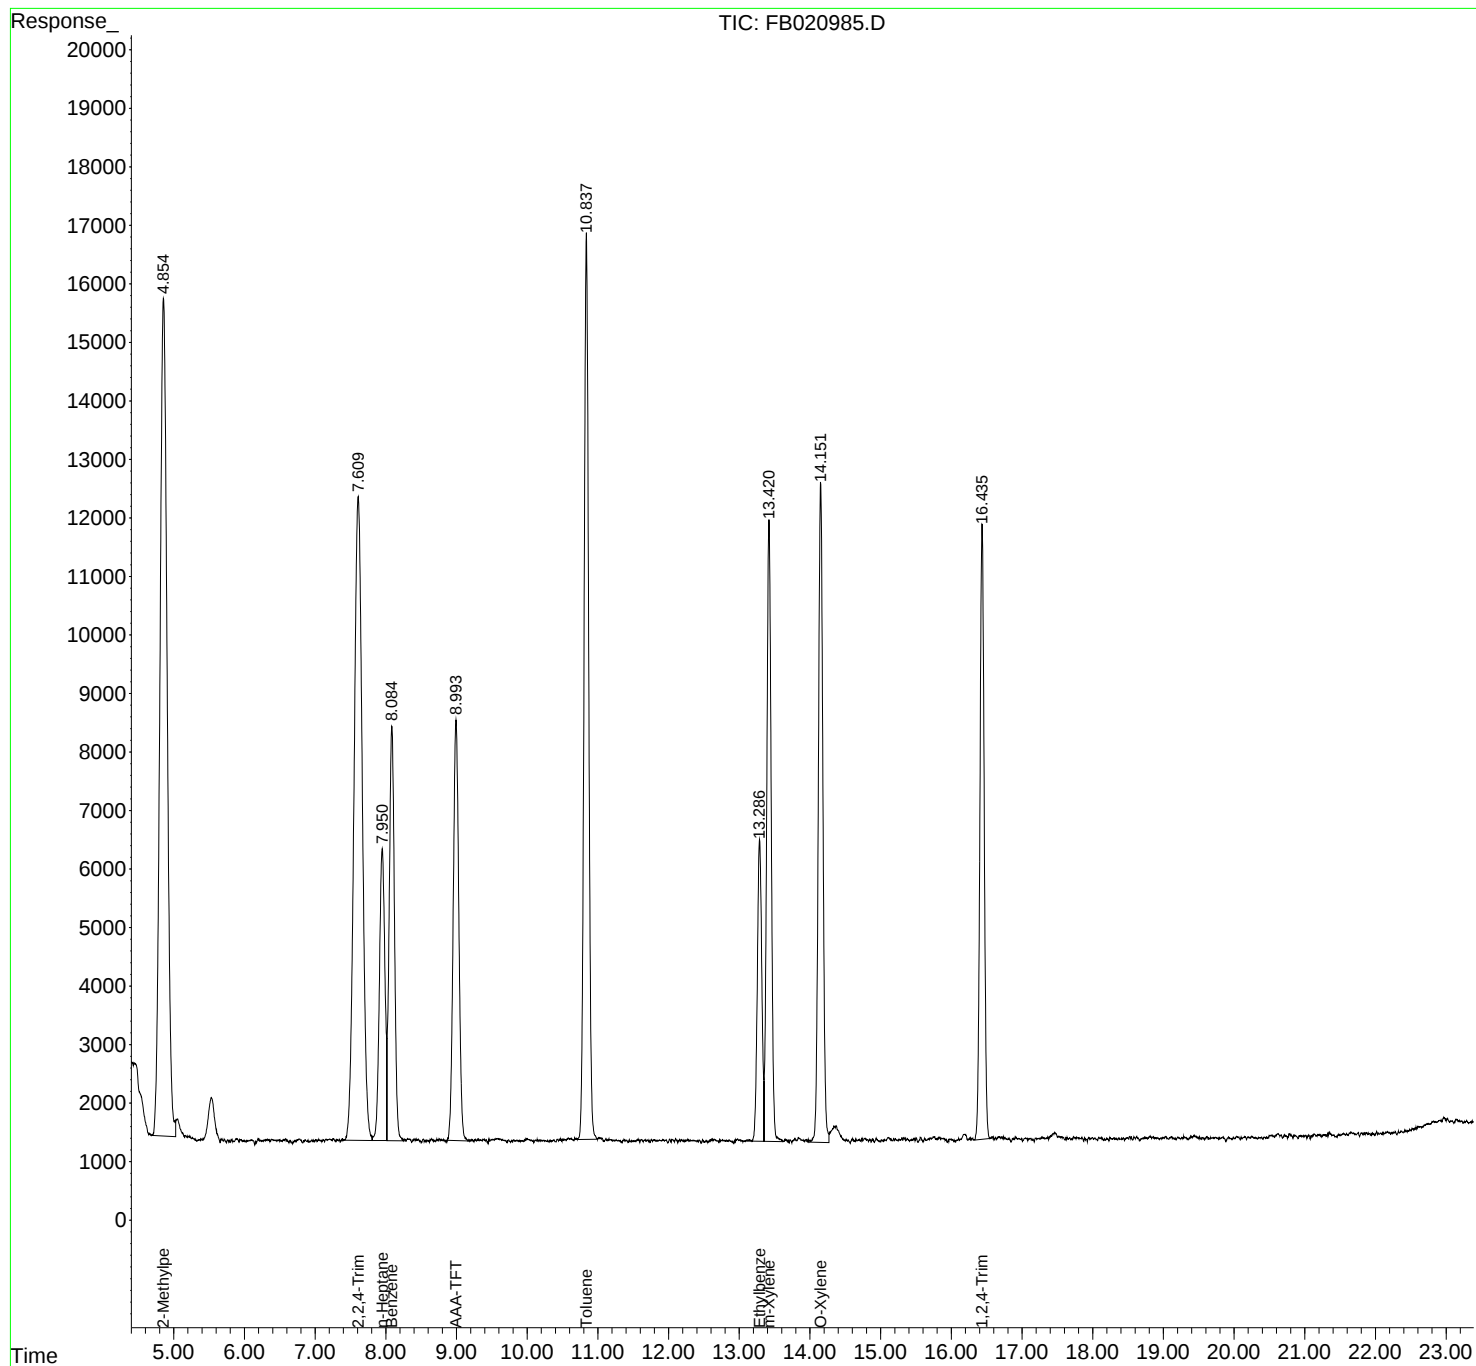

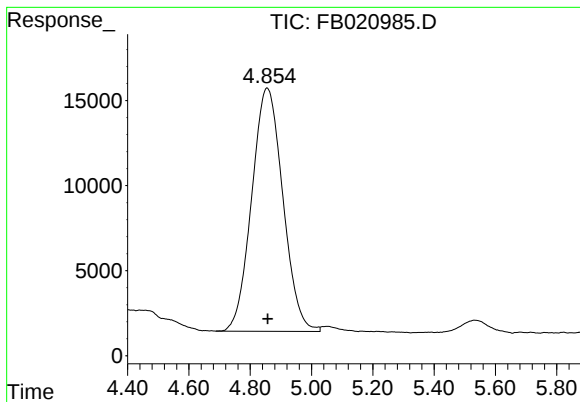


#1 2-Methylpentane

R.T.: 4.856 min
 Delta R.T.: -0.001 min
 Response: 1010042
 Conc: 22.39 ng/ml

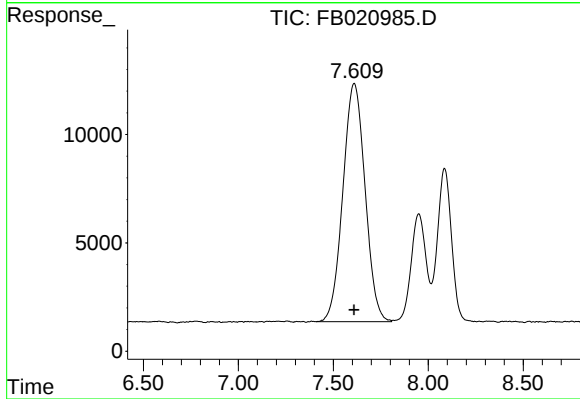


#2 2,2,4-Trimethylpentane

R.T.: 7.610 min
 Delta R.T.: 0.002 min
 Response: 892438
 Conc: 21.41 ng/ml

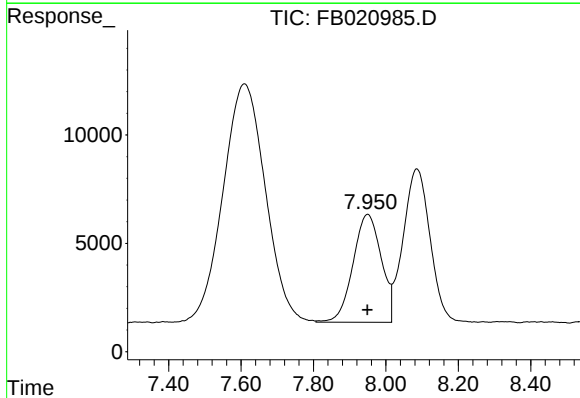


#3 n-Heptane

R.T.: 7.950 min
 Delta R.T.: 0.002 min
 Response: 269281
 Conc: 6.80 ng/ml

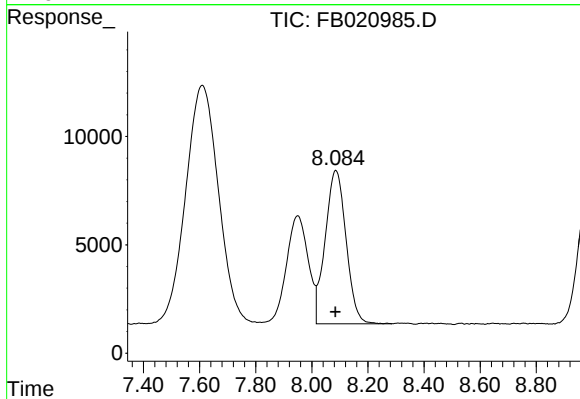


#4 Benzene

R.T.: 8.086 min
 Delta R.T.: 0.002 min
 Response: 366010
 Conc: 8.75 ng/ml

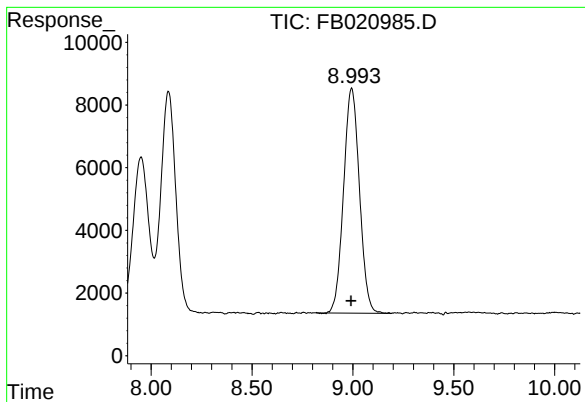


#5 AAA-TFT

R.T.: 8.994 min
Delta R.T.: 0.002 min
Response: 393033
Conc: 21.91 ng/ml

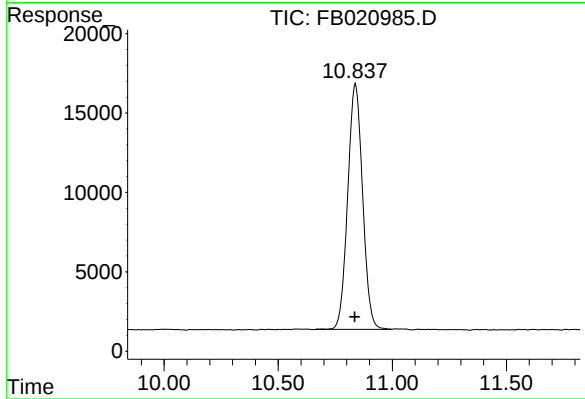


#6 Toluene

R.T.: 10.838 min
Delta R.T.: 0.002 min
Response: 700533
Conc: 25.29 ng/ml

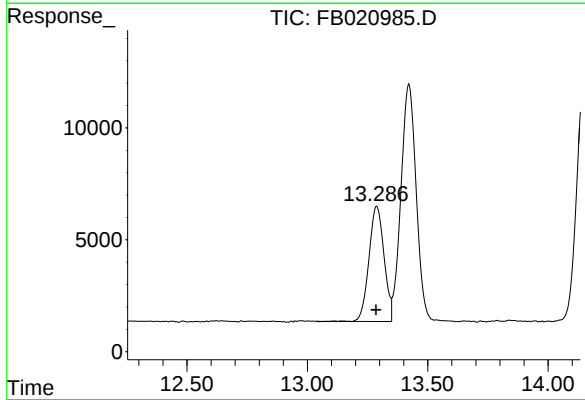


#7 Ethylbenzene

R.T.: 13.288 min
Delta R.T.: 0.002 min
Response: 224876
Conc: 8.02 ng/ml

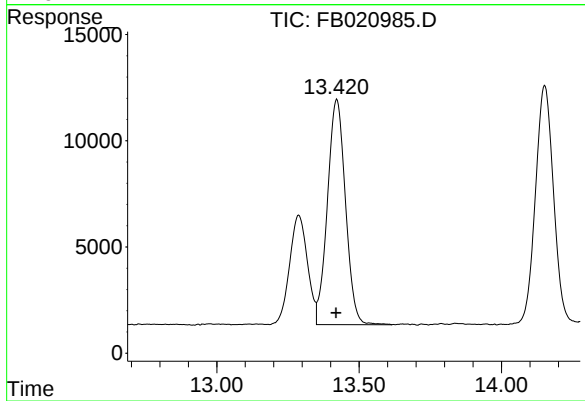


#8 m-Xylene

R.T.: 13.422 min
Delta R.T.: 0.003 min
Response: 467222
Conc: 15.72 ng/ml

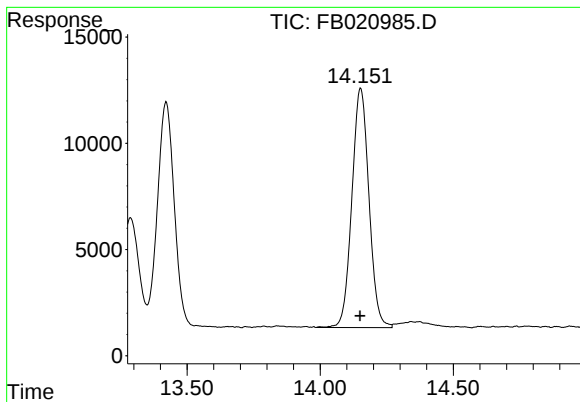

#9 O-Xylene

R.T.: 14.152 min
Delta R.T.: 0.003 min
Response: 501994
Conc: 16.20 ng/ml

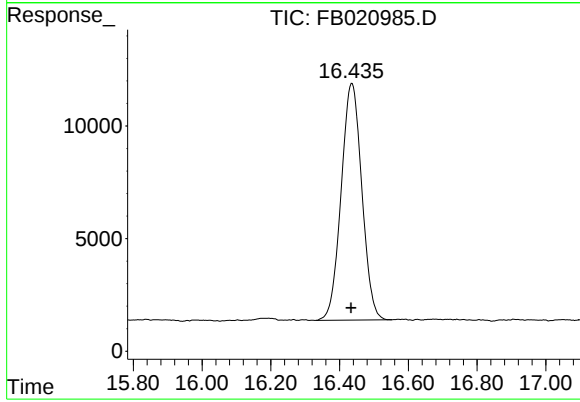

#10 1,2,4-Trimethylbenzene

R.T.: 16.436 min
Delta R.T.: 0.003 min
Response: 438661
Conc: 14.14 ng/ml