

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB050820\
 Data File : FB024294.D
 Signal(s) : FID2B.CH
 Acq On : 8 May 2020 17:15
 Operator : DD/AJ
 Sample : L2506-02
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: May 09 01:03:46 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040820.M
 Quant Title :
 QLast Update : Wed Apr 08 10:11:26 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.801	454846	18.155 ng/ml
Target Compounds			
6) t Toluene	10.640	2670	0.068 ng/ml
7) t Ethylbenzene	13.065	6489	0.178 ng/ml
8) t m-Xylene	13.207	11878	0.339 ng/ml
9) t O-Xylene	13.935	10183	0.299 ng/ml
10) t 1,2,4-Trimethylbenzene	16.215	16488	0.581 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB050820\
Data File : FB024294.D
Signal(s) : FID2B.CH
Acq On : 8 May 2020 17:15
Operator : DD/AJ
Sample : L2506-02
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: May 09 01:03:46 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040820.M
Quant Title :
QLast Update : Wed Apr 08 10:11:26 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

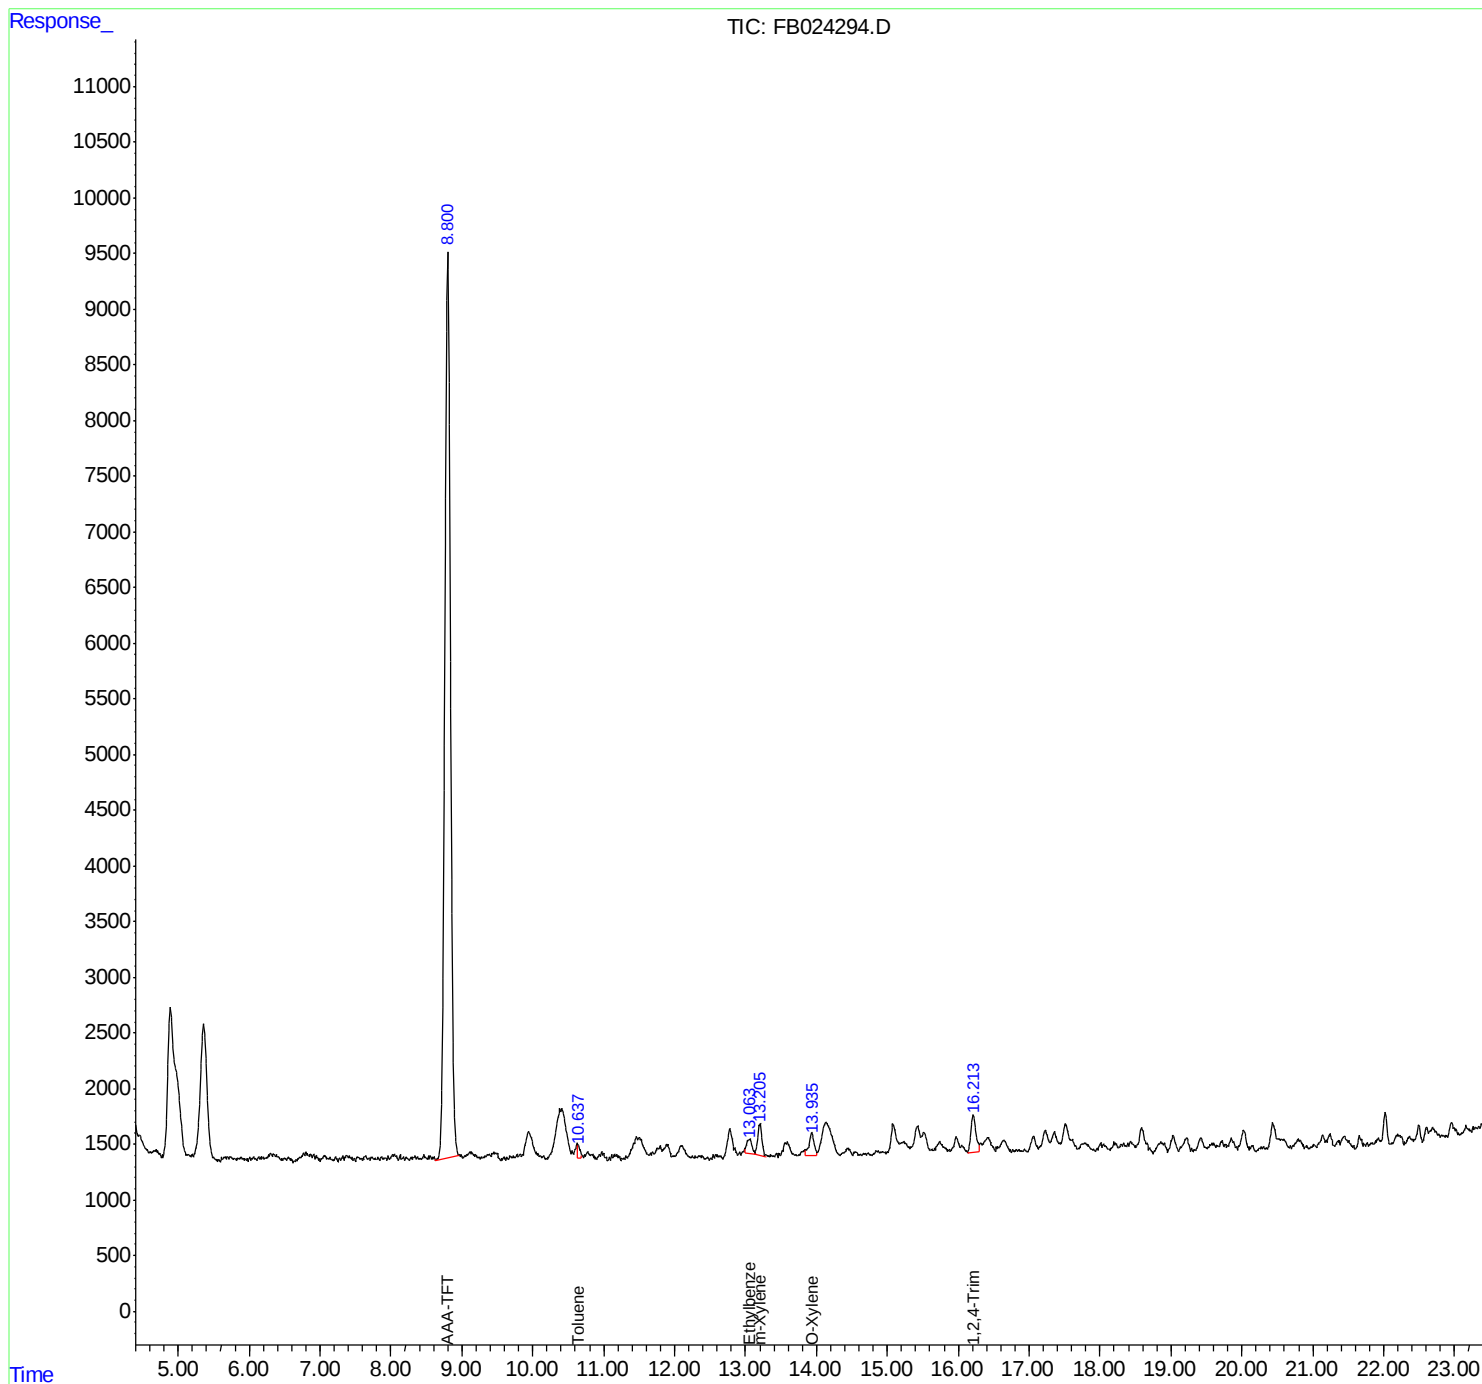


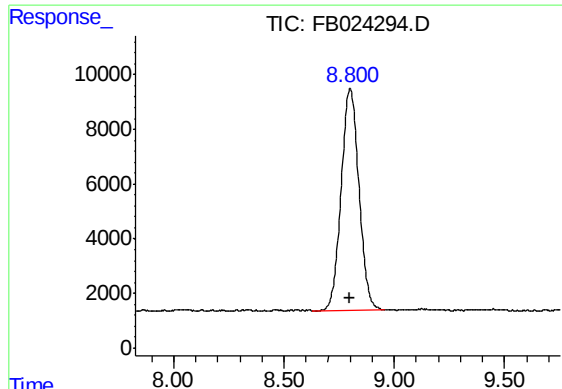

#5 AAA-TFT


R.T.: 8.801 min
Delta R.T.: 0.000 min
Response: 454846
Conc: 18.15 ng/ml

Instrument :
FID_B
ClientSampleId :

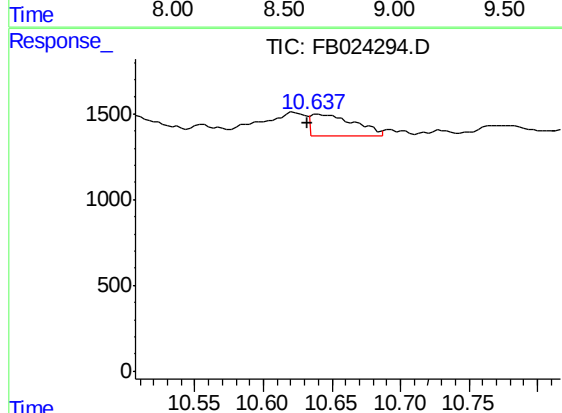


#6 Toluene

R.T.: 10.640 min
Delta R.T.: 0.008 min
Response: 2670
Conc: 0.07 ng/ml

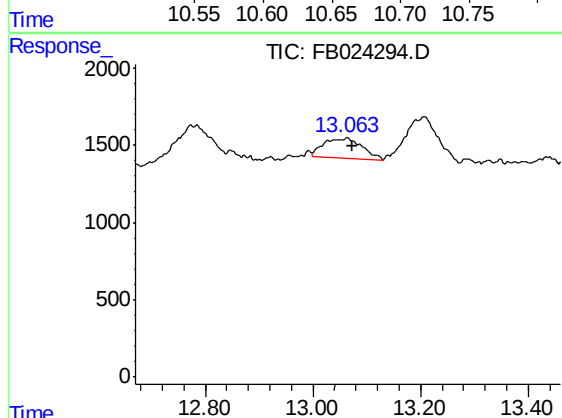


#7 Ethylbenzene

R.T.: 13.065 min
Delta R.T.: -0.008 min
Response: 6489
Conc: 0.18 ng/ml

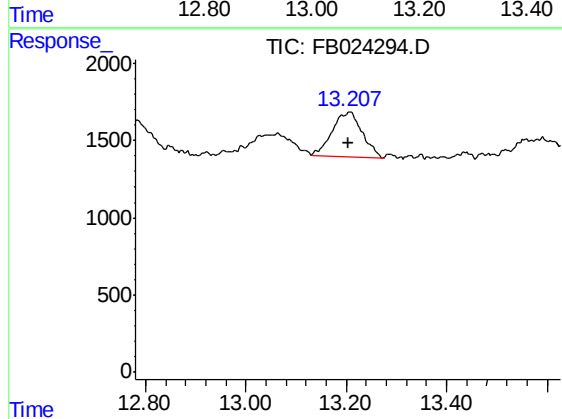

#8 m-Xylene


R.T.: 13.207 min
Delta R.T.: 0.002 min
Response: 11878
Conc: 0.34 ng/ml

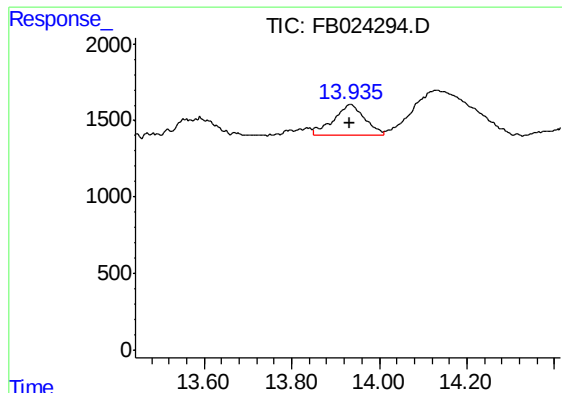

#9 O-Xylene

R.T.: 13.935 min
Delta R.T.: 0.002 min
Response: 10183
Conc: 0.30 ng/ml

Instrument :
FID_B
ClientSampleId :

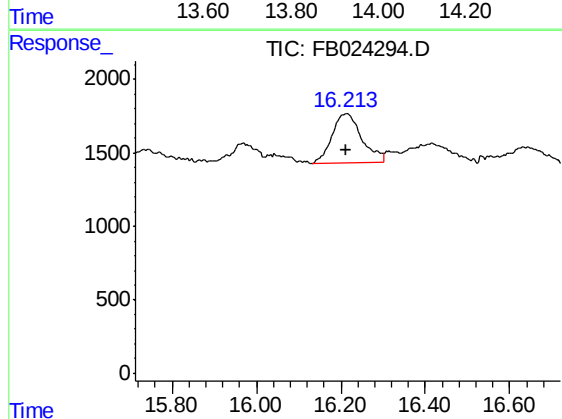

#10 1,2,4-Trimethylbenzene

R.T.: 16.215 min
Delta R.T.: 0.003 min
Response: 16488
Conc: 0.58 ng/ml