

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB050820\
Data File : FB024298.D
Signal(s) : FID2B.CH
Acq On : 8 May 2020 19:18
Operator : DD/AJ
Sample : L2557-03
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: May 09 01:04:23 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040820.M
Quant Title :
QLast Update : Wed Apr 08 10:11:26 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.801	448186	17.889 ng/ml
Target Compounds			
4) t Benzene	7.889	9605	0.238 ng/ml
6) t Toluene	10.615	172	0.004 ng/ml
7) t Ethylbenzene	13.078	1257	0.034 ng/ml
8) t m-Xylene	13.198	8371	0.239 ng/ml
9) t O-Xylene	13.927	2735	0.080 ng/ml
10) t 1,2,4-Trimethylbenzene	16.218	573	0.020 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB050820\
Data File : FB024298.D
Signal(s) : FID2B.CH
Acq On : 8 May 2020 19:18
Operator : DD/AJ
Sample : L2557-03
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: May 09 01:04:23 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040820.M
Quant Title :
QLast Update : Wed Apr 08 10:11:26 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

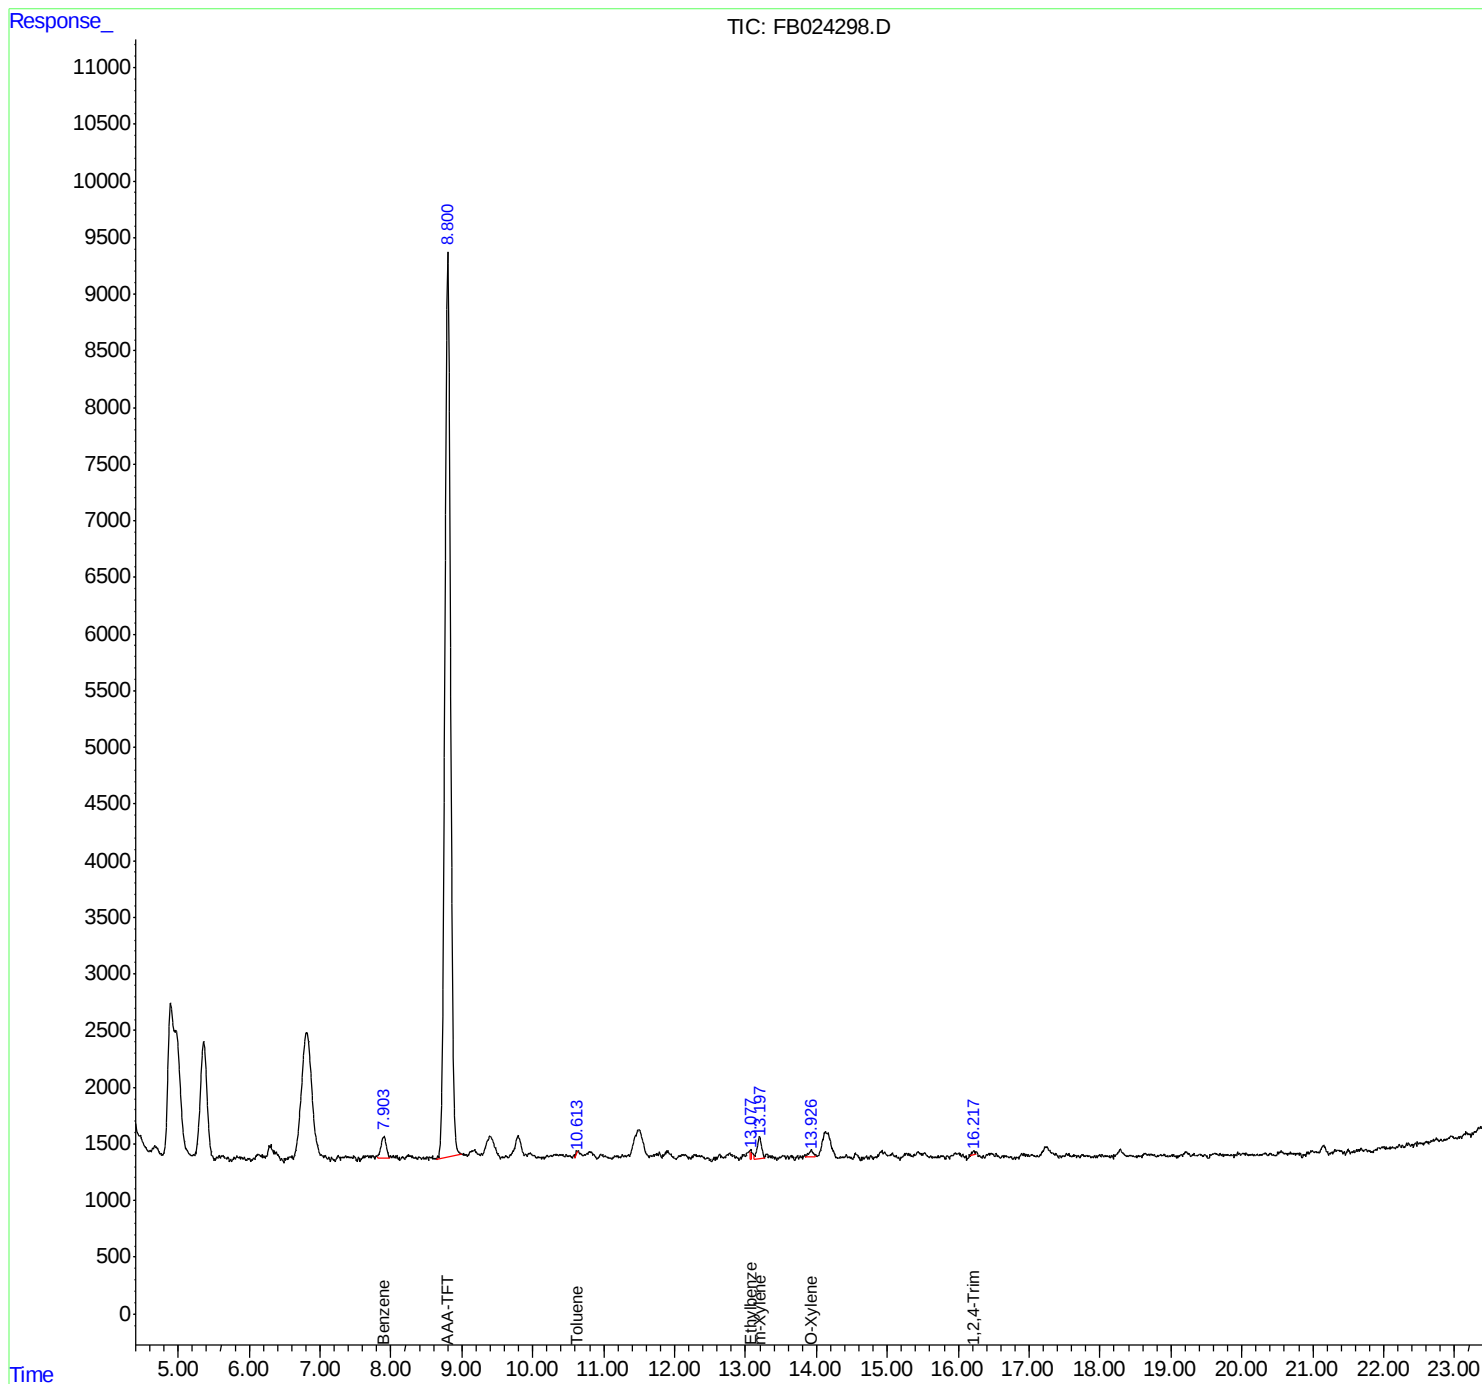


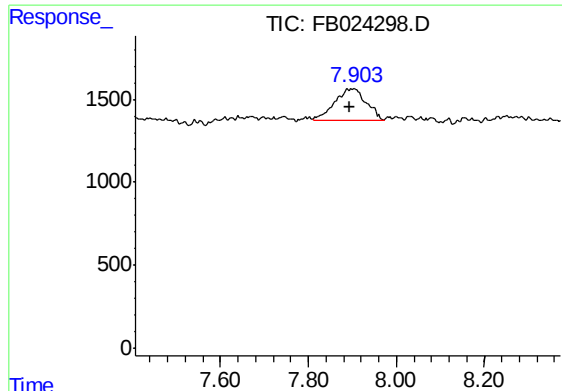

#4 Benzene


R.T.: 7.889 min
Delta R.T.: -0.005 min
Response: 9605
Conc: 0.24 ng/ml

Instrument :
FID_B
ClientSampleId :

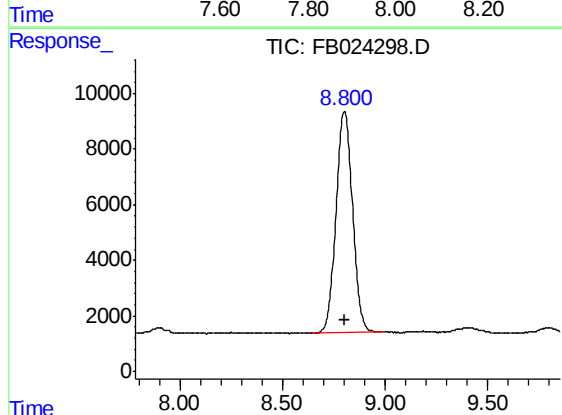


#5 AAA-TFT

R.T.: 8.801 min
Delta R.T.: 0.000 min
Response: 448186
Conc: 17.89 ng/ml

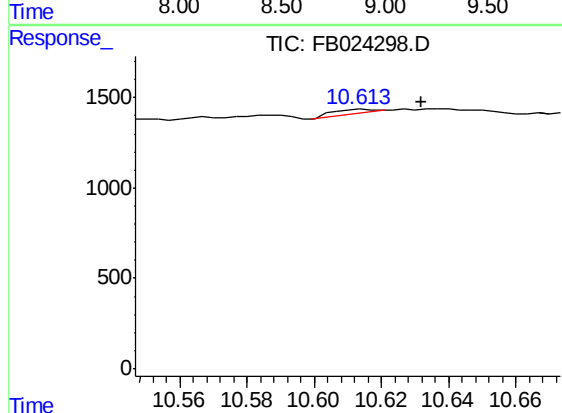


#6 Toluene

R.T.: 10.615 min
Delta R.T.: -0.017 min
Response: 172
Conc: 0.00 ng/ml

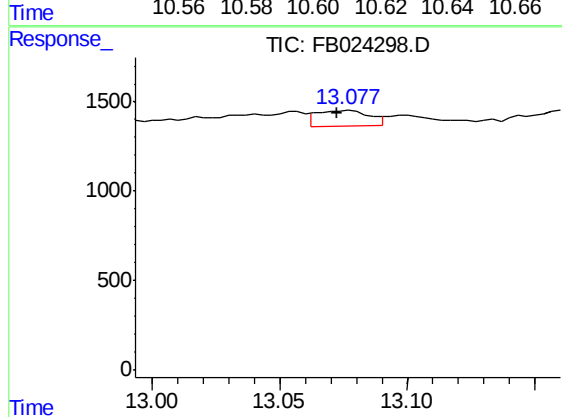

#7 Ethylbenzene


R.T.: 13.078 min
Delta R.T.: 0.006 min
Response: 1257
Conc: 0.03 ng/ml

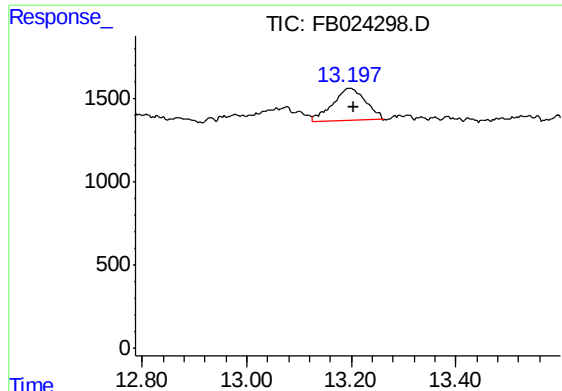

#8 m-Xylene


R.T.: 13.198 min
Delta R.T.: -0.007 min
Response: 8371
Conc: 0.24 ng/ml

Instrument :
FID_B
ClientSampleId :

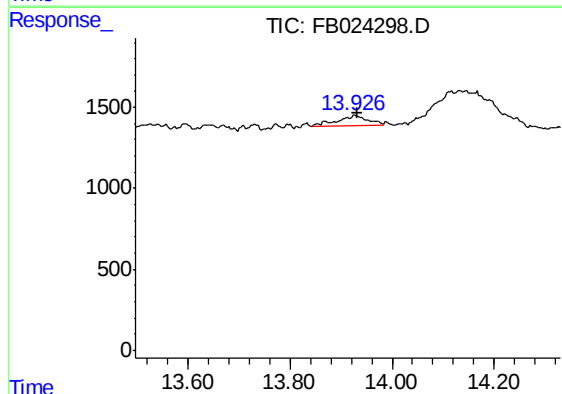

#9 o-Xylene

R.T.: 13.927 min
Delta R.T.: -0.006 min
Response: 2735
Conc: 0.08 ng/ml

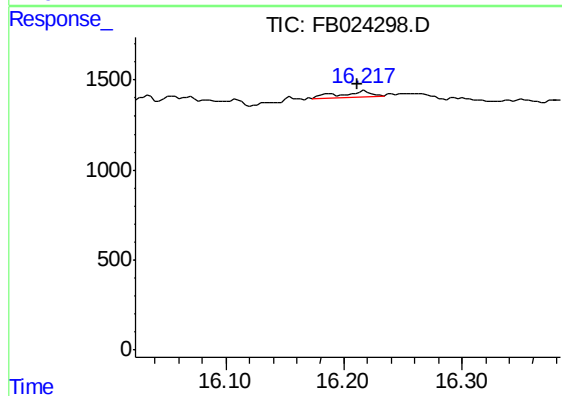

#10 1,2,4-Trimethylbenzene

R.T.: 16.218 min
Delta R.T.: 0.007 min
Response: 573
Conc: 0.02 ng/ml