

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB050820\
Data File : FB024299.D
Signal(s) : FID2B.CH
Acq On : 8 May 2020 19:48
Operator : DD/AJ
Sample : L2557-06
Misc : 5.08g/5.00ml DI WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: May 09 01:04:33 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040820.M
Quant Title :
QLast Update : Wed Apr 08 10:11:26 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.800	558093	22.276 ng/ml
Target Compounds			
7) t Ethylbenzene	13.049	617	0.017 ng/ml
8) t m-Xylene	13.209	1770	0.051 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB050820\
Data File : FB024299.D
Signal(s) : FID2B.CH
Acq On : 8 May 2020 19:48
Operator : DD/AJ
Sample : L2557-06
Misc : 5.08g/5.00ml DI WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: May 09 01:04:33 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040820.M
Quant Title :
QLast Update : Wed Apr 08 10:11:26 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

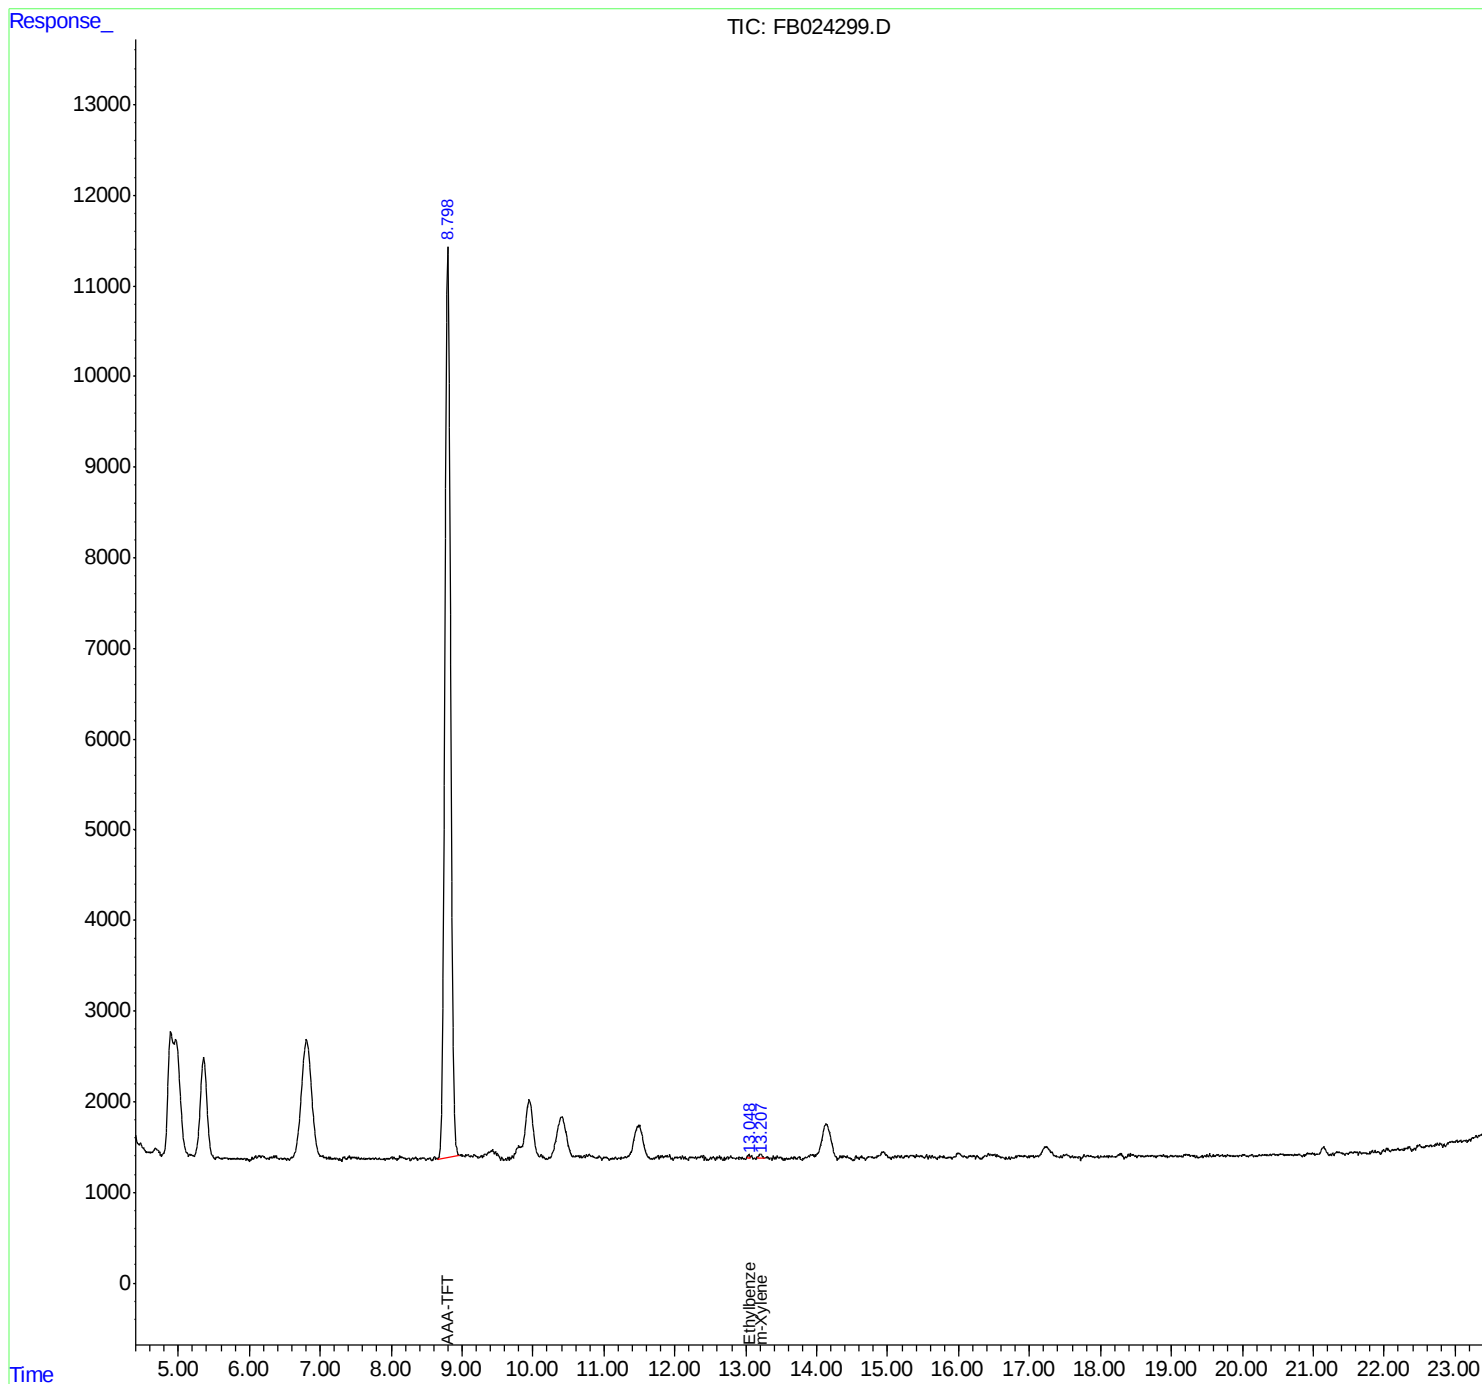


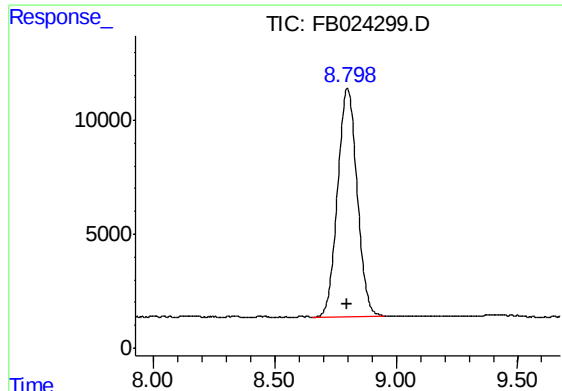

#5 AAA-TFT


R.T.: 8.800 min
Delta R.T.: 0.000 min
Response: 558093
Conc: 22.28 ng/ml

Instrument :
FID_B
ClientSampleId :

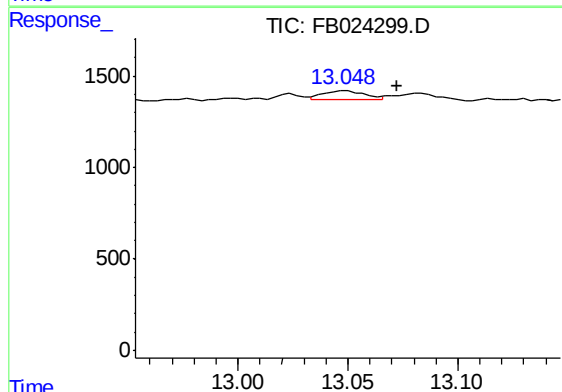

#7 Ethylbenzene

R.T.: 13.049 min
Delta R.T.: -0.023 min
Response: 617
Conc: 0.02 ng/ml

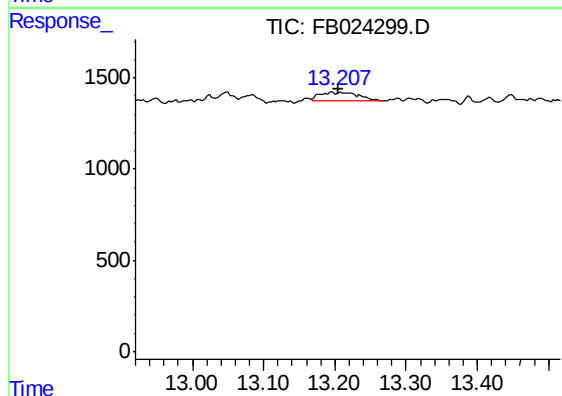

#8 m-Xylene

R.T.: 13.209 min
Delta R.T.: 0.003 min
Response: 1770
Conc: 0.05 ng/ml