

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB050820\
 Data File : FB024279.D
 Signal(s) : FID2B.CH
 Acq On : 8 May 2020 8:54
 Operator : DD/AJ
 Sample : BSF0508S1
 Misc : 5.00g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: May 09 01:01:31 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040820.M
 Quant Title :
 QLast Update : Wed Apr 08 10:11:26 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.797	526848	21.029 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.688	1005638	30.808 ng/ml
2) t 2,2,4-Trimethylpentane	7.416	1087702	31.872 ng/ml
3) t n-Heptane	7.755	360503	10.681 ng/ml
4) t Benzene	7.890	430169	10.658 ng/ml
6) t Toluene	10.628	1219701	31.027 ng/ml
7) t Ethylbenzene	13.069	376448	10.326 ng/ml
8) t m-Xylene	13.202	734631	20.986 ng/ml
9) t O-Xylene	13.930	713686	20.940 ng/ml
10) t 1,2,4-Trimethylbenzene	16.209	601888	21.198 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB050820\
Data File : FB024279.D
Signal(s) : FID2B.CH
Acq On : 8 May 2020 8:54
Operator : DD/AJ
Sample : BSF0508S1
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: May 09 01:01:31 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040820.M
Quant Title :
QLast Update : Wed Apr 08 10:11:26 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

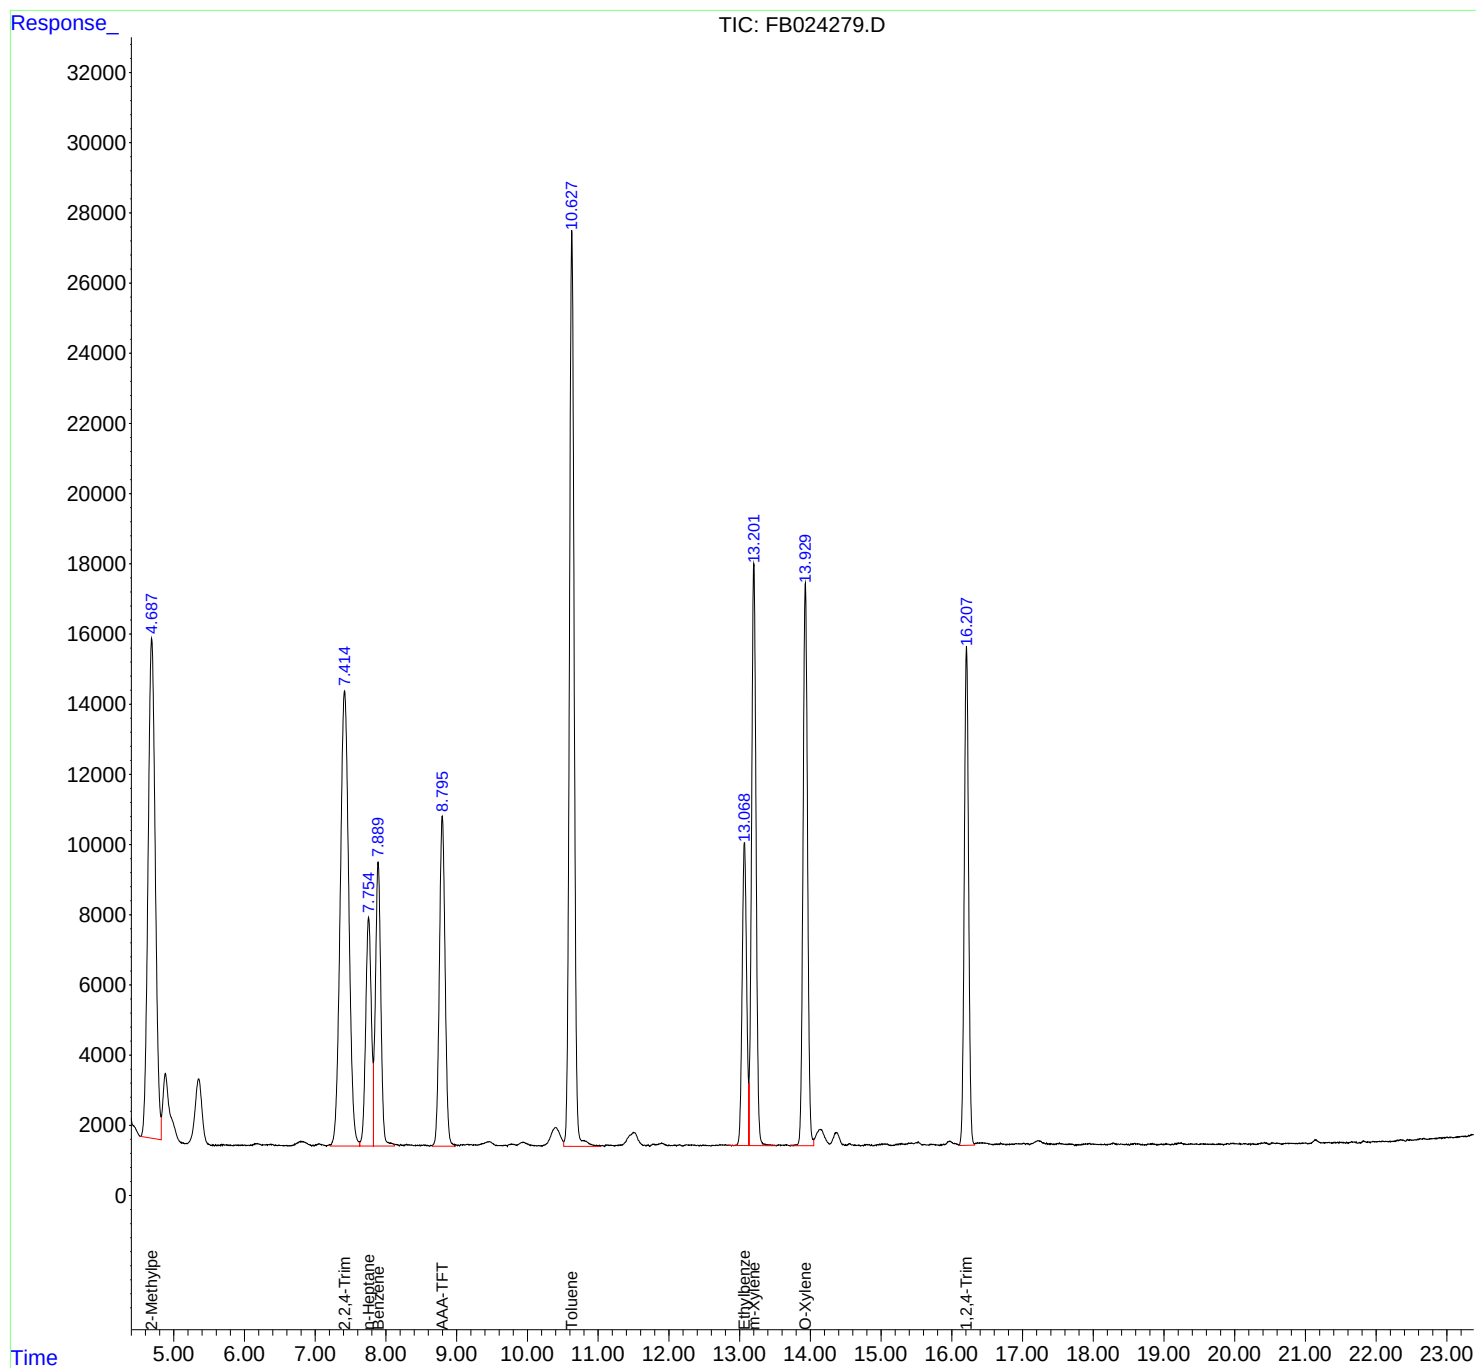


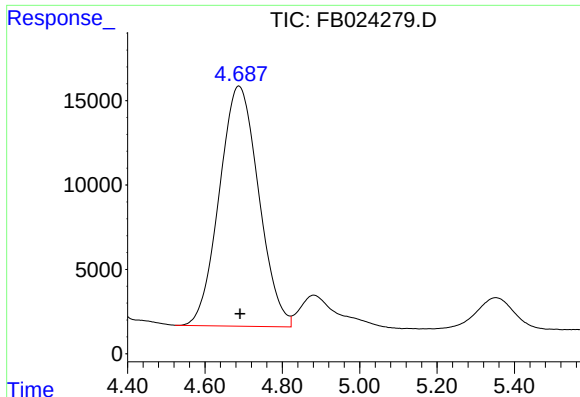

#1 2-Methylpentane


R.T.: 4.688 min
Delta R.T.: -0.003 min
Response: 1005638
Conc: 30.81 ng/ml

Instrument :
FID_B
ClientSampleId :

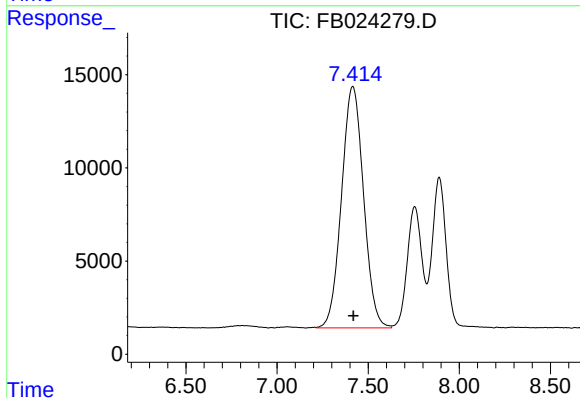


#2 2,2,4-Trimethylpentane

R.T.: 7.416 min
Delta R.T.: -0.004 min
Response: 1087702
Conc: 31.87 ng/ml

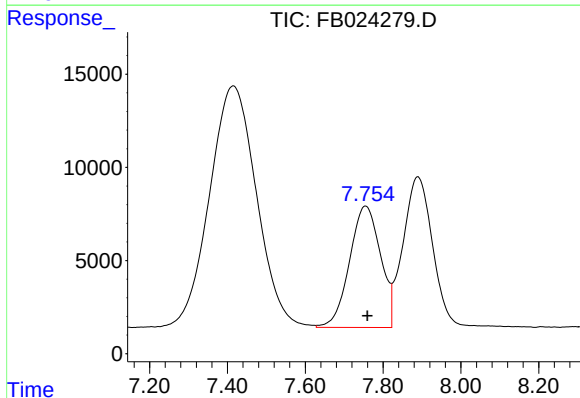


#3 n-Heptane

R.T.: 7.755 min
Delta R.T.: -0.004 min
Response: 360503
Conc: 10.68 ng/ml

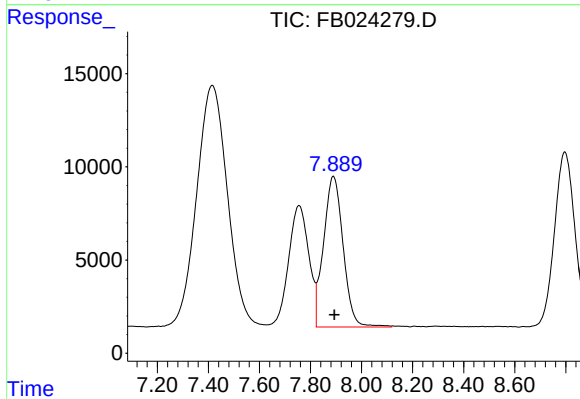

#4 Benzene


R.T.: 7.890 min
Delta R.T.: -0.004 min
Response: 430169
Conc: 10.66 ng/ml

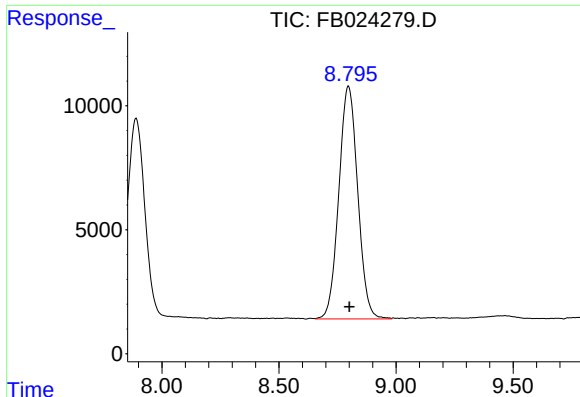

#5 AAA-TFT


R.T.: 8.797 min
Delta R.T.: -0.004 min
Response: 526848
Conc: 21.03 ng/ml

Instrument :
FID_B
ClientSampleId :

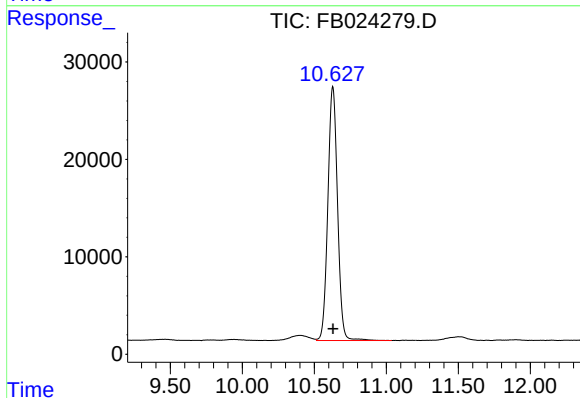


#6 Toluene

R.T.: 10.628 min
Delta R.T.: -0.004 min
Response: 1219701
Conc: 31.03 ng/ml

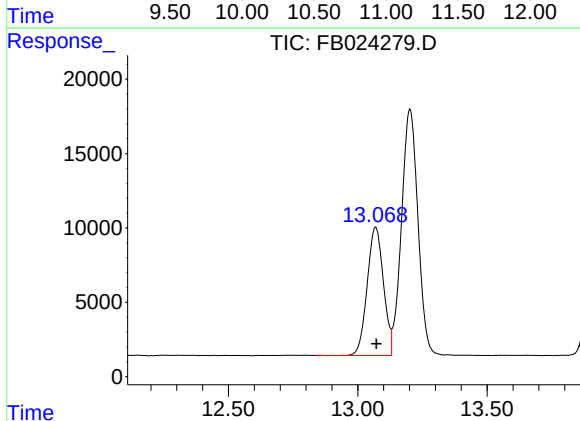


#7 Ethylbenzene

R.T.: 13.069 min
Delta R.T.: -0.003 min
Response: 376448
Conc: 10.33 ng/ml

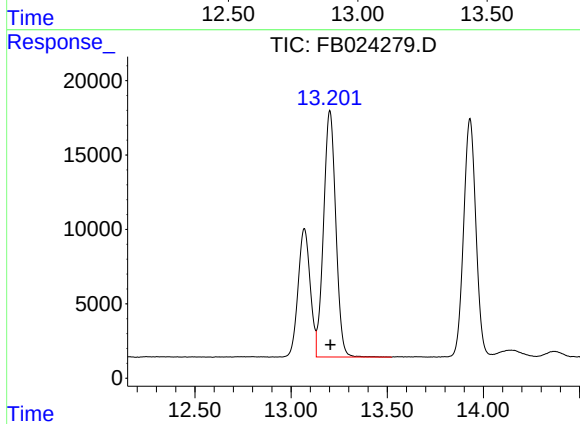

#8 m-Xylene


R.T.: 13.202 min
Delta R.T.: -0.003 min
Response: 734631
Conc: 20.99 ng/ml

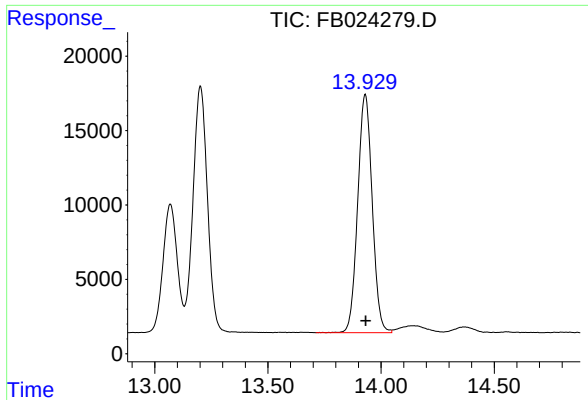

#9 O-Xylene

R.T.: 13.930 min
Delta R.T.: -0.003 min
Response: 713686
Conc: 20.94 ng/ml

Instrument :
FID_B
ClientSampleId :

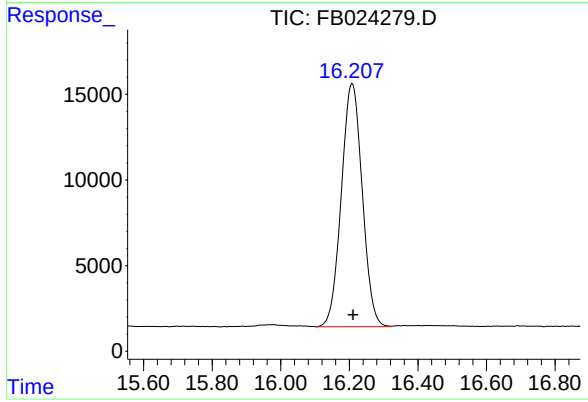

#10 1,2,4-Trimethylbenzene

R.T.: 16.209 min
Delta R.T.: -0.003 min
Response: 601888
Conc: 21.20 ng/ml