

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB050820\
 Data File : FB024300.D
 Signal(s) : FID2B.CH
 Acq On : 8 May 2020 20:19
 Operator : DD/AJ
 Sample : L2557-06MS
 Misc : 5.03g/5.00ml DI WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: May 09 01:04:41 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040820.M
 Quant Title :
 QLast Update : Wed Apr 08 10:11:26 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.800	507474	20.256 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.691	1004502	30.773 ng/ml
2) t 2,2,4-Trimethylpentane	7.419	1088343	31.891 ng/ml
3) t n-Heptane	7.758	353258	10.467 ng/ml
4) t Benzene	7.894	425753	10.549 ng/ml
6) t Toluene	10.632	1188300	30.228 ng/ml
7) t Ethylbenzene	13.072	370481	10.163 ng/ml
8) t m-Xylene	13.205	721090	20.599 ng/ml
9) t O-Xylene	13.933	703737	20.648 ng/ml
10) t 1,2,4-Trimethylbenzene	16.211	572918	20.178 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB050820\
Data File : FB024300.D
Signal(s) : FID2B.CH
Acq On : 8 May 2020 20:19
Operator : DD/AJ
Sample : L2557-06MS
Misc : 5.03g/5.00ml DI WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: May 09 01:04:41 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040820.M
Quant Title :
QLast Update : Wed Apr 08 10:11:26 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

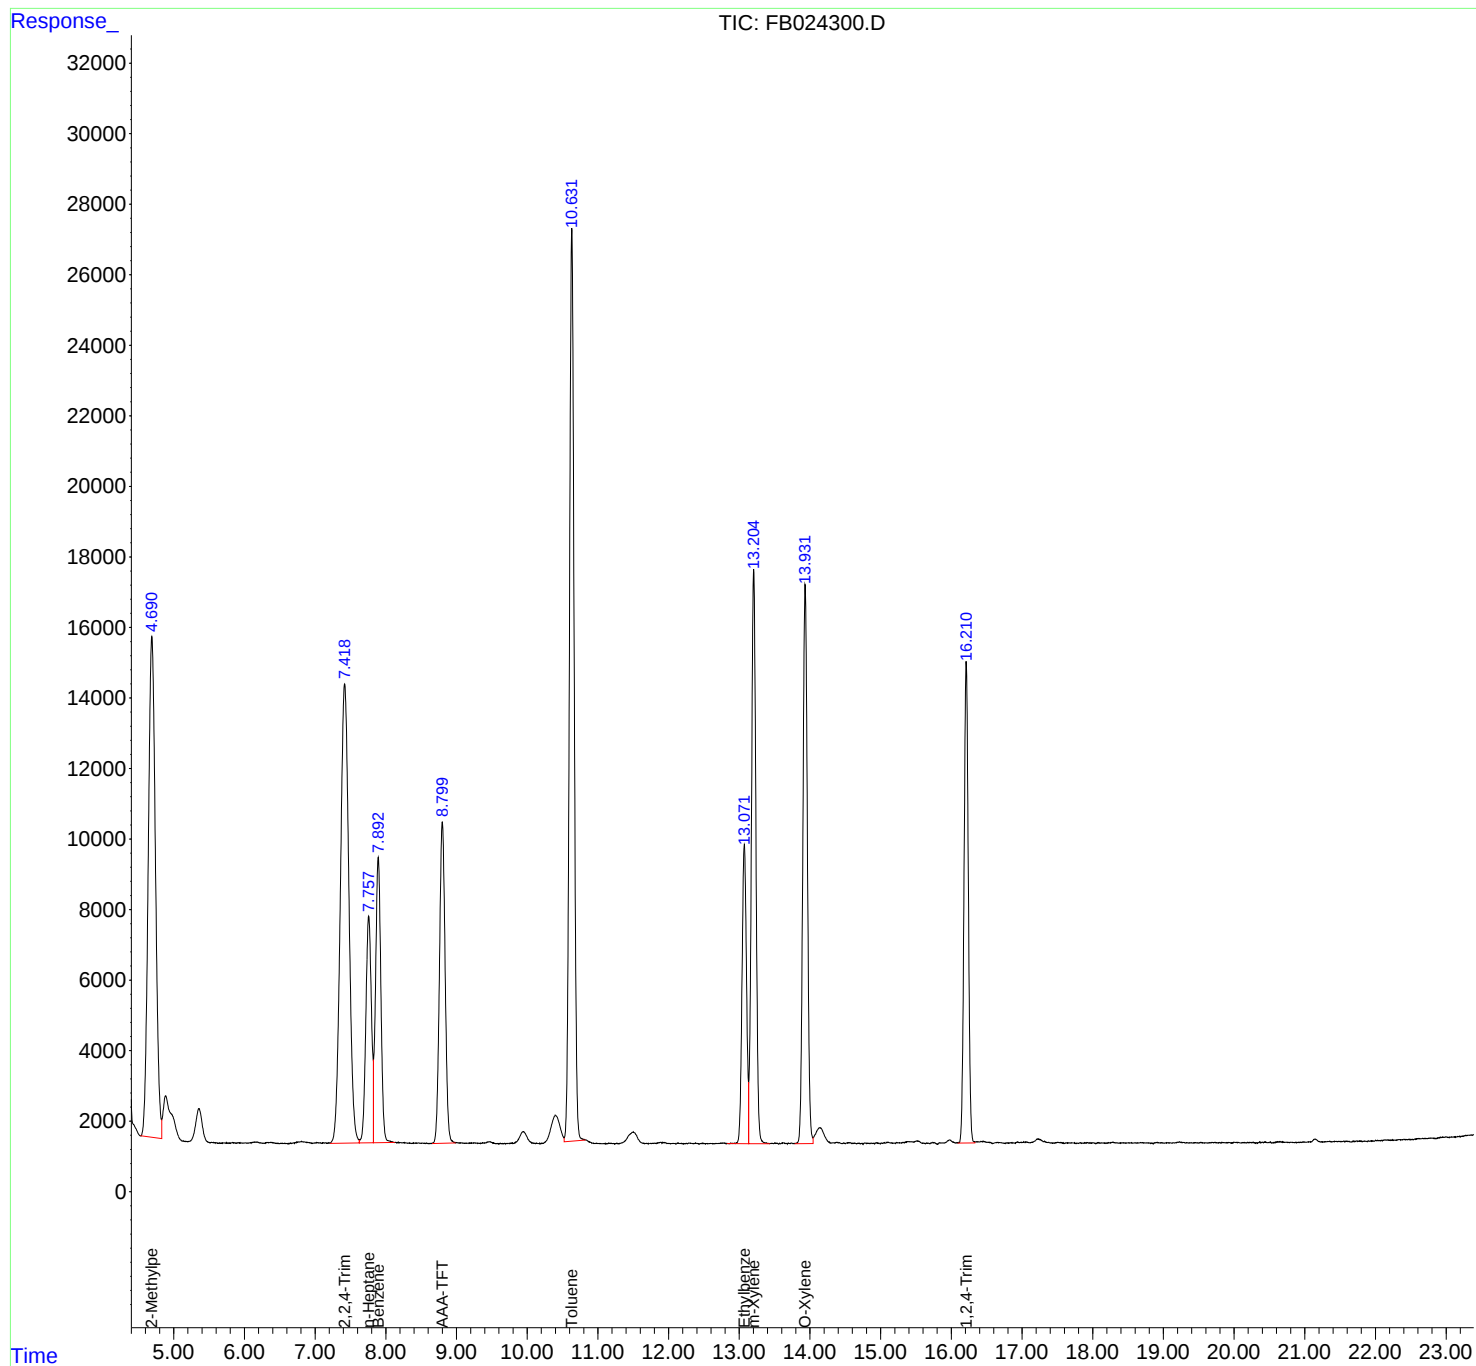


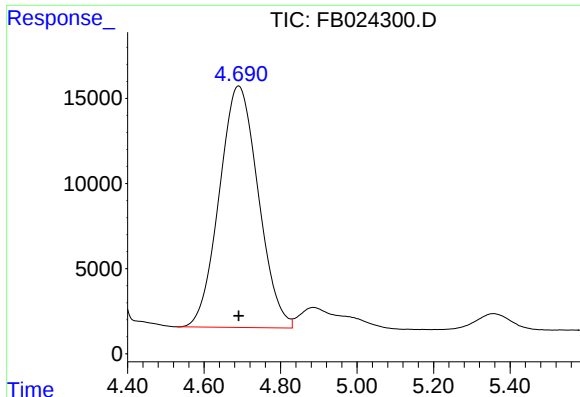

#1 2-Methylpentane


R.T.: 4.691 min
Delta R.T.: 0.000 min
Response: 1004502
Conc: 30.77 ng/ml

Instrument :
FID_B
ClientSampleId :

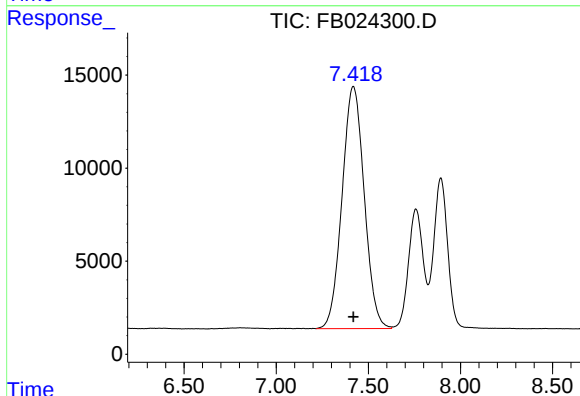


#2 2,2,4-Trimethylpentane

R.T.: 7.419 min
Delta R.T.: 0.000 min
Response: 1088343
Conc: 31.89 ng/ml

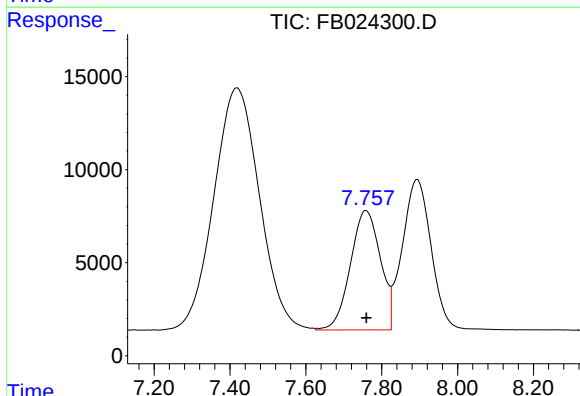


#3 n-Heptane

R.T.: 7.758 min
Delta R.T.: -0.001 min
Response: 353258
Conc: 10.47 ng/ml

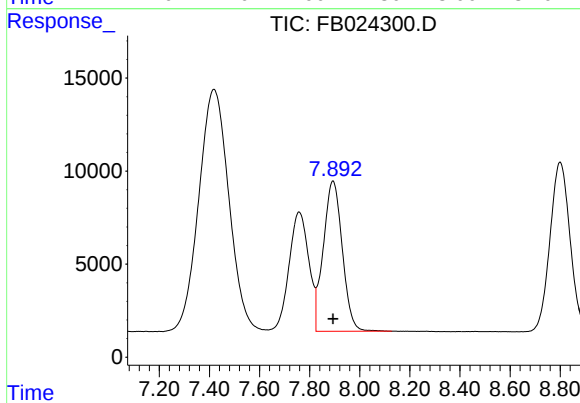

#4 Benzene


R.T.: 7.894 min
Delta R.T.: 0.000 min
Response: 425753
Conc: 10.55 ng/ml

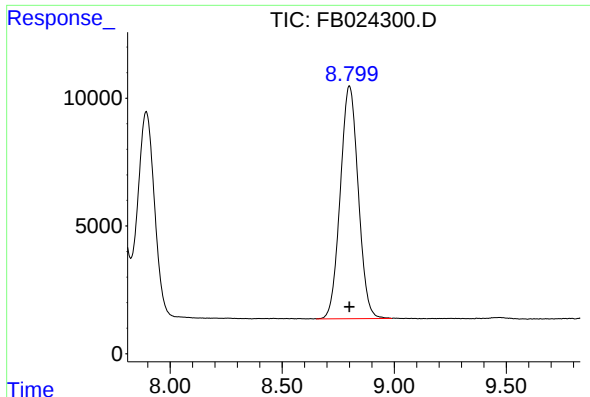

#5 AAA-TFT


R.T.: 8.800 min
Delta R.T.: 0.000 min
Response: 507474
Conc: 20.26 ng/ml

Instrument :
FID_B
ClientSampleId :

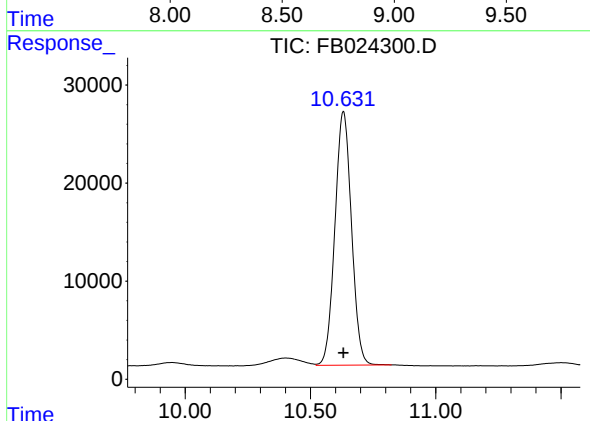


#6 Toluene

R.T.: 10.632 min
Delta R.T.: 0.000 min
Response: 1188300
Conc: 30.23 ng/ml

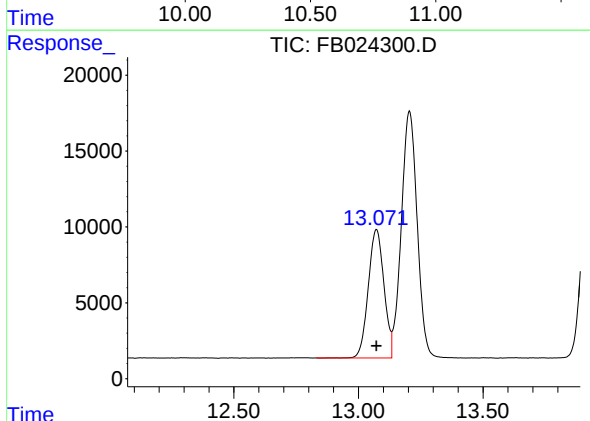


#7 Ethylbenzene

R.T.: 13.072 min
Delta R.T.: 0.000 min
Response: 370481
Conc: 10.16 ng/ml

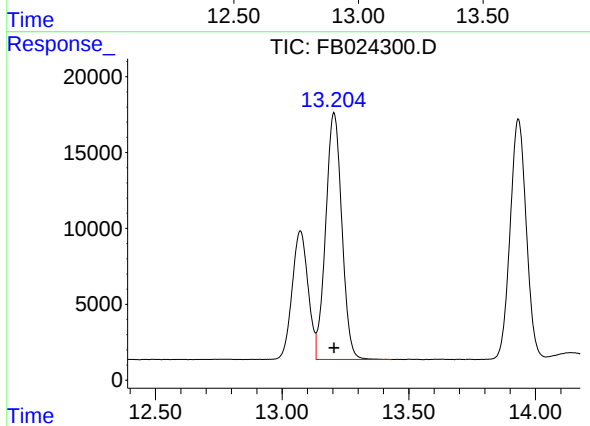

#8 m-Xylene


R.T.: 13.205 min
Delta R.T.: 0.000 min
Response: 721090
Conc: 20.60 ng/ml

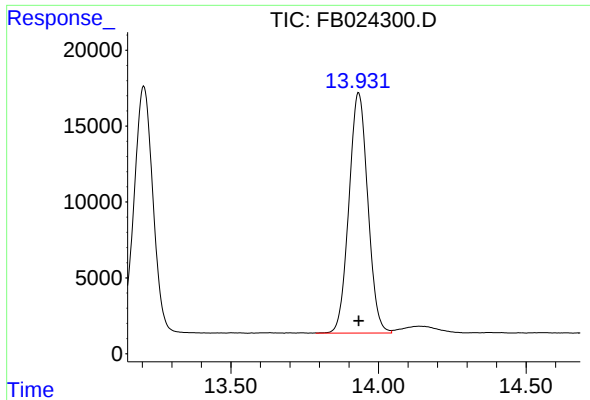

#9 O-Xylene

R.T.: 13.933 min
Delta R.T.: 0.000 min
Response: 703737
Conc: 20.65 ng/ml

Instrument :
FID_B
ClientSampleId :

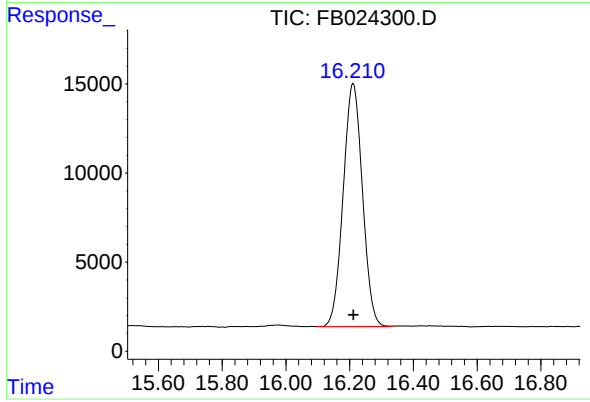

#10 1,2,4-Trimethylbenzene

R.T.: 16.211 min
Delta R.T.: 0.000 min
Response: 572918
Conc: 20.18 ng/ml