

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB050823\
Data File : FB029773.D
Signal(s) : FID2B.CH
Acq On : 8 May 2023 18:10
Operator : YP/AJ
Sample : 02666-01 50X
Misc : 5.10G/5.00 ML DI WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: May 09 01:21:12 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB041723.M
Quant Title :
QLast Update : Mon Apr 17 12:32:26 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.789	247184	18.549 ng/ml
Target Compounds			
8) t m-Xylene	13.185	9141	0.505 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB050823\
Data File : FB029773.D
Signal(s) : FID2B.CH
Acq On : 8 May 2023 18:10
Operator : YP/AJ
Sample : 02666-01 50X
Misc : 5.10G/5.00 ML DI WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: May 09 01:21:12 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB041723.M
Quant Title :
QLast Update : Mon Apr 17 12:32:26 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

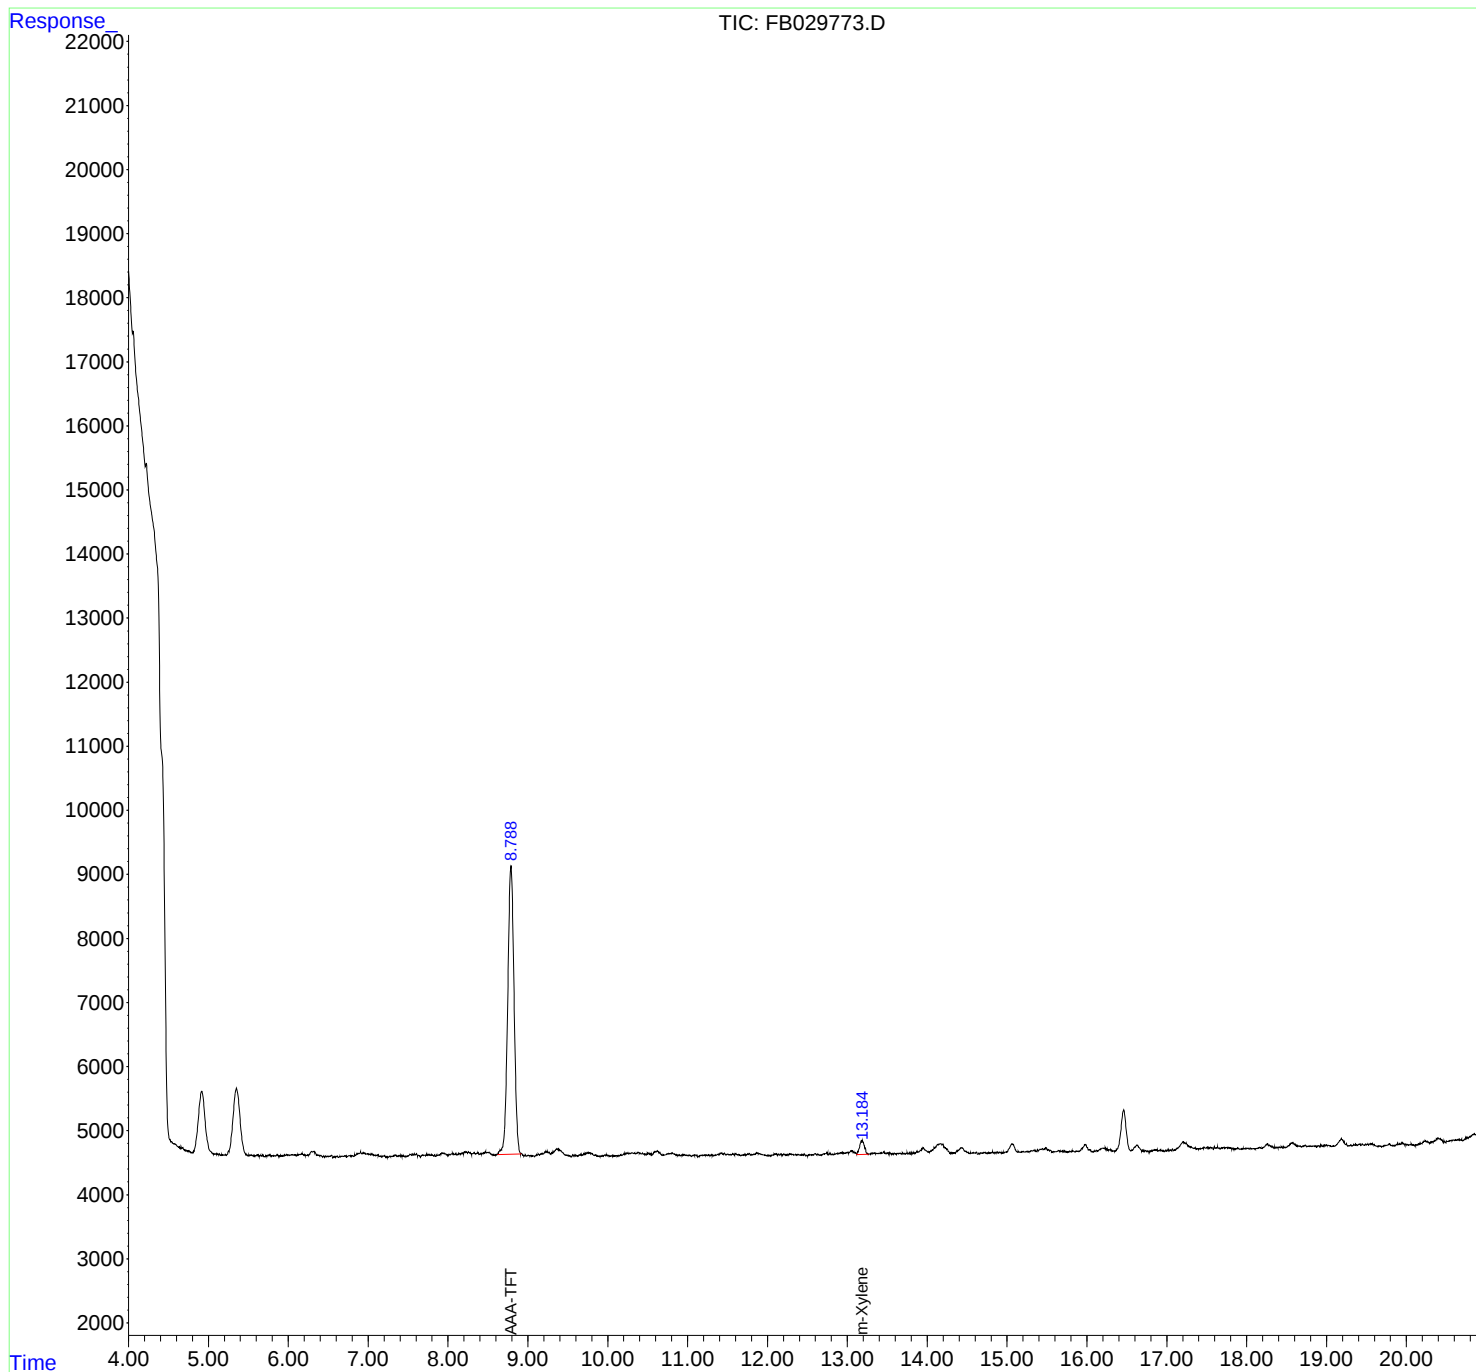


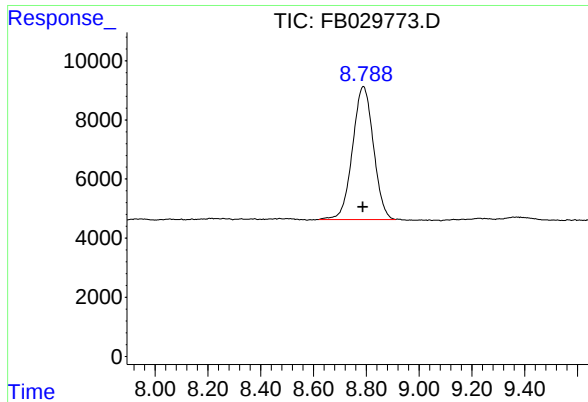

#5 AAA-TFT

R.T.: 8.789 min
Delta R.T.: 0.002 min
Response: 247184
Conc: 18.55 ng/ml

Instrument :
FID_B
ClientSampleId :

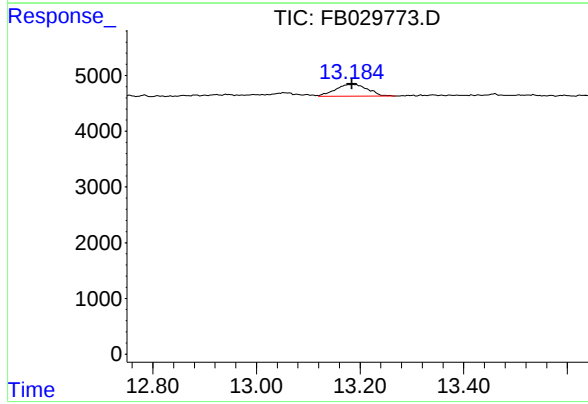

#8 m-Xylene

R.T.: 13.185 min
Delta R.T.: 0.000 min
Response: 9141
Conc: 0.51 ng/ml