

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB050823\
 Data File : FB029776.D
 Signal(s) : FID2B.CH
 Acq On : 8 May 2023 20:03
 Operator : YP/AJ
 Sample : BSF0508S2
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: May 09 01:21:27 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB041723.M
 Quant Title :
 QLast Update : Mon Apr 17 12:32:26 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.791	220098	16.516 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.710	473129	33.628 ng/ml
2) t 2,2,4-Trimethylpentane	7.416	508676	33.116 ng/ml
3) t n-Heptane	7.750	155470	9.660 ng/ml
4) t Benzene	7.887	191910	9.665 ng/ml
6) t Toluene	10.619	552714	28.616 ng/ml
7) t Ethylbenzene	13.056	178363	9.855 ng/ml
8) t m-Xylene	13.188	356484	19.711 ng/ml
9) t O-Xylene	13.915	349480	19.930 ng/ml
10) t 1,2,4-Trimethylbenzene	16.189	352530	19.726 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB050823\
Data File : FB029776.D
Signal(s) : FID2B.CH
Acq On : 8 May 2023 20:03
Operator : YP/AJ
Sample : BSF0508S2
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: May 09 01:21:27 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB041723.M
Quant Title :
QLast Update : Mon Apr 17 12:32:26 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

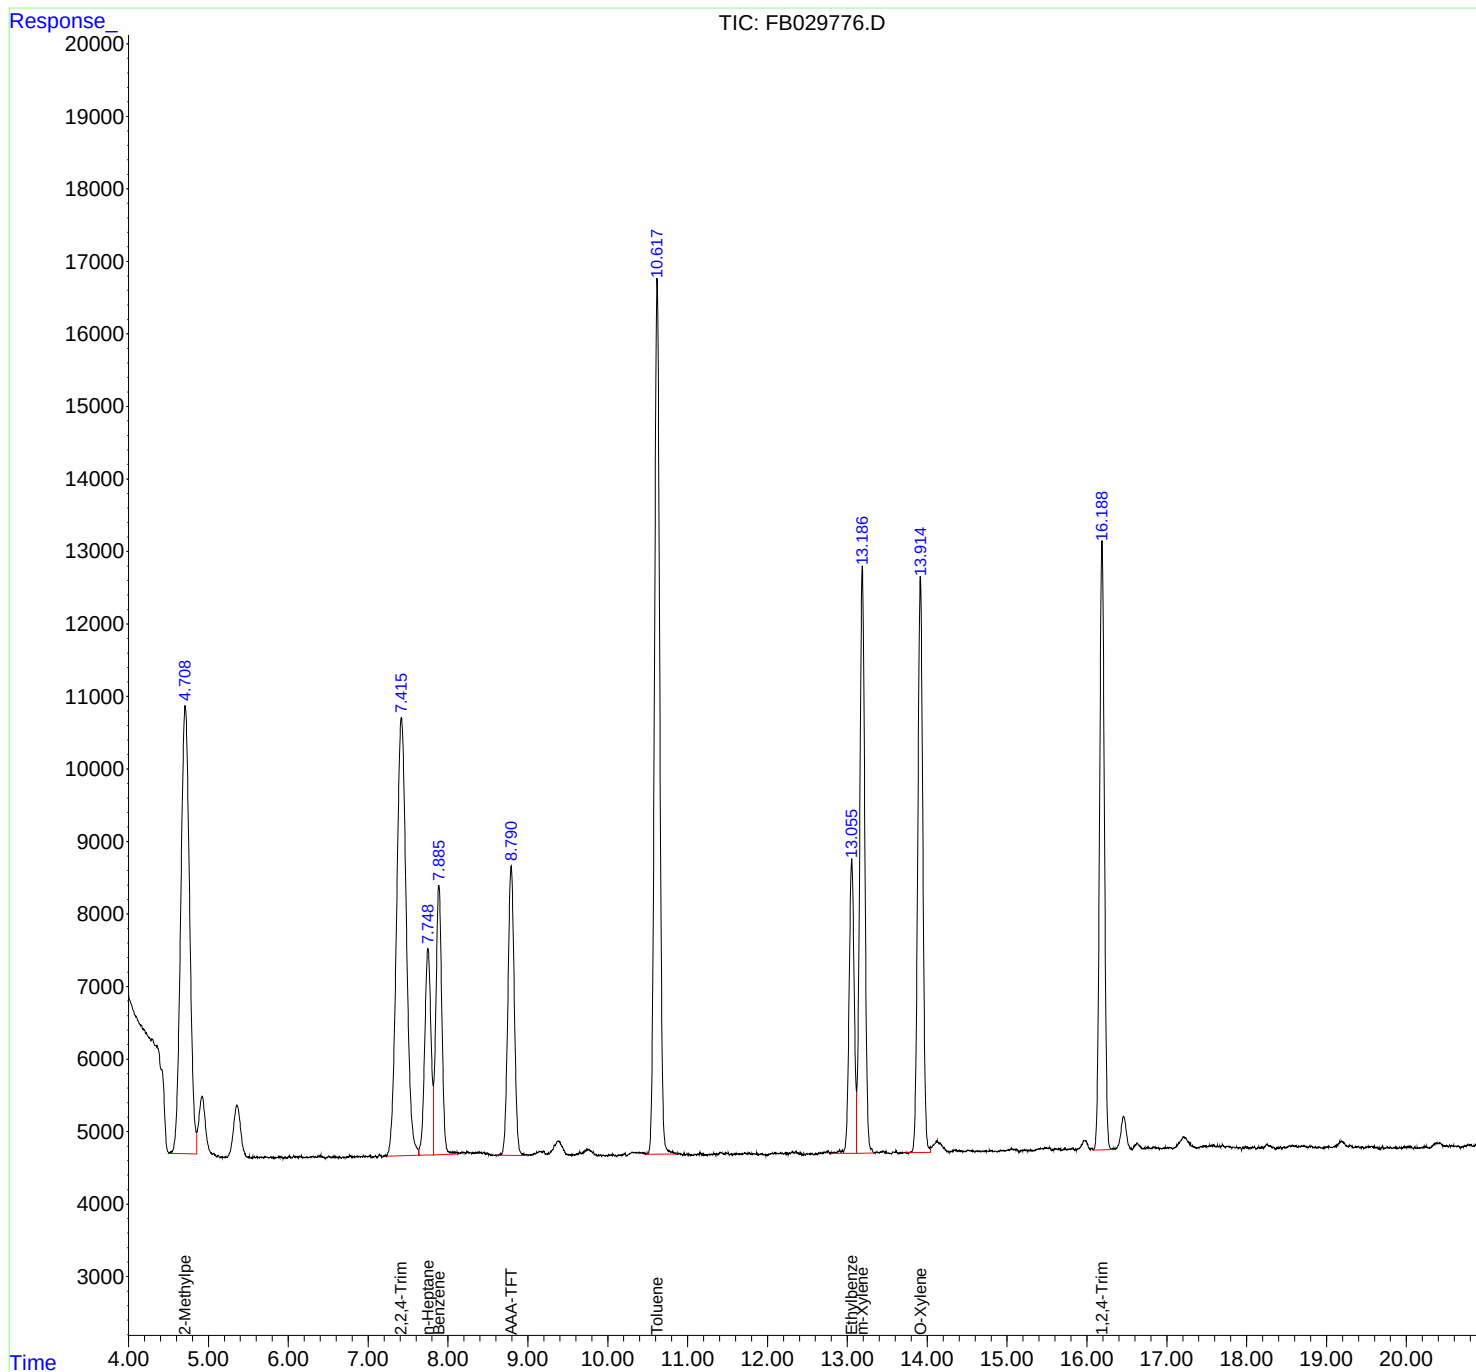

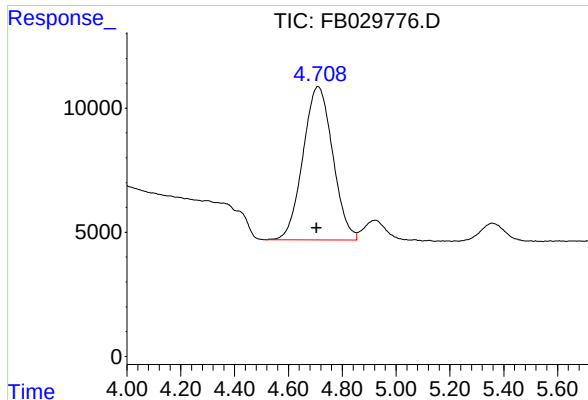


#1 2-Methylpentane

R.T.: 4.710 min
Delta R.T.: 0.005 min
Response: 473129
Conc: 33.63 ng/ml

Instrument :


FID_B

ClientSampleId :

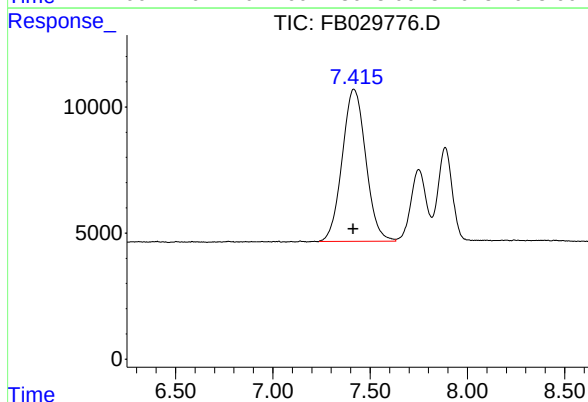


#2 2,2,4-Trimethylpentane

R.T.: 7.416 min
Delta R.T.: 0.004 min
Response: 508676
Conc: 33.12 ng/ml

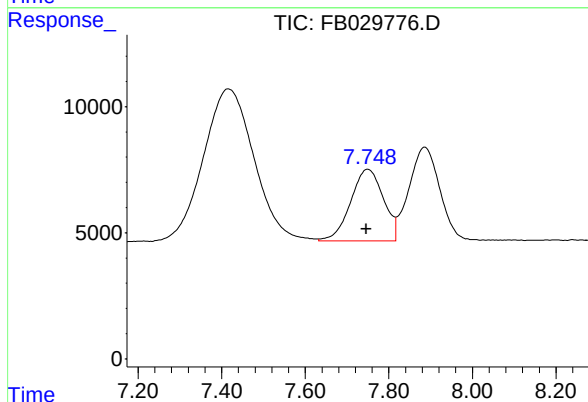


#3 n-Heptane

R.T.: 7.750 min
Delta R.T.: 0.003 min
Response: 155470
Conc: 9.66 ng/ml

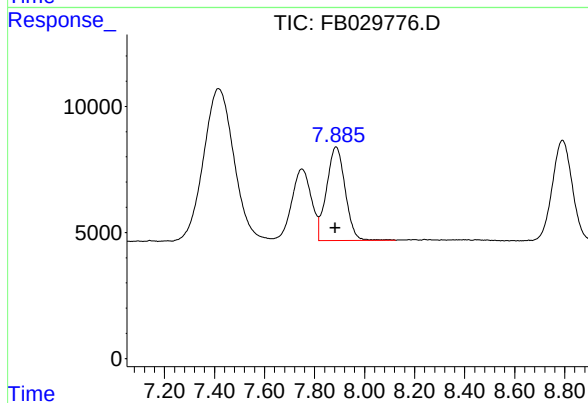

#4 Benzene


R.T.: 7.887 min
Delta R.T.: 0.004 min
Response: 191910
Conc: 9.66 ng/ml

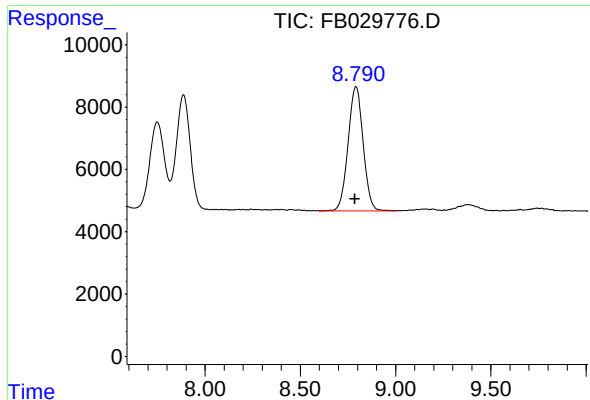

#5 AAA-TFT


R.T.: 8.791 min
Delta R.T.: 0.004 min
Response: 220098
Conc: 16.52 ng/ml

Instrument :
FID_B
ClientSampleId :

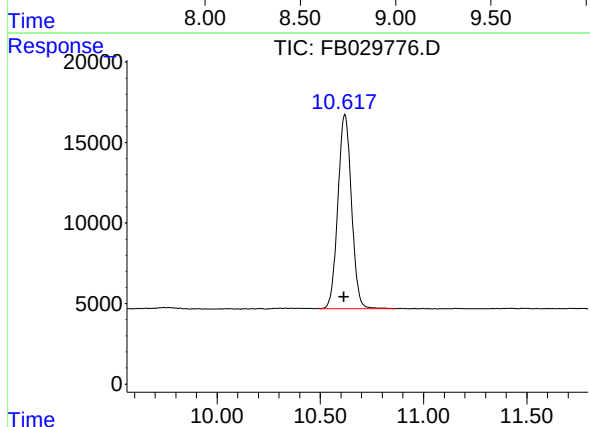


#6 Toluene

R.T.: 10.619 min
Delta R.T.: 0.003 min
Response: 552714
Conc: 28.62 ng/ml

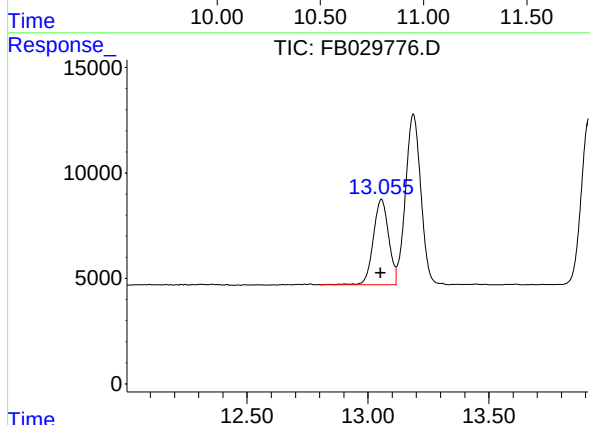


#7 Ethylbenzene

R.T.: 13.056 min
Delta R.T.: 0.004 min
Response: 178363
Conc: 9.85 ng/ml

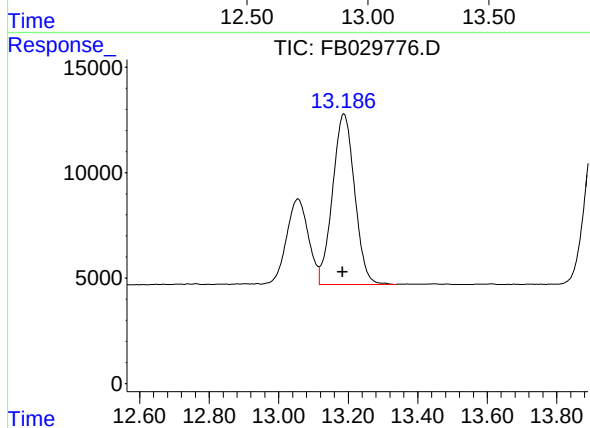

#8 m-Xylene


R.T.: 13.188 min
Delta R.T.: 0.003 min
Response: 356484
Conc: 19.71 ng/ml

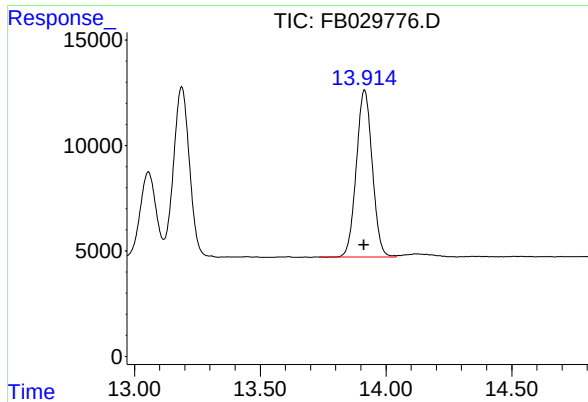

#9 O-Xylene

R.T.: 13.915 min
Delta R.T.: 0.003 min
Response: 349480
Conc: 19.93 ng/ml

Instrument :
FID_B
ClientSampleId :

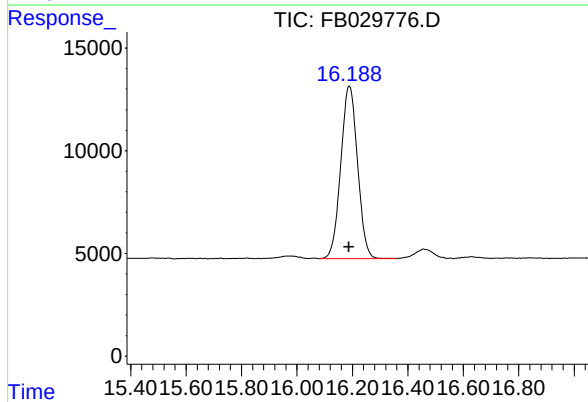

#10 1,2,4-Trimethylbenzene

R.T.: 16.189 min
Delta R.T.: 0.003 min
Response: 352530
Conc: 19.73 ng/ml