

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB050919\
 Data File : FB021001.D
 Signal(s) : FID2B.CH
 Acq On : 9 May 2019 9:57
 Operator : MJ/SJ
 Sample : BSF0509S1
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: May 10 01:42:22 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB042919.M
 Quant Title :
 QLast Update : Mon Apr 29 15:53:58 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.991	400054	22.300 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.854	1287486	28.542 ng/ml
2) t 2,2,4-Trimethylpentane	7.607	1231727	29.549 ng/ml
3) t n-Heptane	7.947	385479	9.737 ng/ml
4) t Benzene	8.083	410813	9.820 ng/ml
6) t Toluene	10.835	805335	29.072 ng/ml
7) t Ethylbenzene	13.285	258979	9.234 ng/ml
8) t m-Xylene	13.418	551042	18.541 ng/ml
9) t O-Xylene	14.148	568119	18.329 ng/ml
10) t 1,2,4-Trimethylbenzene	16.432	584880	18.859 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB050919\
Data File : FB021001.D
Signal(s) : FID2B.CH
Acq On : 9 May 2019 9:57
Operator : MJ/SJ
Sample : BSF0509S1
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: May 10 01:42:22 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB042919.M
Quant Title :
QLast Update : Mon Apr 29 15:53:58 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

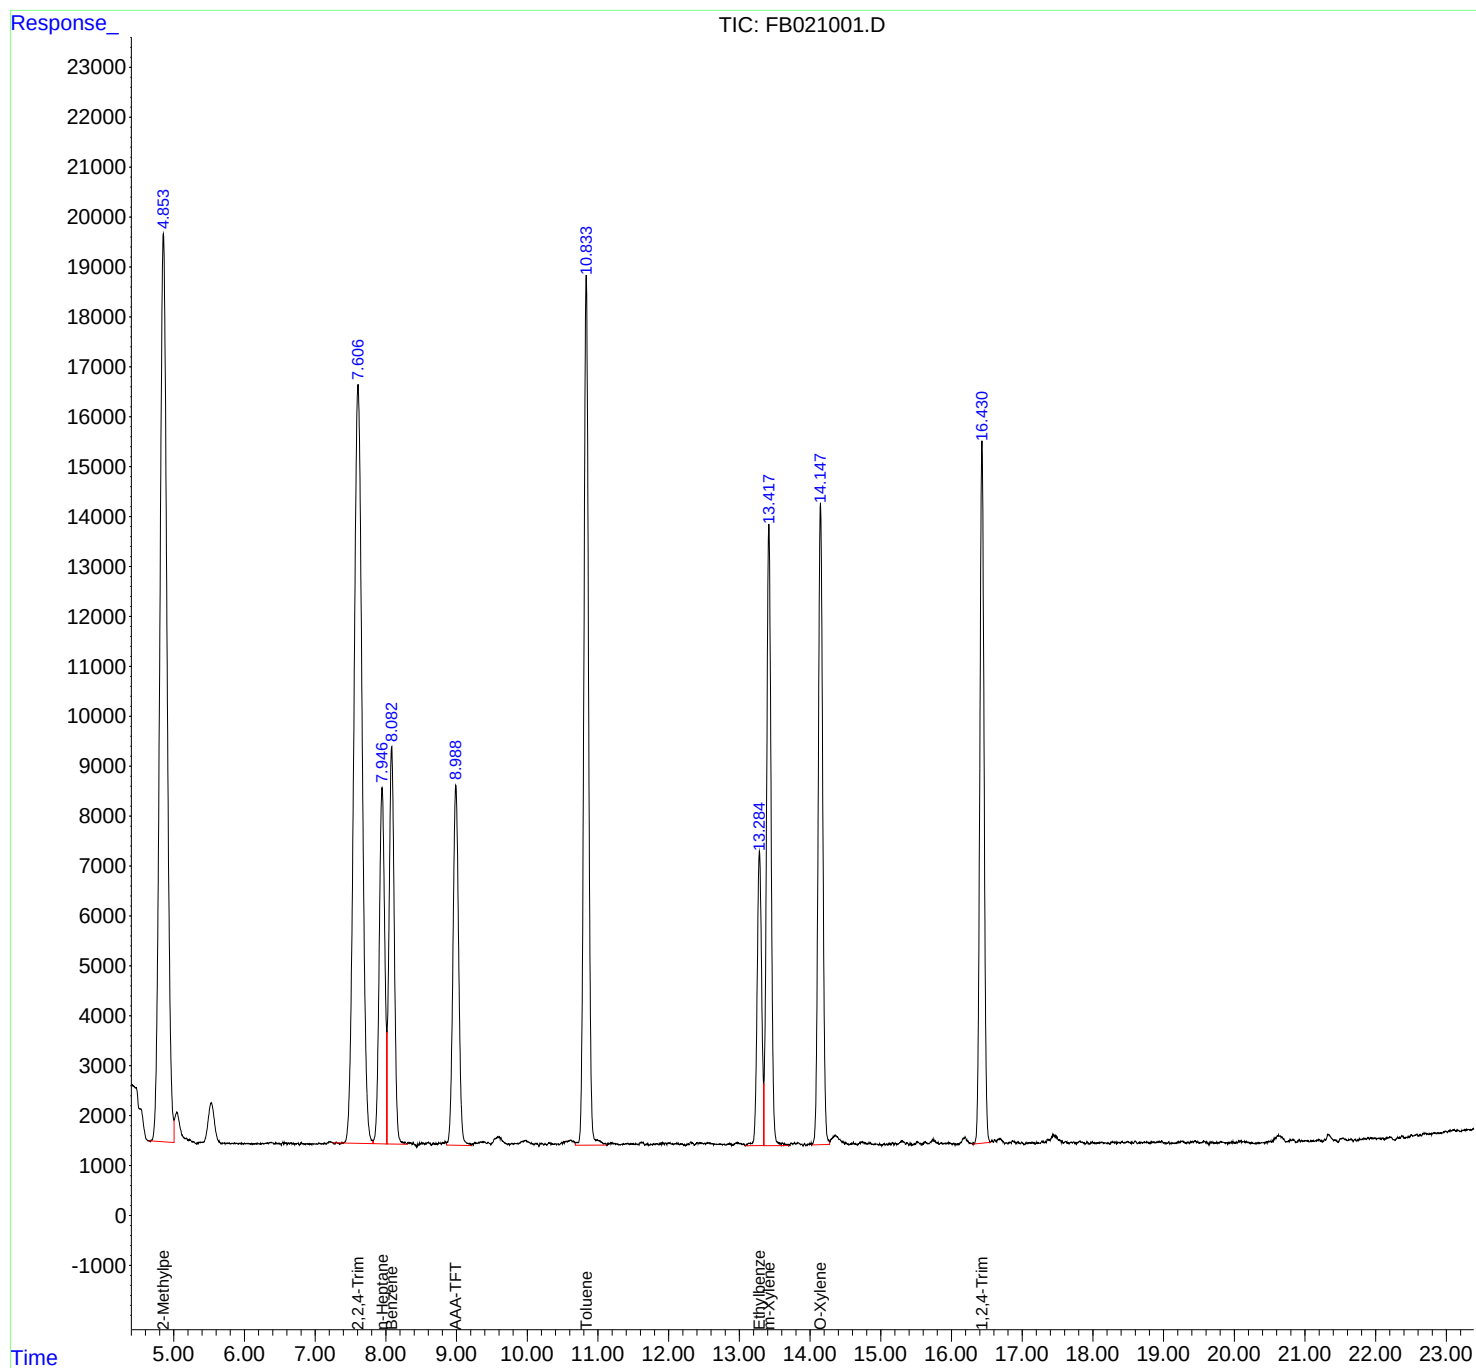

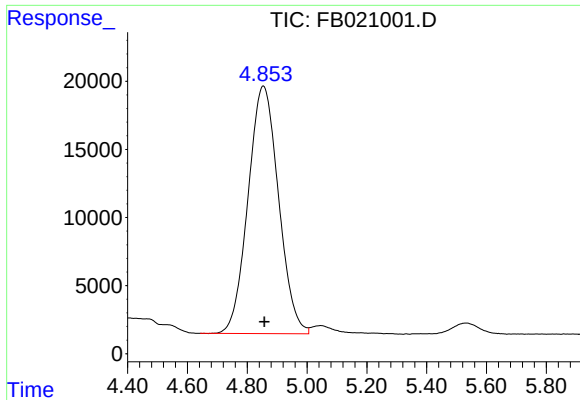


#1 2-Methylpentane

R.T.: 4.854 min
Delta R.T.: -0.003 min
Response: 1287486
Conc: 28.54 ng/ml

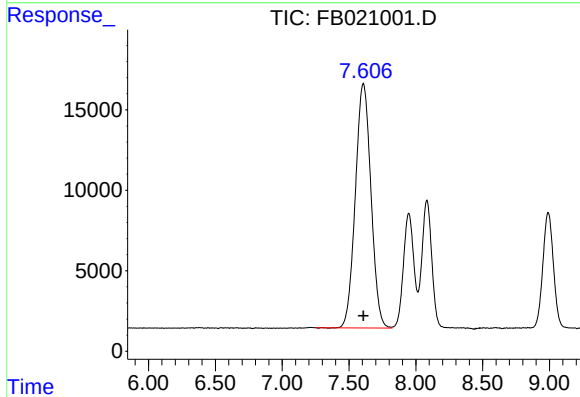


#2 2,2,4-Trimethylpentane

R.T.: 7.607 min
Delta R.T.: -0.002 min
Response: 1231727
Conc: 29.55 ng/ml

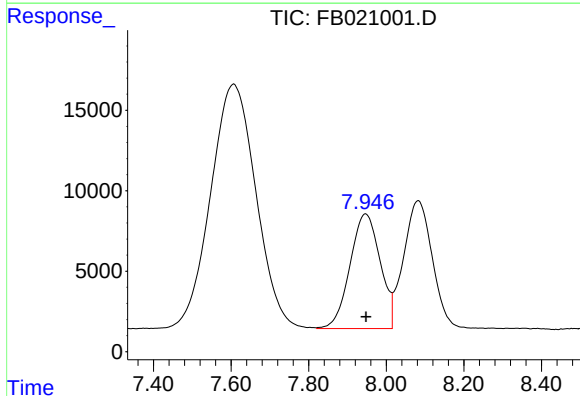


#3 n-Heptane

R.T.: 7.947 min
Delta R.T.: -0.001 min
Response: 385479
Conc: 9.74 ng/ml

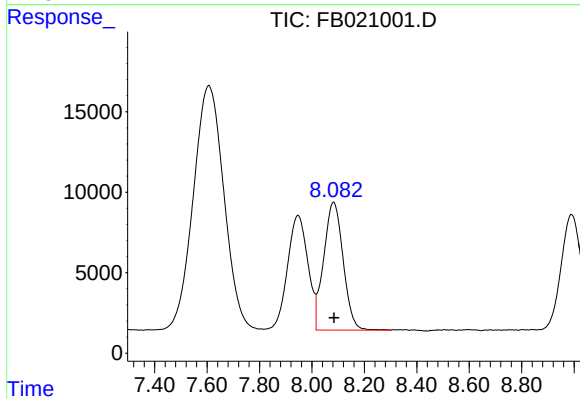


#4 Benzene

R.T.: 8.083 min
Delta R.T.: -0.002 min
Response: 410813
Conc: 9.82 ng/ml

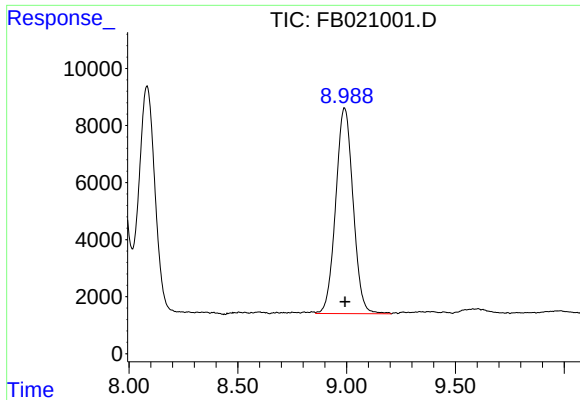


#5 AAA-TFT

R.T.: 8.991 min
Delta R.T.: -0.001 min
Response: 400054
Conc: 22.30 ng/ml

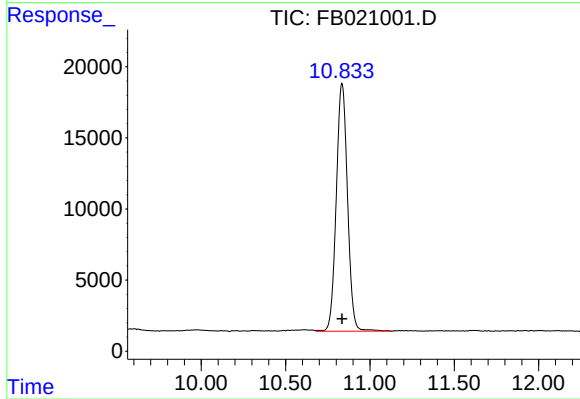


#6 Toluene

R.T.: 10.835 min
Delta R.T.: -0.001 min
Response: 805335
Conc: 29.07 ng/ml

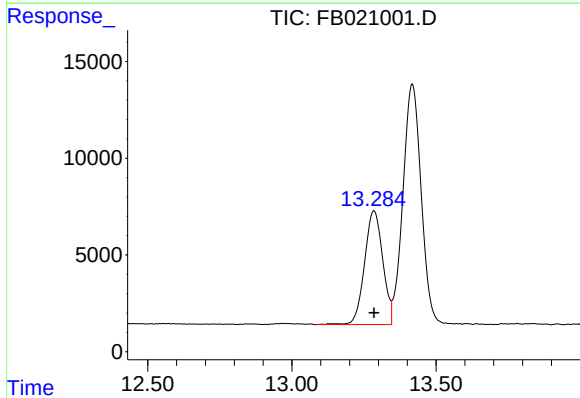


#7 Ethylbenzene

R.T.: 13.285 min
Delta R.T.: 0.000 min
Response: 258979
Conc: 9.23 ng/ml

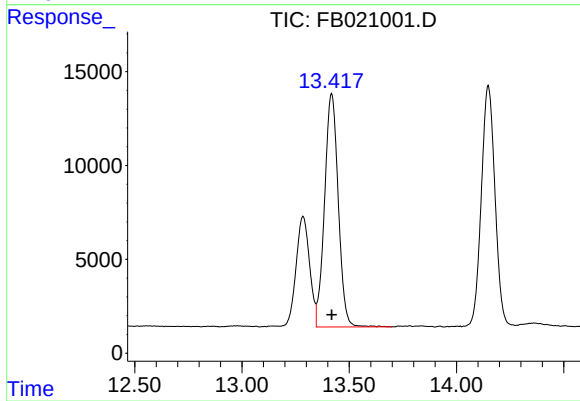


#8 m-Xylene

R.T.: 13.418 min
Delta R.T.: 0.000 min
Response: 551042
Conc: 18.54 ng/ml

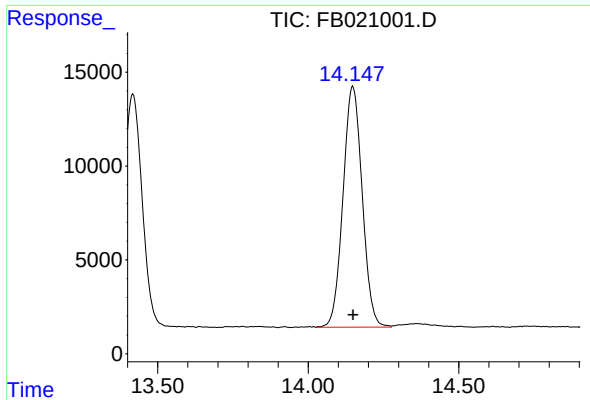

#9 O-Xylene

R.T.: 14.148 min
Delta R.T.: -0.001 min
Response: 568119
Conc: 18.33 ng/ml

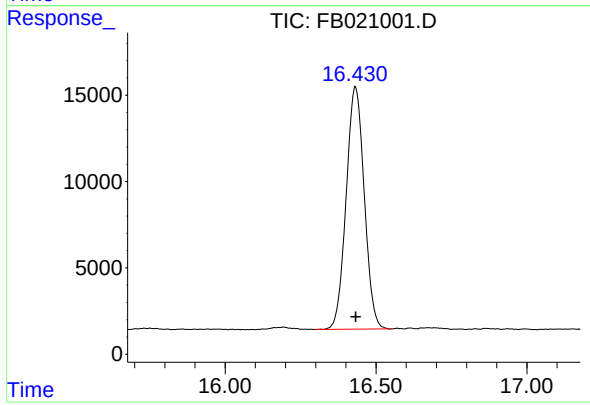

#10 1,2,4-Trimethylbenzene

R.T.: 16.432 min
Delta R.T.: -0.001 min
Response: 584880
Conc: 18.86 ng/ml