

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB050919\
 Data File : FB021007.D
 Signal(s) : FID2B.CH
 Acq On : 9 May 2019 13:19
 Operator : MJ/SJ
 Sample : K2754-01MSD
 Misc : 5.05g/5.00ml DI WATER
 ALS Vial : 9 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: May 10 01:43:27 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB042919.M
 Quant Title :
 QLast Update : Mon Apr 29 15:53:58 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.992	392138	21.859 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.856	974264	21.598 ng/ml
2) t	2,2,4-Trimethylpentane	7.609	876969	21.039 ng/ml
3) t	n-Heptane	7.949	270430	6.831 ng/ml
4) t	Benzene	8.085	357089	8.536 ng/ml
6) t	Toluene	10.836	685282	24.738 ng/ml
7) t	Ethylbenzene	13.287	215025	7.667 ng/ml
8) t	m-Xylene	13.420	467132	15.718 ng/ml
9) t	O-Xylene	14.150	482657	15.571 ng/ml
10) t	1,2,4-Trimethylbenzene	16.434	471761	15.211 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB050919\
Data File : FB021007.D
Signal(s) : FID2B.CH
Acq On : 9 May 2019 13:19
Operator : MJ/SJ
Sample : K2754-01MSD
Misc : 5.05g/5.00ml DI WATER
ALS Vial : 9 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: May 10 01:43:27 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB042919.M
Quant Title :
QLast Update : Mon Apr 29 15:53:58 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

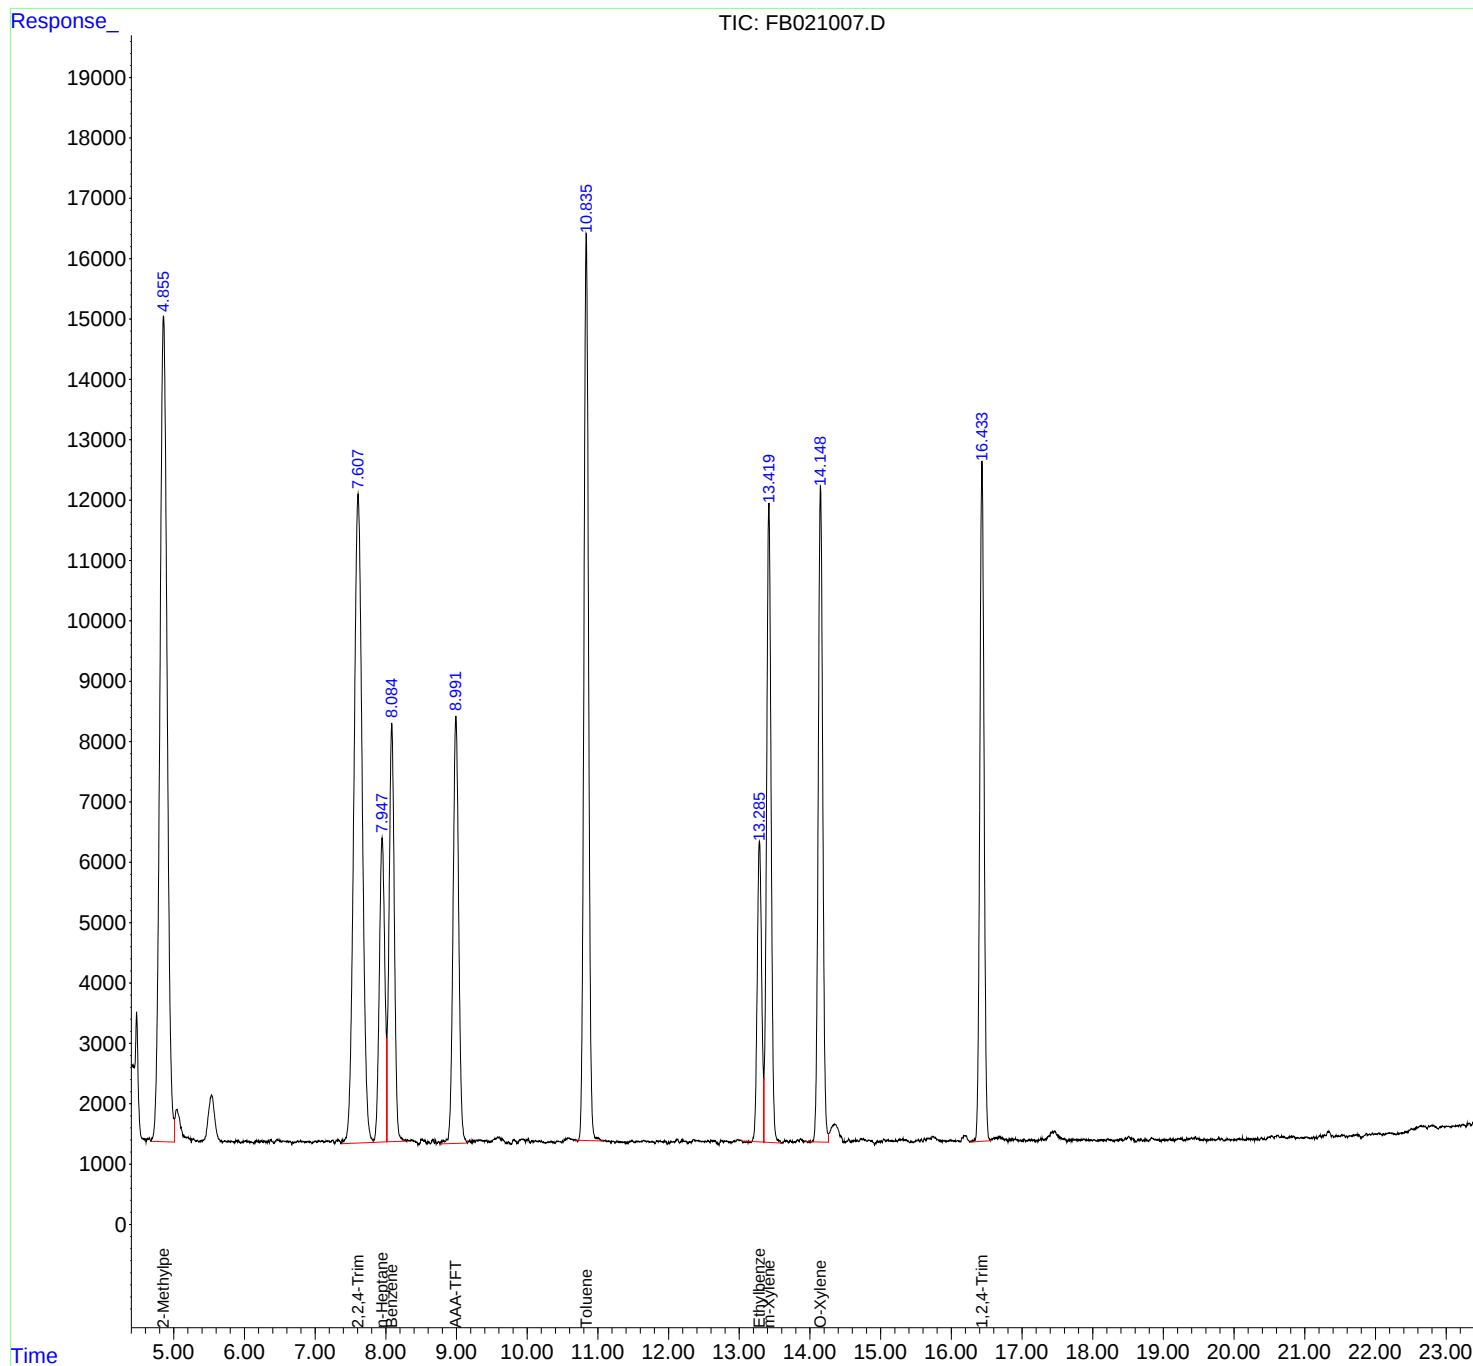

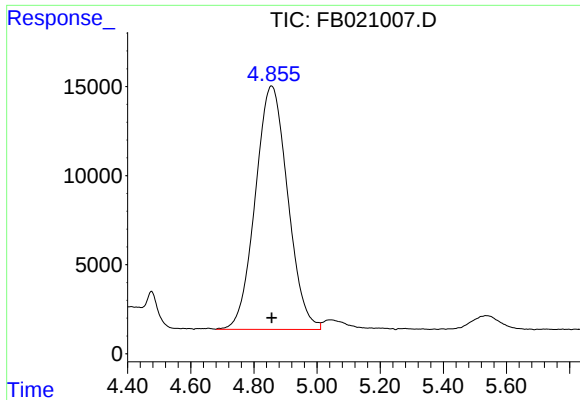


#1 2-Methylpentane

R.T.: 4.856 min
Delta R.T.: 0.000 min
Response: 974264
Conc: 21.60 ng/ml

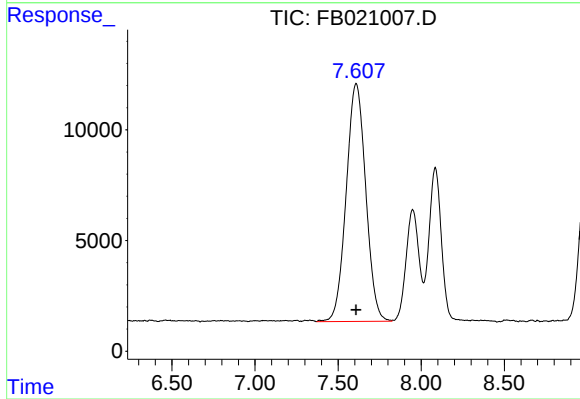


#2 2,2,4-Trimethylpentane

R.T.: 7.609 min
Delta R.T.: 0.000 min
Response: 876969
Conc: 21.04 ng/ml

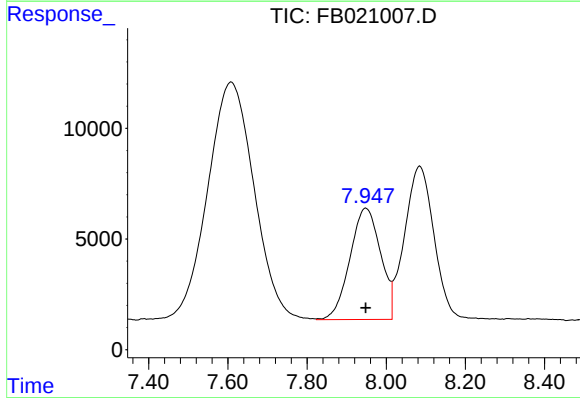


#3 n-Heptane

R.T.: 7.949 min
Delta R.T.: 0.000 min
Response: 270430
Conc: 6.83 ng/ml

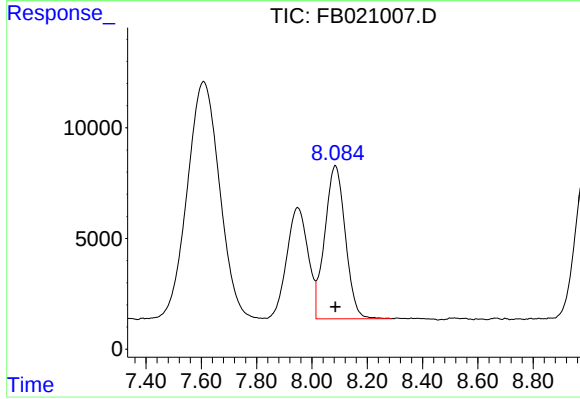


#4 Benzene

R.T.: 8.085 min
Delta R.T.: 0.000 min
Response: 357089
Conc: 8.54 ng/ml

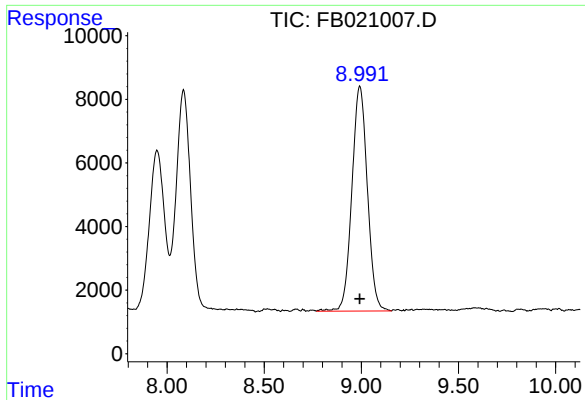


#5 AAA-TFT

R.T.: 8.992 min
Delta R.T.: 0.000 min
Response: 392138
Conc: 21.86 ng/ml

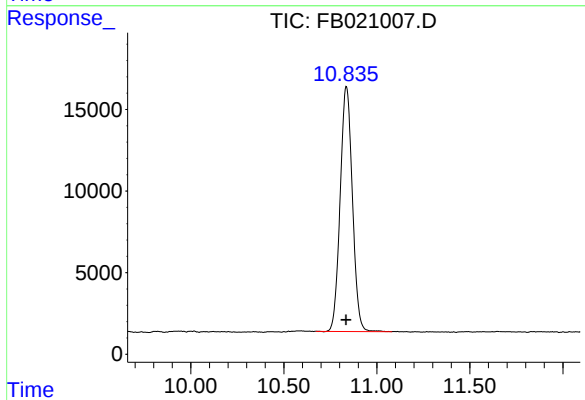


#6 Toluene

R.T.: 10.836 min
Delta R.T.: 0.000 min
Response: 685282
Conc: 24.74 ng/ml

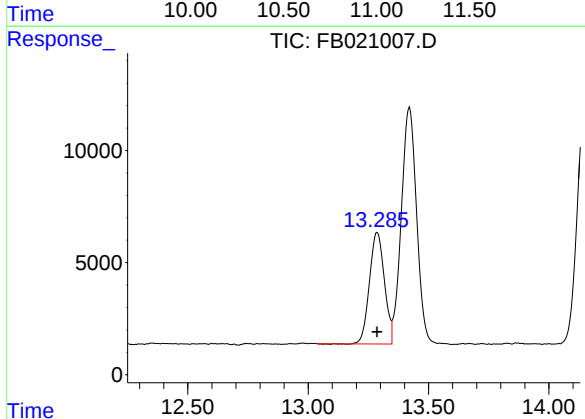


#7 Ethylbenzene

R.T.: 13.287 min
Delta R.T.: 0.000 min
Response: 215025
Conc: 7.67 ng/ml

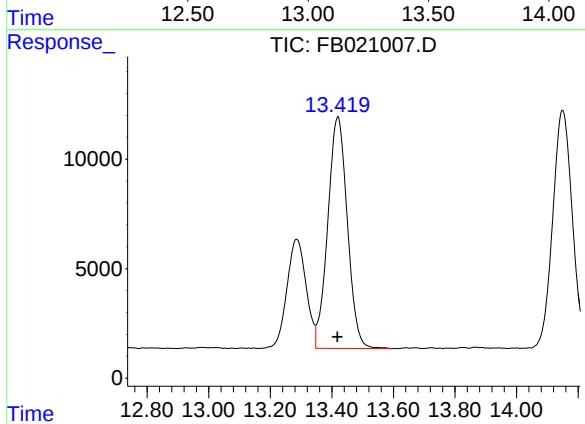


#8 m-Xylene

R.T.: 13.420 min
Delta R.T.: 0.001 min
Response: 467132
Conc: 15.72 ng/ml

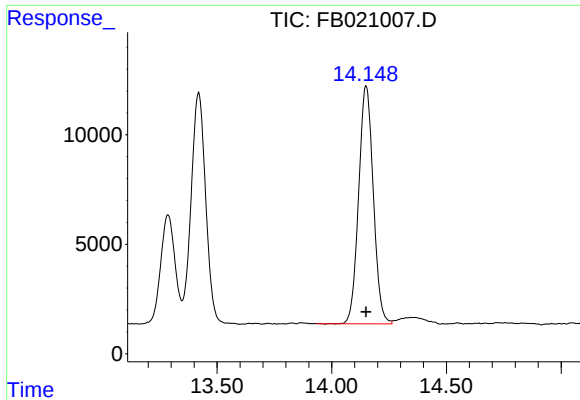

#9 O-Xylene

R.T.: 14.150 min
Delta R.T.: 0.000 min
Response: 482657
Conc: 15.57 ng/ml

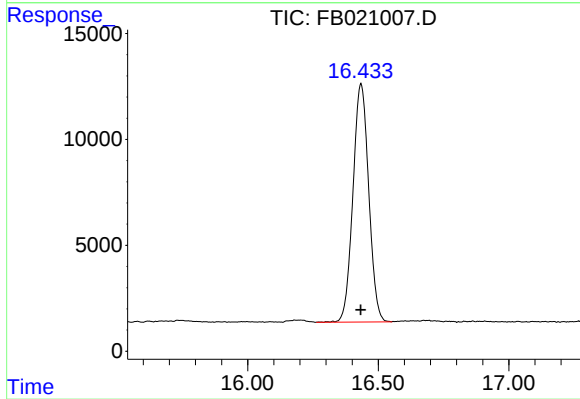

#10 1,2,4-Trimethylbenzene

R.T.: 16.434 min
Delta R.T.: 0.001 min
Response: 471761
Conc: 15.21 ng/ml