

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB050923\
 Data File : FB029783.D
 Signal(s) : FID2B.CH
 Acq On : 9 May 2023 14:03
 Operator : YP/AJ
 Sample : BSF0509S2
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0509S2

Integration File: Calibration.e
 Quant Time: May 10 06:07:09 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB041723.M
 Quant Title :
 QLast Update : Mon Apr 17 12:32:26 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.787	282765	21.219 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.700	481868	34.249 ng/ml
2) t	2,2,4-Trimethylpentane	7.411	455116	29.629 ng/ml
3) t	n-Heptane	7.745	164713	10.234 ng/ml
4) t	Benzene	7.882	202595	10.203 ng/ml
6) t	Toluene	10.614	569004	29.459 ng/ml
7) t	Ethylbenzene	13.051	175998	9.724 ng/ml
8) t	m-Xylene	13.183	353172	19.528 ng/ml
9) t	O-Xylene	13.910	332807	18.979 ng/ml
10) t	1,2,4-Trimethylbenzene	16.185	318453	17.819 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB050923\
Data File : FB029783.D
Signal(s) : FID2B.CH
Acq On : 9 May 2023 14:03
Operator : YP/AJ
Sample : BSF0509S2
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0509S2

Integration File: Calibration.e
Quant Time: May 10 06:07:09 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB041723.M
Quant Title :
QLast Update : Mon Apr 17 12:32:26 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

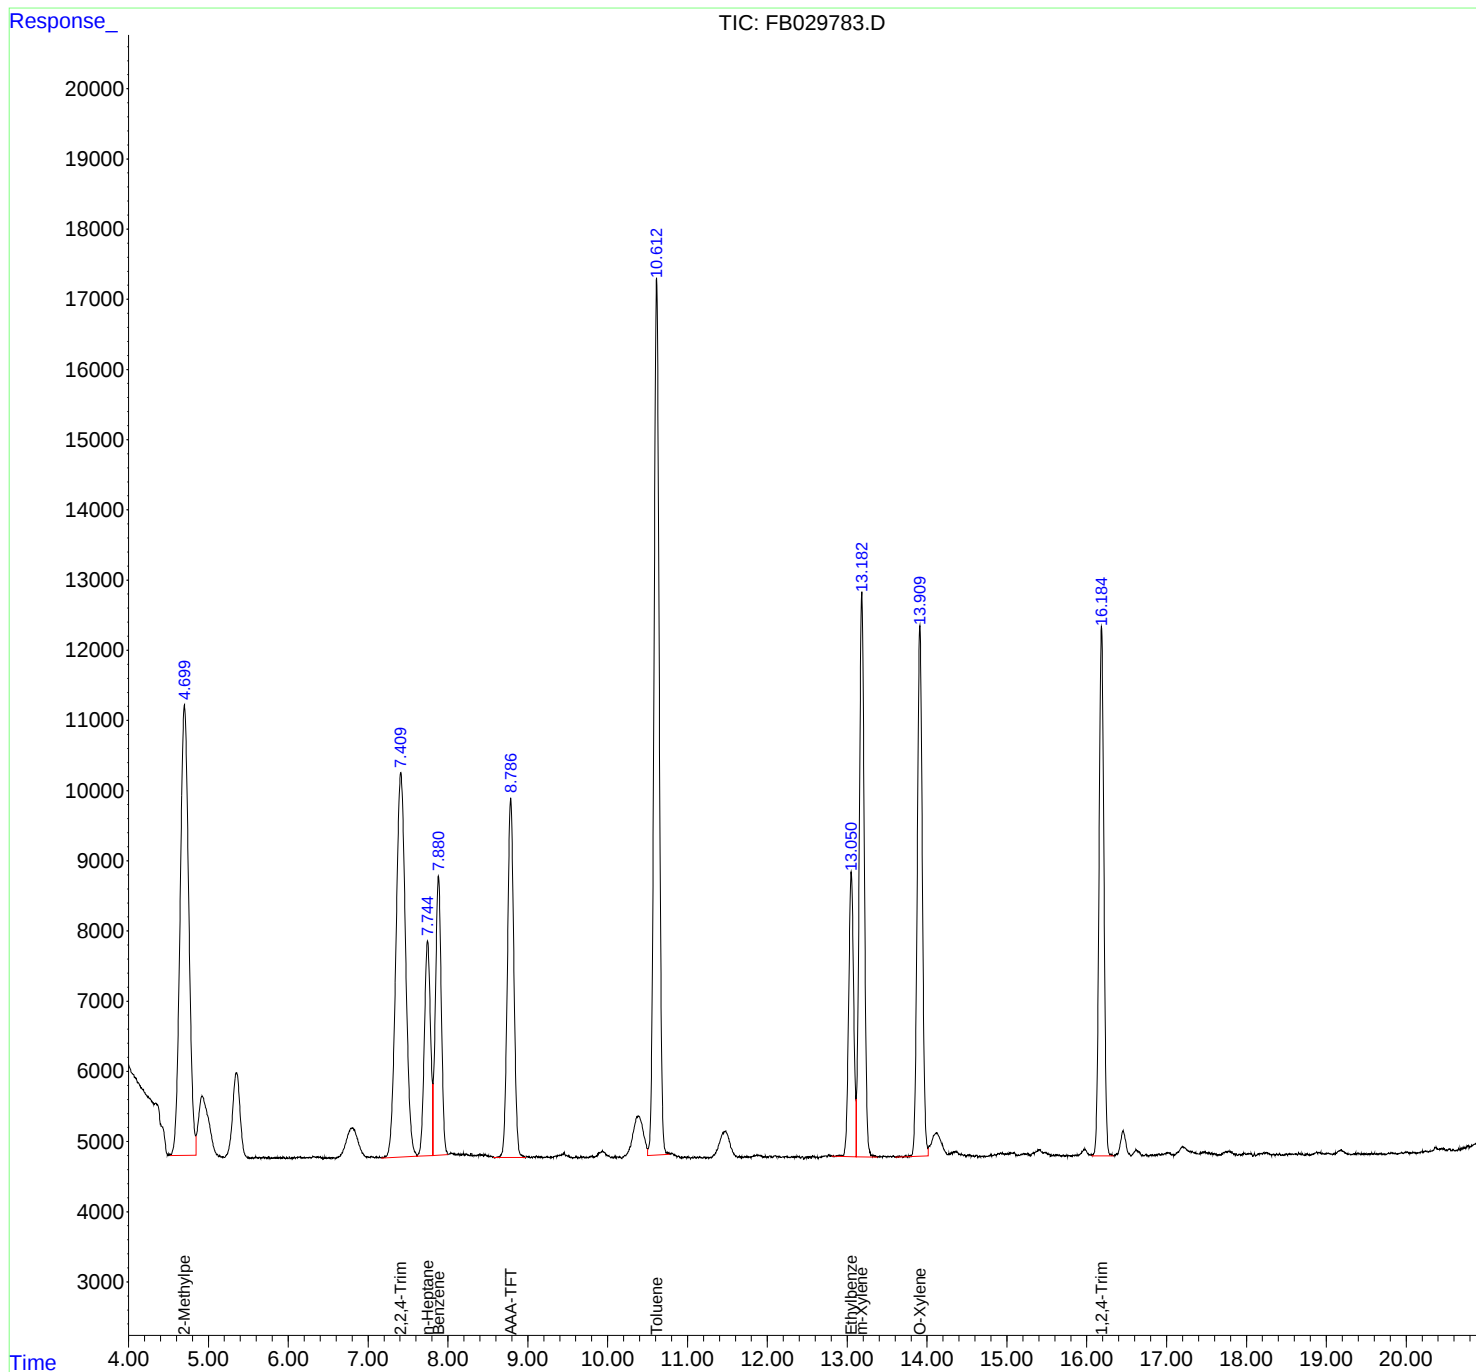


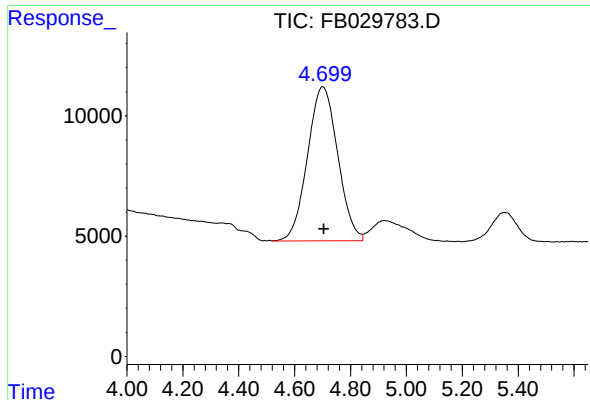

#1 2-Methylpentane


R.T.: 4.700 min
Delta R.T.: -0.005 min
Response: 481868
Conc: 34.25 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0509S2

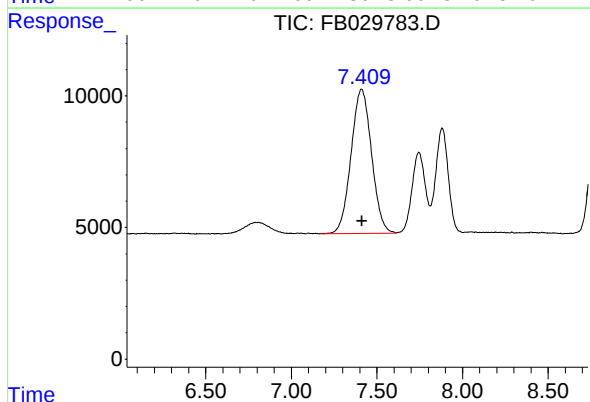


#2 2,2,4-Trimethylpentane

R.T.: 7.411 min
Delta R.T.: -0.002 min
Response: 455116
Conc: 29.63 ng/ml

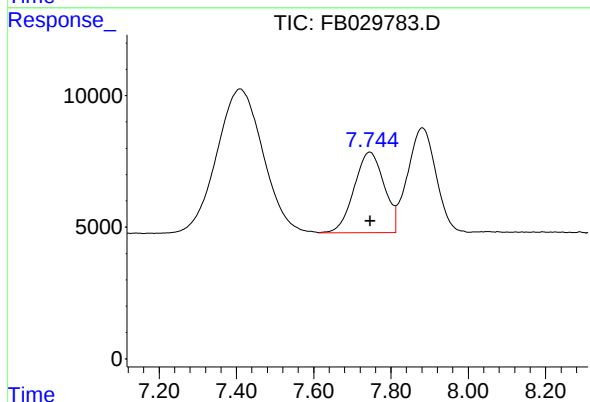


#3 n-Heptane

R.T.: 7.745 min
Delta R.T.: -0.001 min
Response: 164713
Conc: 10.23 ng/ml

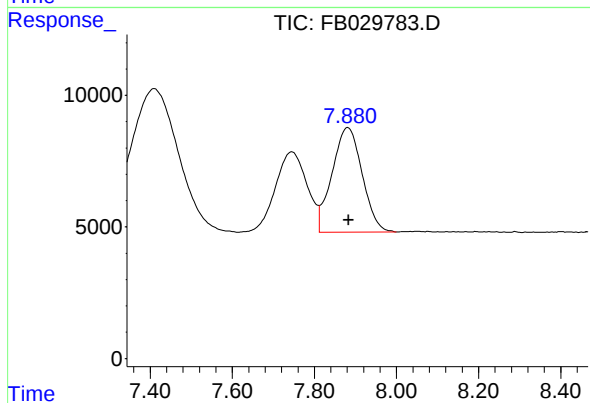

#4 Benzene


R.T.: 7.882 min
Delta R.T.: -0.002 min
Response: 202595
Conc: 10.20 ng/ml

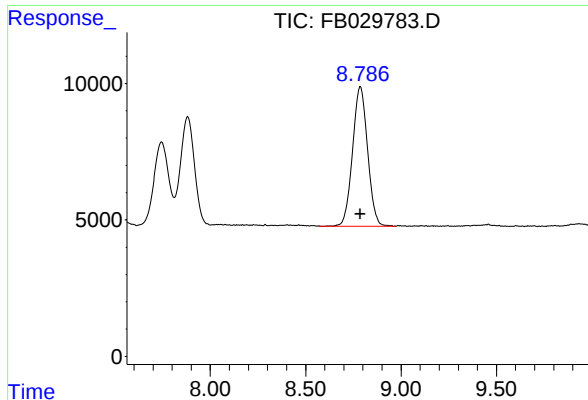

#5 AAA-TFT


R.T.: 8.787 min
Delta R.T.: 0.000 min
Response: 282765
Conc: 21.22 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0509S2

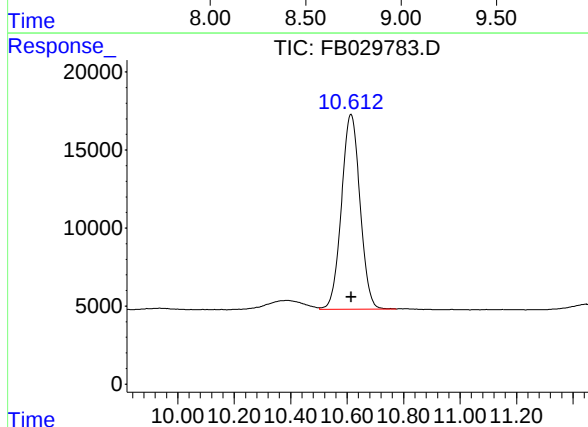


#6 Toluene

R.T.: 10.614 min
Delta R.T.: -0.002 min
Response: 569004
Conc: 29.46 ng/ml

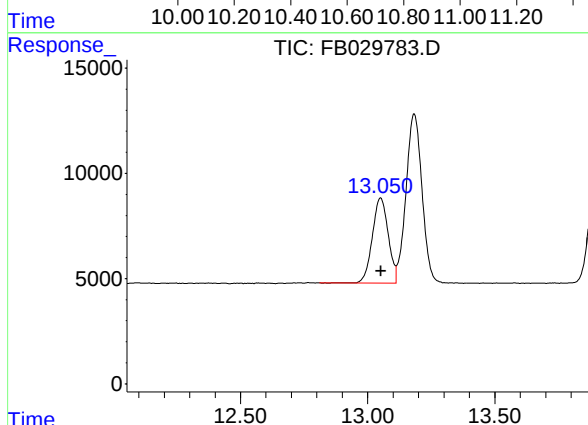


#7 Ethylbenzene

R.T.: 13.051 min
Delta R.T.: -0.001 min
Response: 175998
Conc: 9.72 ng/ml

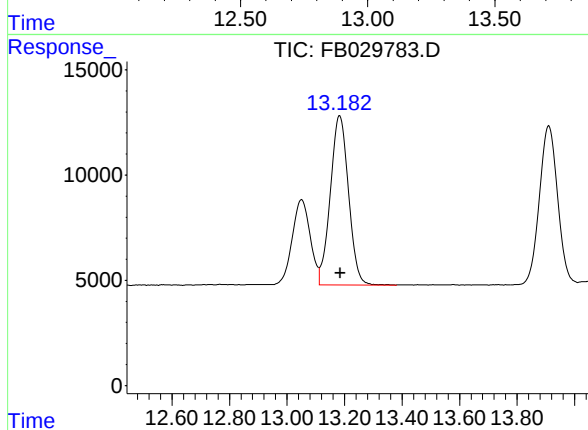

#8 m-Xylene


R.T.: 13.183 min
Delta R.T.: -0.001 min
Response: 353172
Conc: 19.53 ng/ml

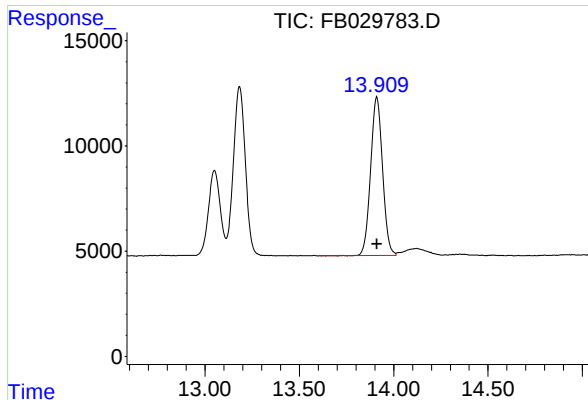

#9 O-Xylene

R.T.: 13.910 min
Delta R.T.: -0.001 min
Response: 332807
Conc: 18.98 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0509S2

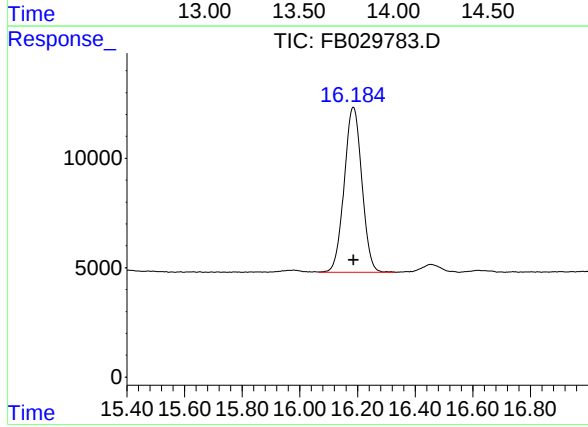

#10 1,2,4-Trimethylbenzene

R.T.: 16.185 min
Delta R.T.: -0.001 min
Response: 318453
Conc: 17.82 ng/ml