

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB051021\
 Data File : FB025739.D
 Signal(s) : FID2B.CH
 Acq On : 10 May 2021 10:47
 Operator : DD/AJ
 Sample : BSF0510S1
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: May 11 01:11:29 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB050521.M
 Quant Title :
 QLast Update : Thu May 06 15:01:51 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.228	407065	18.965 ng/ml
Target Compounds			
1) t 2-Methylpentane	5.187	783336	31.210 ng/ml
2) t 2,2,4-Trimethylpentane	7.881	738970	34.338 ng/ml
3) t n-Heptane	8.204	322055	10.650 ng/ml
4) t Benzene	8.355	387879	10.140 ng/ml
6) t Toluene	11.049	1137345	30.400 ng/ml
7) t Ethylbenzene	13.458	365972	10.110 ng/ml
8) t m-Xylene	13.588	734544	20.201 ng/ml
9) t O-Xylene	14.312	663142	19.210 ng/ml
10) t 1,2,4-Trimethylbenzene	16.566	560329	19.722 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB051021\
Data File : FB025739.D
Signal(s) : FID2B.CH
Acq On : 10 May 2021 10:47
Operator : DD/AJ
Sample : BSF0510S1
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: May 11 01:11:29 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB050521.M
Quant Title :
QLast Update : Thu May 06 15:01:51 2021
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

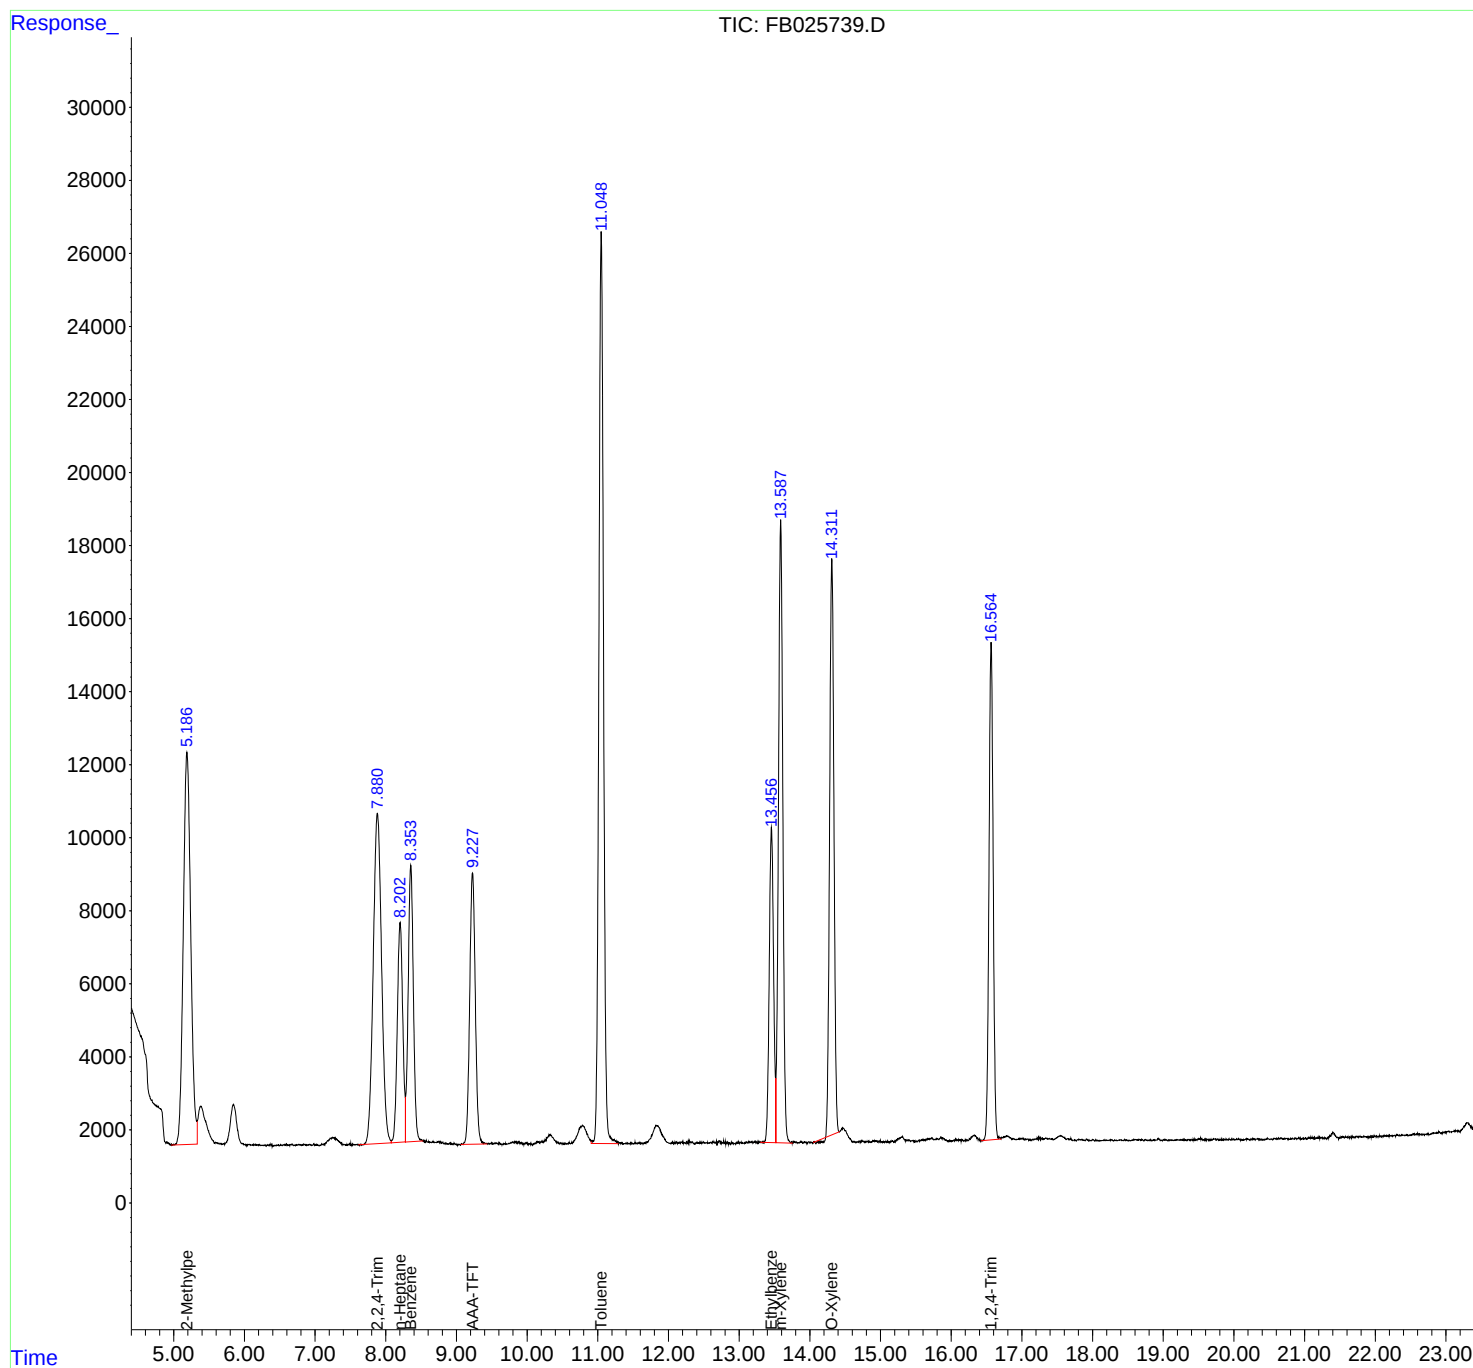

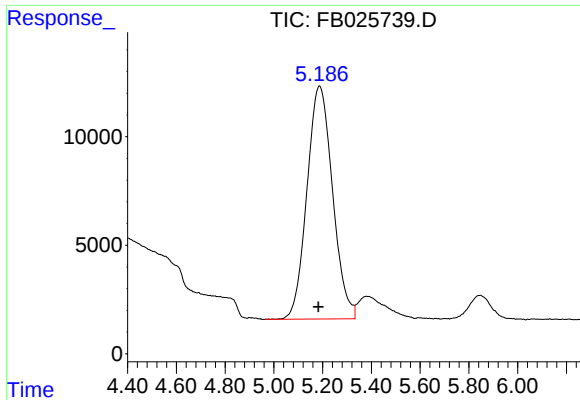


#1 2-Methylpentane

R.T.: 5.187 min
Delta R.T.: 0.004 min
Response: 783336
Conc: 31.21 ng/ml

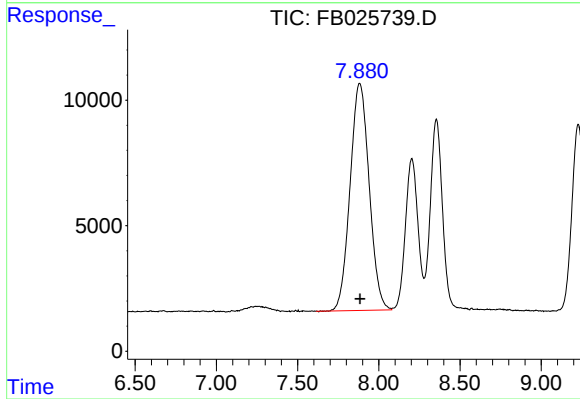


#2 2,2,4-Trimethylpentane

R.T.: 7.881 min
Delta R.T.: -0.003 min
Response: 738970
Conc: 34.34 ng/ml

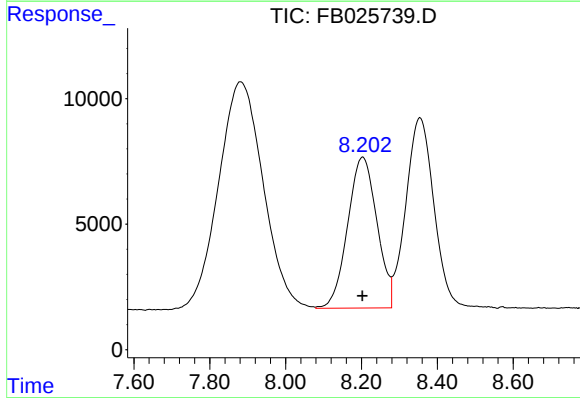


#3 n-Heptane

R.T.: 8.204 min
Delta R.T.: 0.001 min
Response: 322055
Conc: 10.65 ng/ml

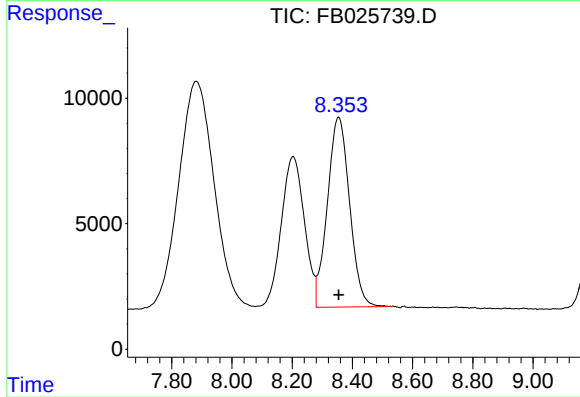


#4 Benzene

R.T.: 8.355 min
Delta R.T.: 0.000 min
Response: 387879
Conc: 10.14 ng/ml

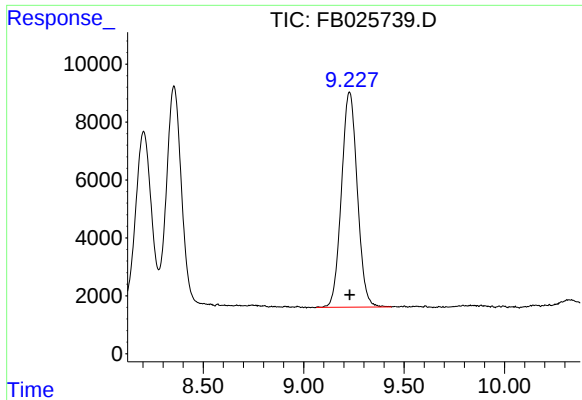


#5 AAA-TFT

R.T.: 9.228 min
Delta R.T.: -0.001 min
Response: 407065
Conc: 18.96 ng/ml

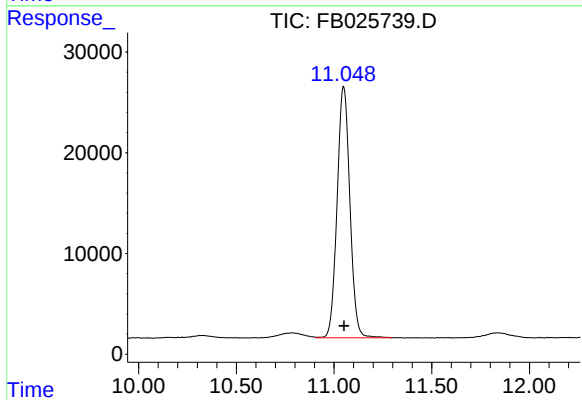


#6 Toluene

R.T.: 11.049 min
Delta R.T.: -0.002 min
Response: 1137345
Conc: 30.40 ng/ml

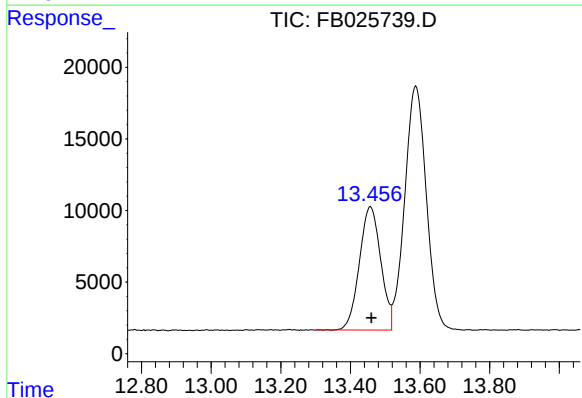


#7 Ethylbenzene

R.T.: 13.458 min
Delta R.T.: -0.003 min
Response: 365972
Conc: 10.11 ng/ml

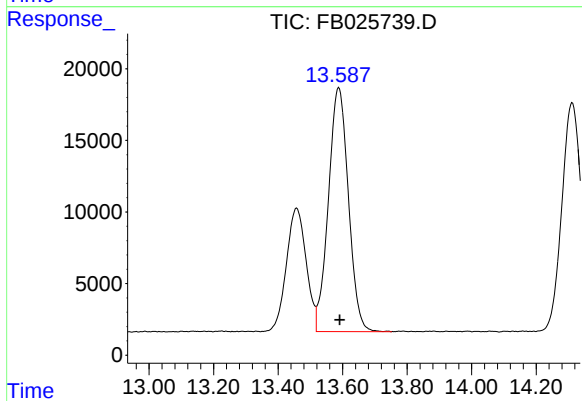


#8 m-Xylene

R.T.: 13.588 min
Delta R.T.: -0.003 min
Response: 734544
Conc: 20.20 ng/ml

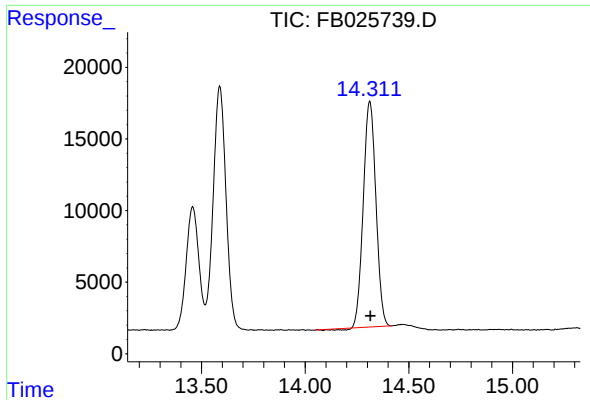

#9 O-Xylene

R.T.: 14.312 min
Delta R.T.: -0.003 min
Response: 663142
Conc: 19.21 ng/ml

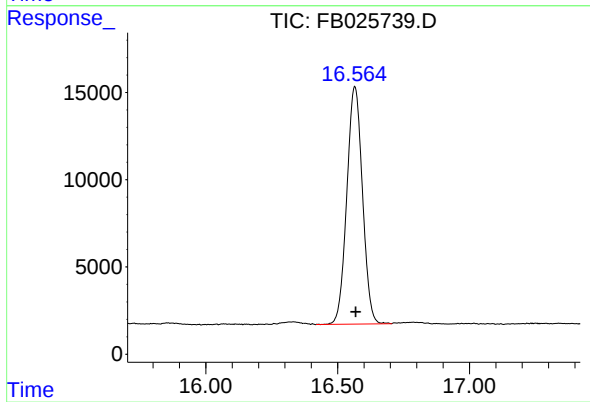

#10 1,2,4-Trimethylbenzene

R.T.: 16.566 min
Delta R.T.: -0.003 min
Response: 560329
Conc: 19.72 ng/ml