

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB051021\
 Data File : FB025745.D
 Signal(s) : FID2B.CH
 Acq On : 10 May 2021 15:01
 Operator : DD/AJ
 Sample : M2262-01
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 9 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: May 11 01:12:12 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB050521.M
 Quant Title :
 QLast Update : Thu May 06 15:01:51 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.233	404768	18.858 ng/ml
Target Compounds			
1) t 2-Methylpentane	5.201	158979	6.334 ng/ml
2) t 2,2,4-Trimethylpentane	7.891	157985	7.341 ng/ml
3) t n-Heptane	8.211	64523	2.134 ng/ml
4) t Benzene	8.361	77806	2.034 ng/ml
6) t Toluene	11.053	227788	6.089 ng/ml
7) t Ethylbenzene	13.460	74801	2.066 ng/ml
8) t m-Xylene	13.590	147681	4.061 ng/ml
9) t O-Xylene	14.313	131933	3.822 ng/ml
10) t 1,2,4-Trimethylbenzene	16.568	109237	3.845 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB051021\
Data File : FB025745.D
Signal(s) : FID2B.CH
Acq On : 10 May 2021 15:01
Operator : DD/AJ
Sample : M2262-01
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 9 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: May 11 01:12:12 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB050521.M
Quant Title :
QLast Update : Thu May 06 15:01:51 2021
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

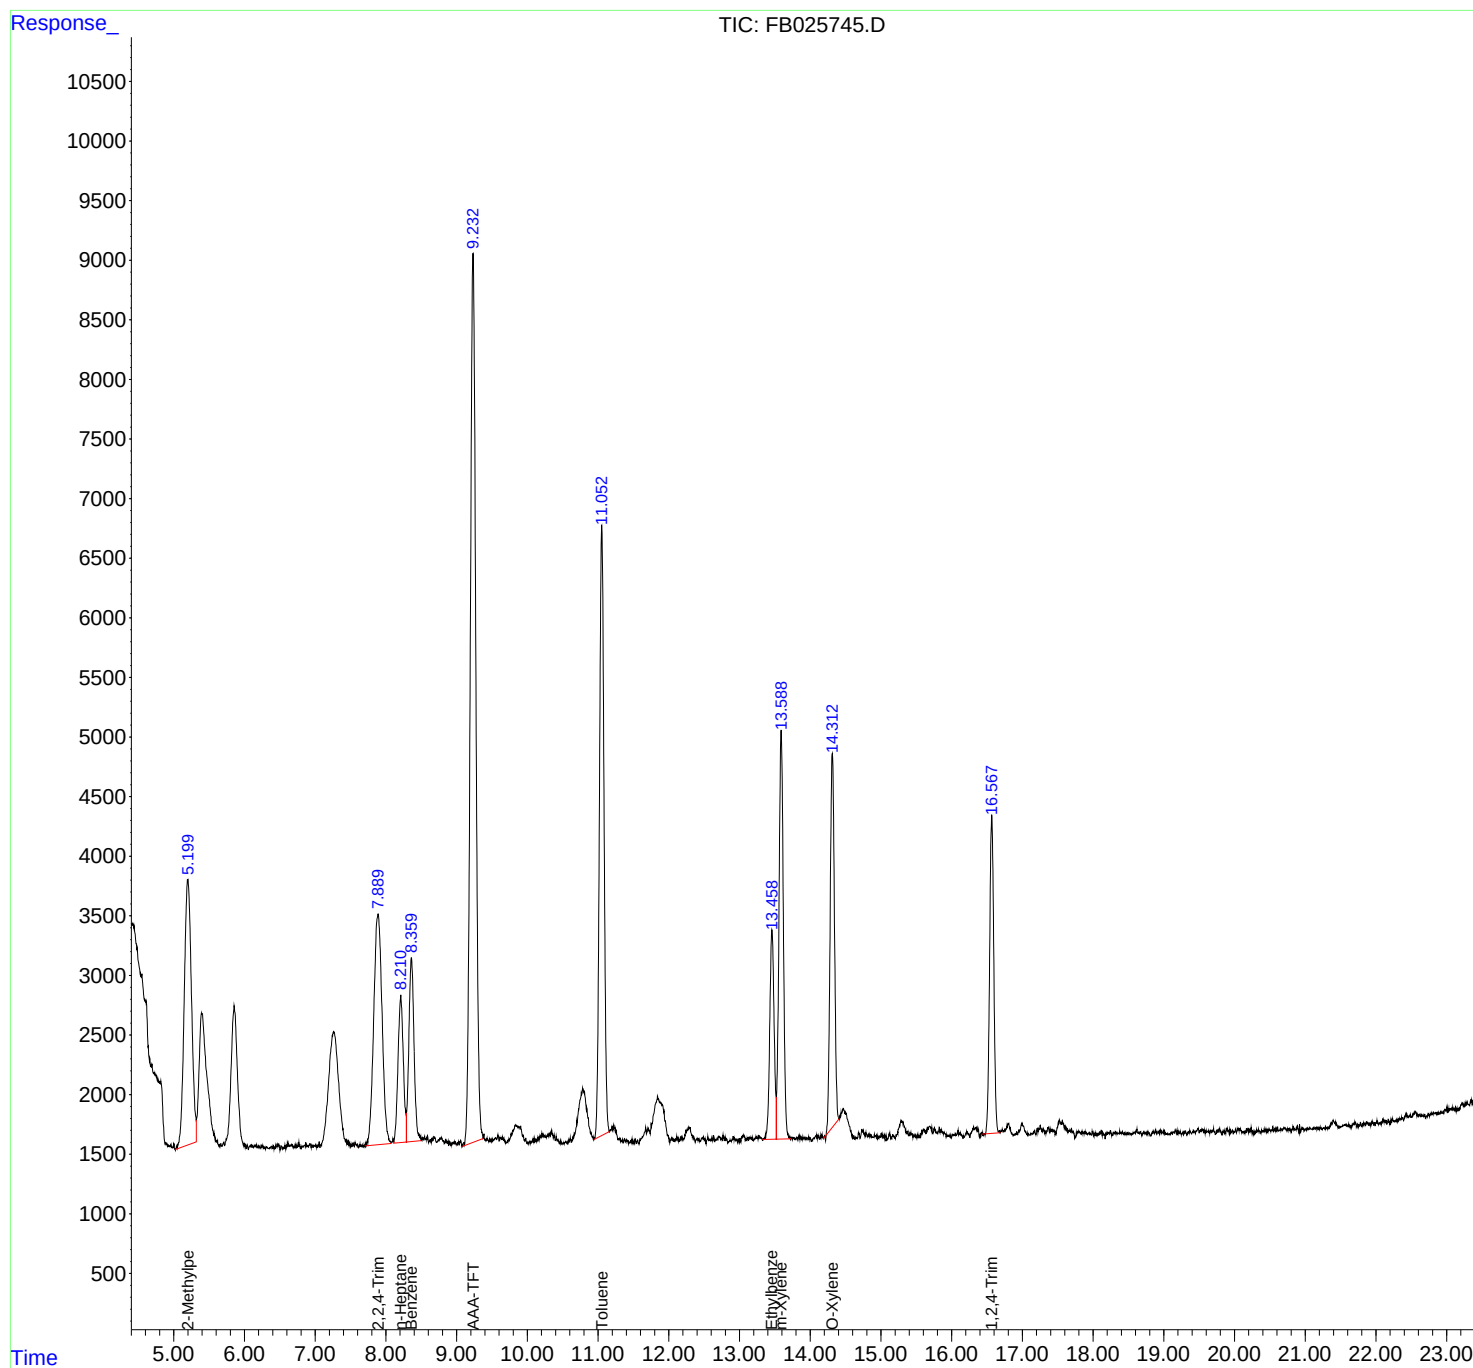

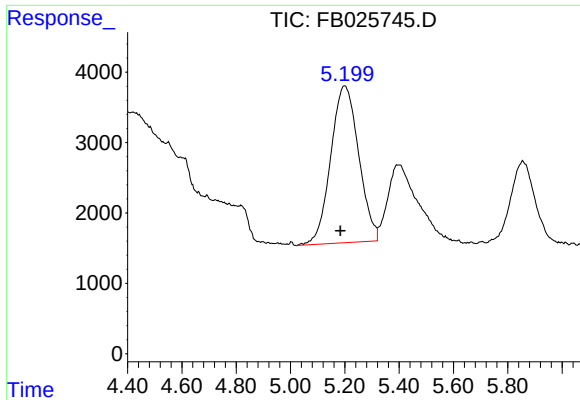


#1 2-Methylpentane

R.T.: 5.201 min
Delta R.T.: 0.018 min
Response: 158979
Conc: 6.33 ng/ml

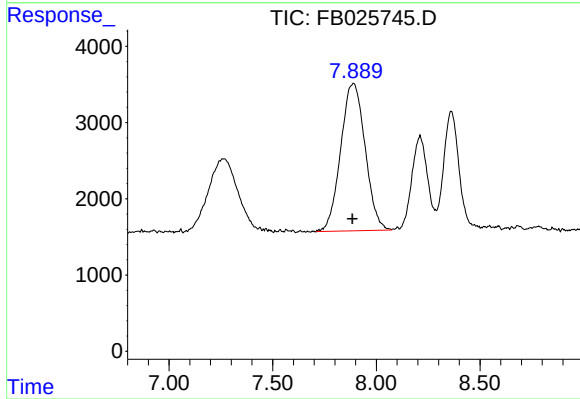


#2 2,2,4-Trimethylpentane

R.T.: 7.891 min
Delta R.T.: 0.007 min
Response: 157985
Conc: 7.34 ng/ml

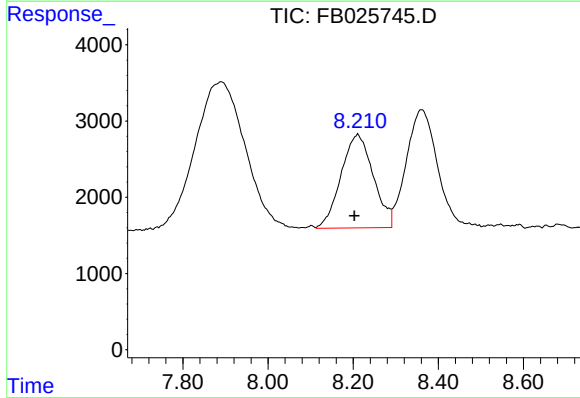


#3 n-Heptane

R.T.: 8.211 min
Delta R.T.: 0.009 min
Response: 64523
Conc: 2.13 ng/ml

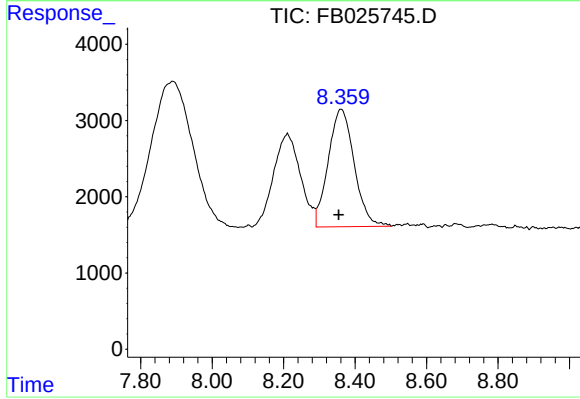


#4 Benzene

R.T.: 8.361 min
Delta R.T.: 0.007 min
Response: 77806
Conc: 2.03 ng/ml

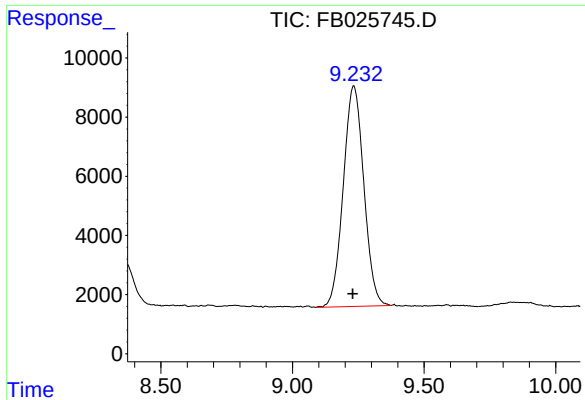


#5 AAA-TFT

R.T.: 9.233 min
Delta R.T.: 0.004 min
Response: 404768
Conc: 18.86 ng/ml

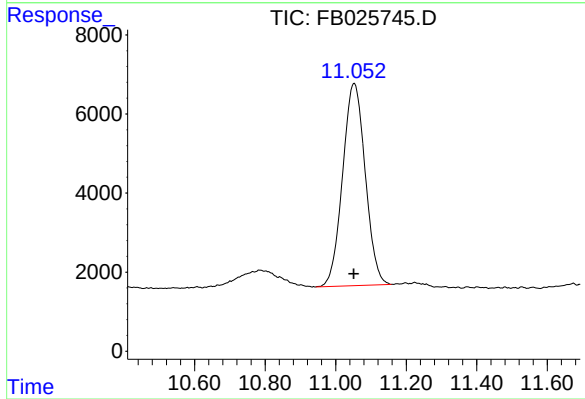


#6 Toluene

R.T.: 11.053 min
Delta R.T.: 0.002 min
Response: 227788
Conc: 6.09 ng/ml

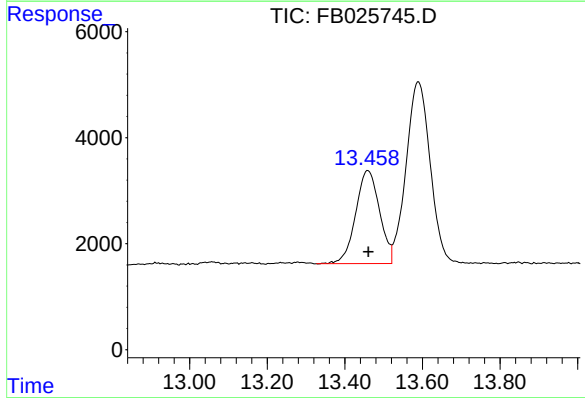


#7 Ethylbenzene

R.T.: 13.460 min
Delta R.T.: 0.000 min
Response: 74801
Conc: 2.07 ng/ml

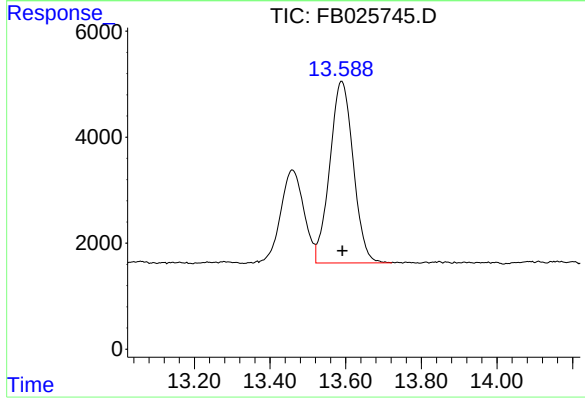


#8 m-Xylene

R.T.: 13.590 min
Delta R.T.: -0.001 min
Response: 147681
Conc: 4.06 ng/ml

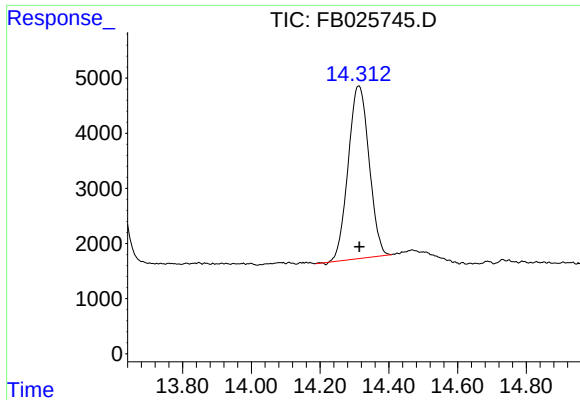

#9 O-Xylene

R.T.: 14.313 min
Delta R.T.: -0.001 min
Response: 131933
Conc: 3.82 ng/ml

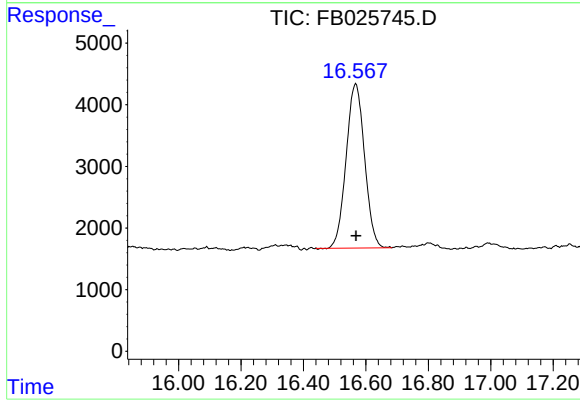

#10 1,2,4-Trimethylbenzene

R.T.: 16.568 min
Delta R.T.: 0.000 min
Response: 109237
Conc: 3.84 ng/ml