

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB051022\
 Data File : FB027135.D
 Signal(s) : FID2B.CH
 Acq On : 10 May 2022 12:36
 Operator : AJ/MA
 Sample : 50 GRO STD
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 50 GRO STD

Integration File: Calibration.e
 Quant Time: May 10 13:28:05 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051022.M
 Quant Title :
 QLast Update : Tue May 10 13:26:50 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.787	537431	53.965 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.703	1295547	79.162 ng/ml
2) t 2,2,4-Trimethylpentane	7.419	1345185	79.881 ng/ml
3) t n-Heptane	7.746	457098	26.939 ng/ml
4) t Benzene	7.882	526075	28.146 ng/ml
6) t Toluene	10.614	1481977	81.853 ng/ml
7) t Ethylbenzene	13.051	454063	27.077 ng/ml
8) t m-Xylene	13.184	901908	53.923 ng/ml
9) t O-Xylene	13.911	883845	53.286 ng/ml
10) t 1,2,4-Trimethylbenzene	16.186	888796	52.558 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB051022\
Data File : FB027135.D
Signal(s) : FID2B.CH
Acq On : 10 May 2022 12:36
Operator : AJ/MA
Sample : 50 GRO STD
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
50 GRO STD

Integration File: Calibration.e
Quant Time: May 10 13:28:05 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051022.M
Quant Title :
QLast Update : Tue May 10 13:26:50 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

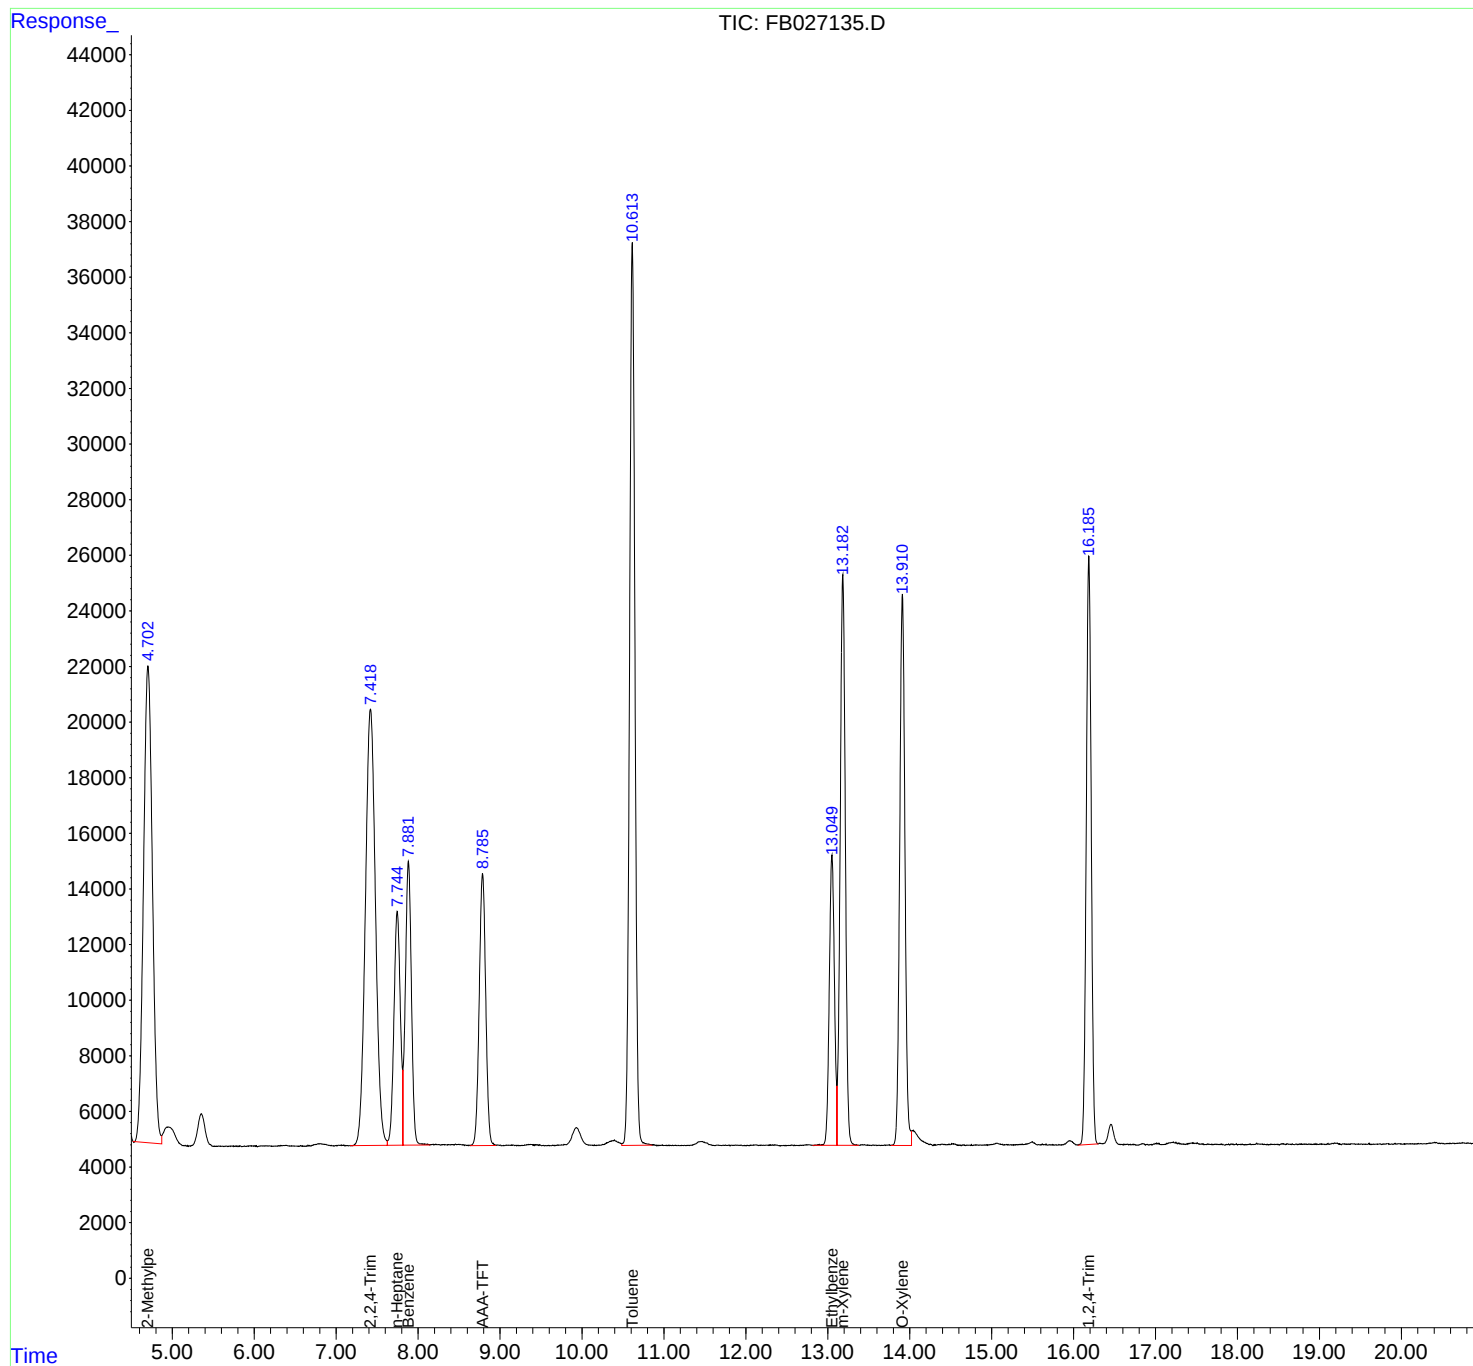


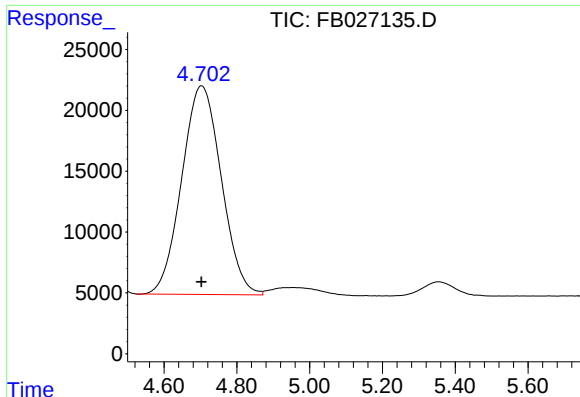

#1 2-Methylpentane


R.T.: 4.703 min
Delta R.T.: 0.000 min
Response: 1295547
Conc: 79.16 ng/ml

Instrument :
FID_B
ClientSampleId :
50 GRO STD

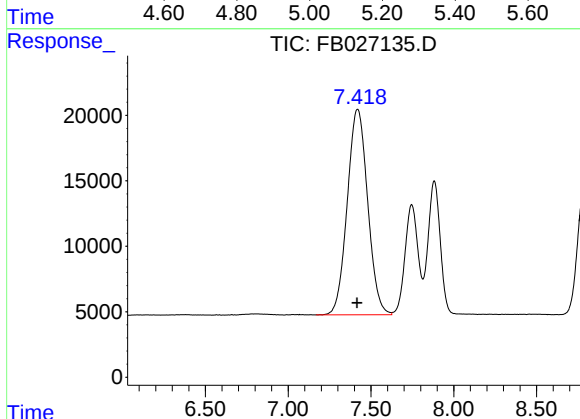


#2 2,2,4-Trimethylpentane

R.T.: 7.419 min
Delta R.T.: 0.004 min
Response: 1345185
Conc: 79.88 ng/ml

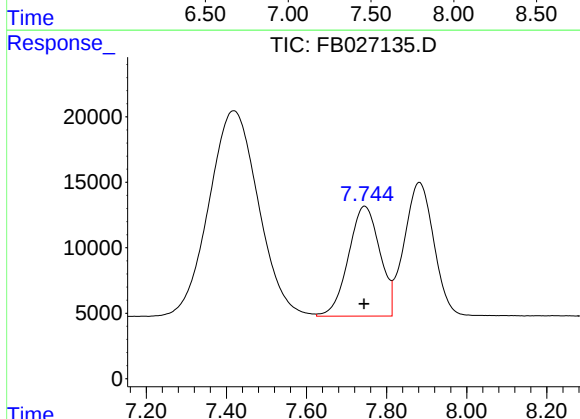


#3 n-Heptane

R.T.: 7.746 min
Delta R.T.: 0.002 min
Response: 457098
Conc: 26.94 ng/ml

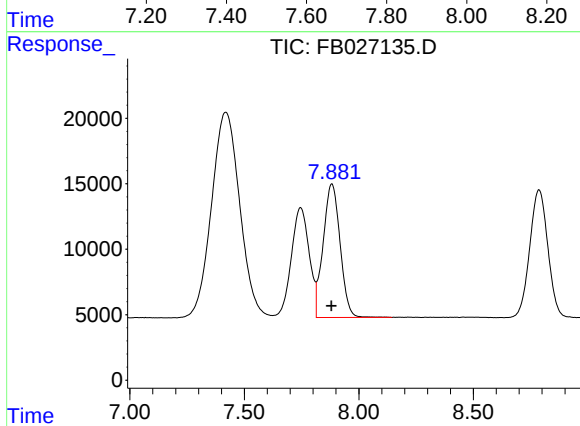

#4 Benzene


R.T.: 7.882 min
Delta R.T.: 0.002 min
Response: 526075
Conc: 28.15 ng/ml

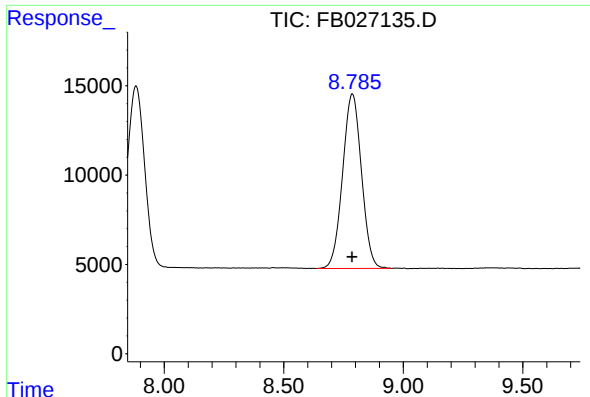

#5 AAA-TFT


R.T.: 8.787 min
Delta R.T.: 0.000 min
Response: 537431
Conc: 53.97 ng/ml

Instrument :
FID_B
ClientSampleId :
50 GRO STD

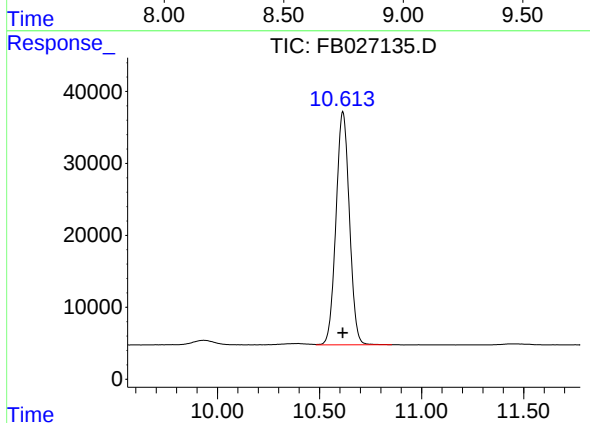


#6 Toluene

R.T.: 10.614 min
Delta R.T.: 0.000 min
Response: 1481977
Conc: 81.85 ng/ml

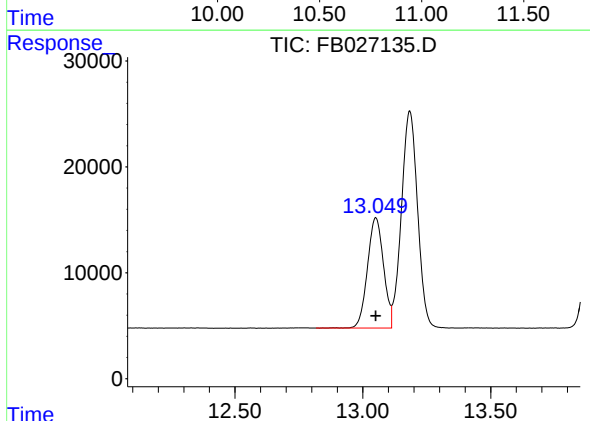


#7 Ethylbenzene

R.T.: 13.051 min
Delta R.T.: 0.000 min
Response: 454063
Conc: 27.08 ng/ml

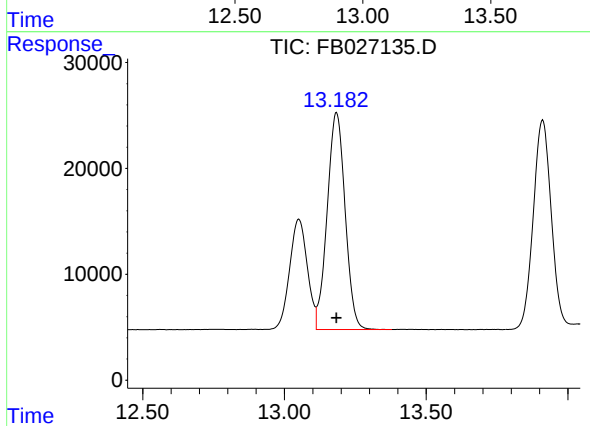

#8 m-Xylene


R.T.: 13.184 min
Delta R.T.: 0.000 min
Response: 901908
Conc: 53.92 ng/ml

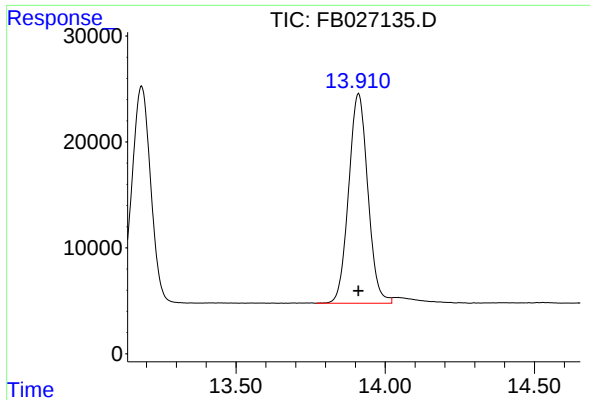

#9 O-Xylene

R.T.: 13.911 min
Delta R.T.: 0.000 min
Response: 883845
Conc: 53.29 ng/ml

Instrument :
FID_B
ClientSampleId :
50 GRO STD

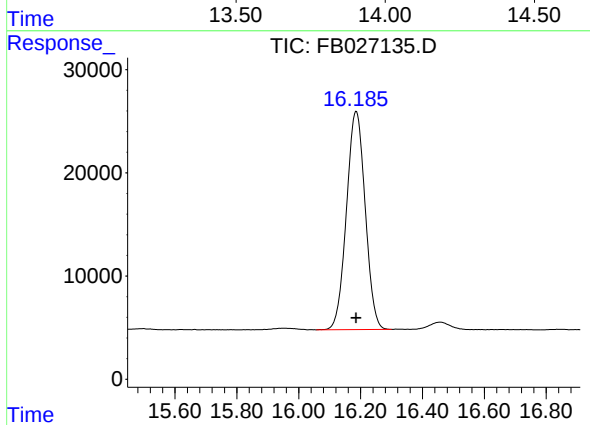

#10 1,2,4-Trimethylbenzene

R.T.: 16.186 min
Delta R.T.: 0.000 min
Response: 888796
Conc: 52.56 ng/ml