

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB051120\
 Data File : FB024312.D
 Signal(s) : FID2B.CH
 Acq On : 11 May 2020 13:10
 Operator : DD/AJ
 Sample : BSF0511S1
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 10 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: May 12 02:20:36 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051120.M
 Quant Title :
 QLast Update : Mon May 11 11:14:42 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.800	470637	21.313 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.691	951790	32.253 ng/ml
2) t 2,2,4-Trimethylpentane	7.419	1016203	33.264 ng/ml
3) t n-Heptane	7.759	334470	11.040 ng/ml
4) t Benzene	7.893	394241	10.428 ng/ml
6) t Toluene	10.632	1130432	31.196 ng/ml
7) t Ethylbenzene	13.072	349829	10.319 ng/ml
8) t m-Xylene	13.205	679505	20.591 ng/ml
9) t O-Xylene	13.933	664700	20.598 ng/ml
10) t 1,2,4-Trimethylbenzene	16.210	561363	20.815 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB051120\
Data File : FB024312.D
Signal(s) : FID2B.CH
Acq On : 11 May 2020 13:10
Operator : DD/AJ
Sample : BSF0511S1
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 10 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: May 12 02:20:36 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051120.M
Quant Title :
QLast Update : Mon May 11 11:14:42 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

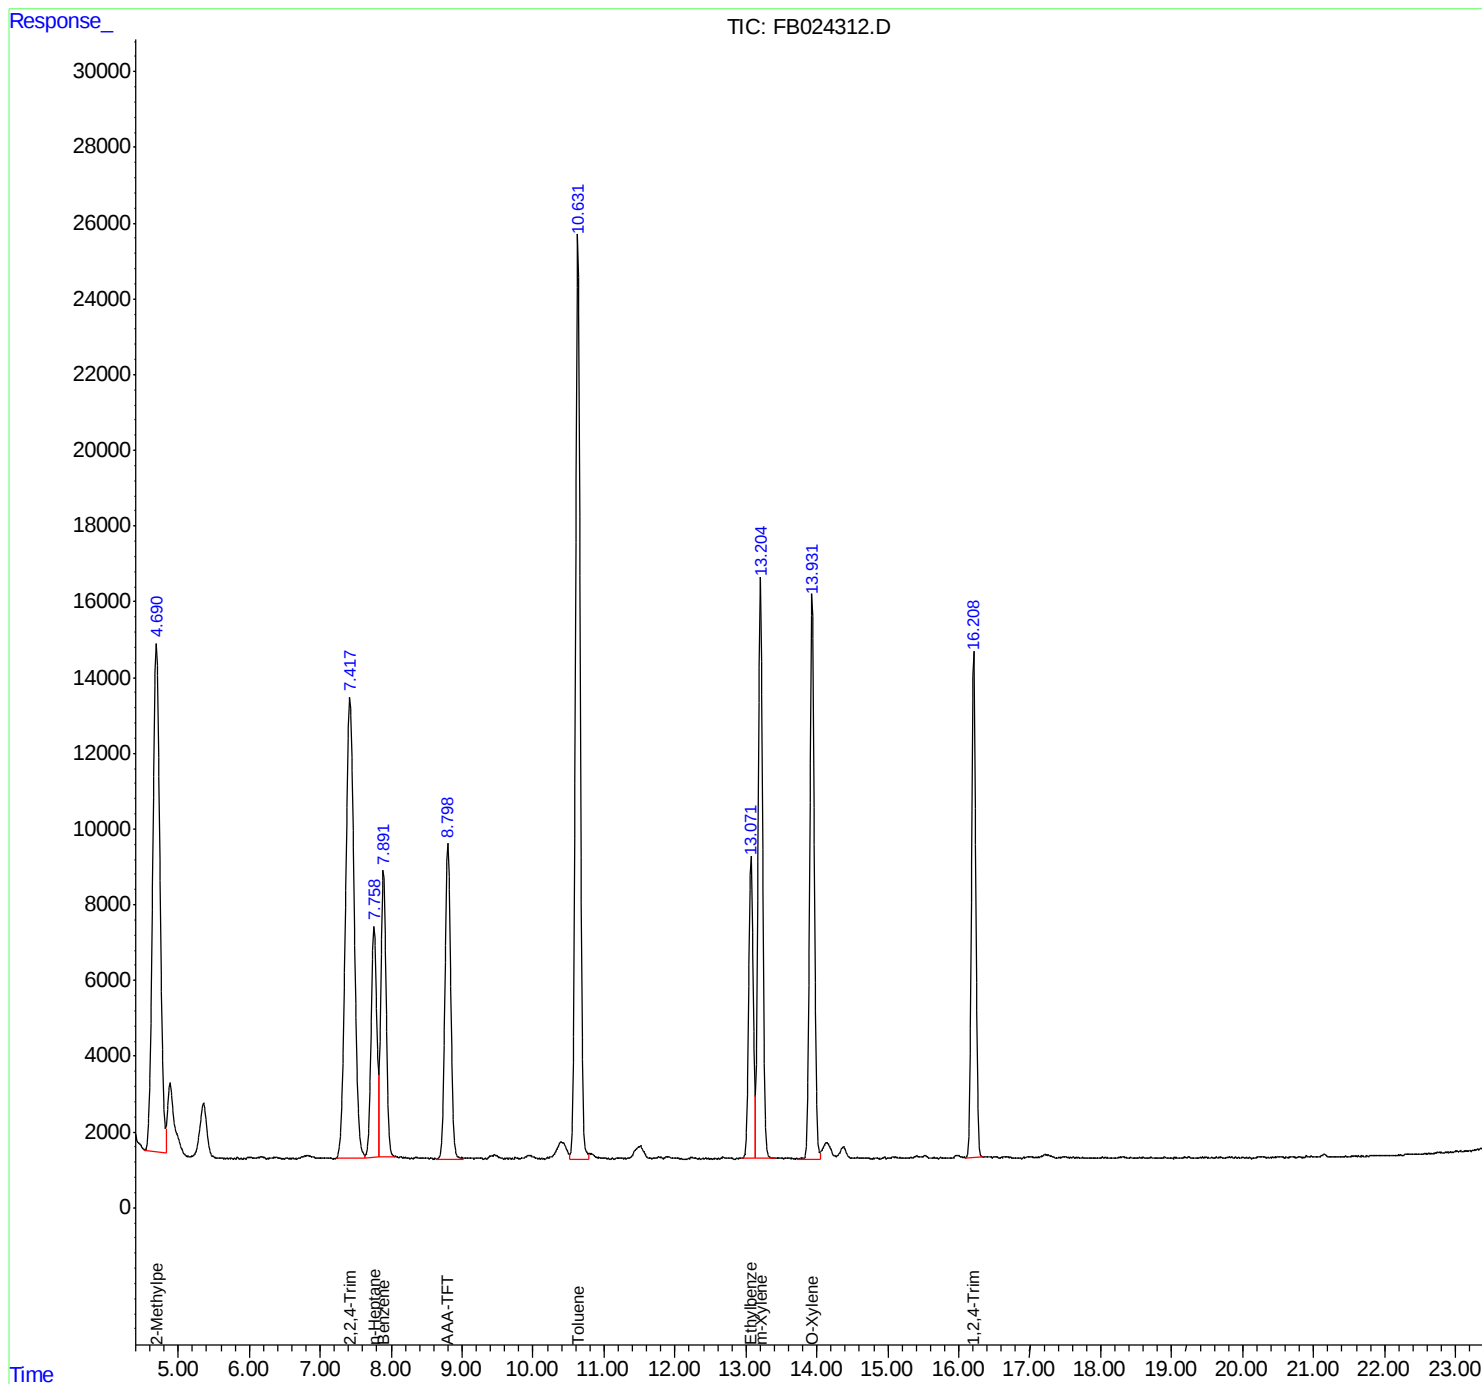

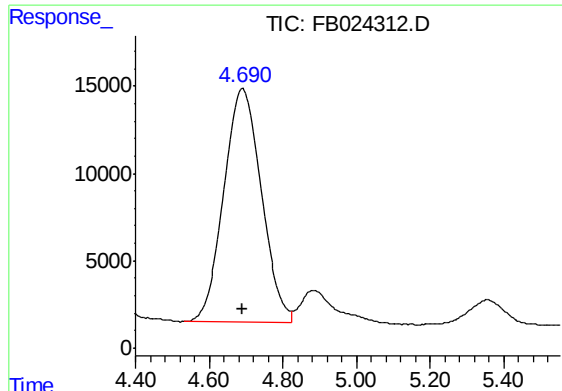


#1 2-Methylpentane

R.T.: 4.691 min
Delta R.T.: 0.002 min
Response: 951790
Conc: 32.25 ng/ml

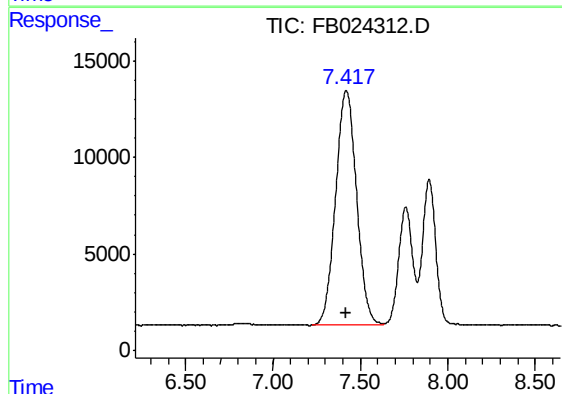


#2 2,2,4-Trimethylpentane

R.T.: 7.419 min
Delta R.T.: 0.002 min
Response: 1016203
Conc: 33.26 ng/ml

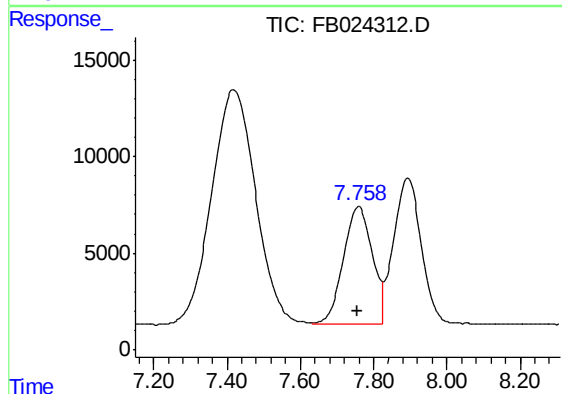


#3 n-Heptane

R.T.: 7.759 min
Delta R.T.: 0.001 min
Response: 334470
Conc: 11.04 ng/ml

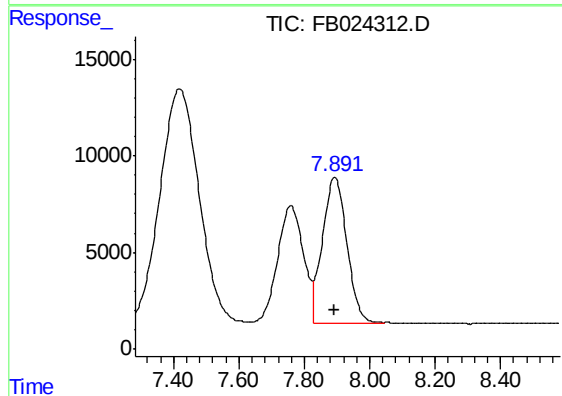


#4 Benzene

R.T.: 7.893 min
Delta R.T.: 0.000 min
Response: 394241
Conc: 10.43 ng/ml

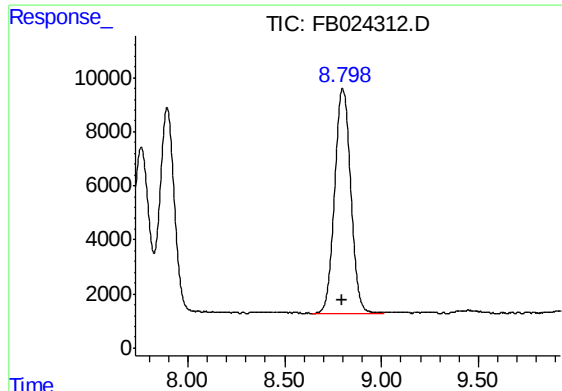


#5 AAA-TFT

R.T.: 8.800 min
Delta R.T.: 0.000 min
Response: 470637
Conc: 21.31 ng/ml

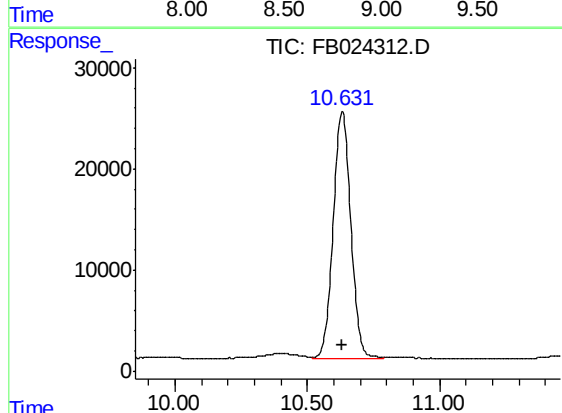


#6 Toluene

R.T.: 10.632 min
Delta R.T.: 0.001 min
Response: 1130432
Conc: 31.20 ng/ml

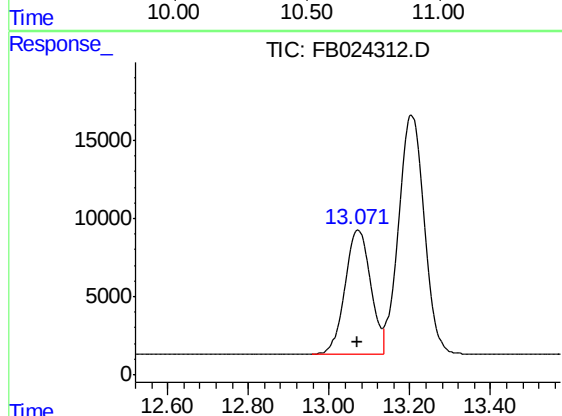


#7 Ethylbenzene

R.T.: 13.072 min
Delta R.T.: 0.001 min
Response: 349829
Conc: 10.32 ng/ml

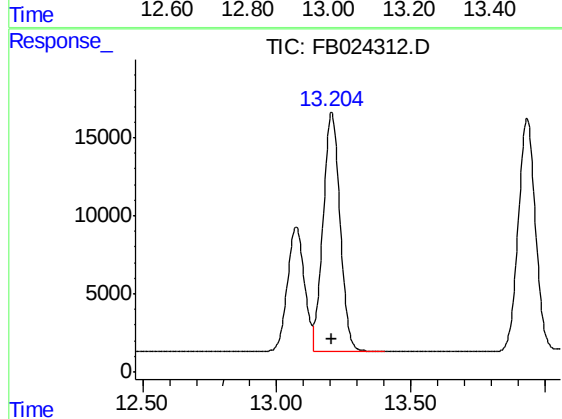


#8 m-Xylene

R.T.: 13.205 min
Delta R.T.: 0.000 min
Response: 679505
Conc: 20.59 ng/ml

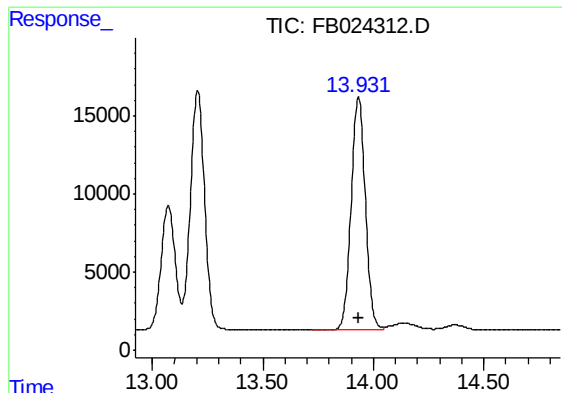

#9 O-Xylene

R.T.: 13.933 min
Delta R.T.: 0.000 min
Response: 664700
Conc: 20.60 ng/ml

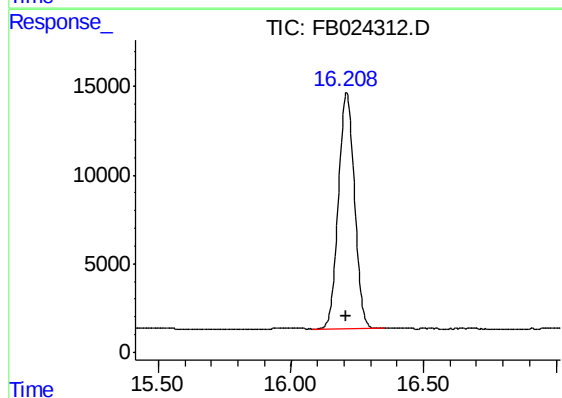

#10 1,2,4-Trimethylbenzene

R.T.: 16.210 min
Delta R.T.: 0.000 min
Response: 561363
Conc: 20.81 ng/ml