

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB051121\
 Data File : FB025757.D
 Signal(s) : FID2B.CH
 Acq On : 11 May 2021 14:26
 Operator : DD/AJ
 Sample : M2262-03
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 8 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: May 12 01:11:11 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB050521.M
 Quant Title :
 QLast Update : Thu May 06 15:01:51 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.231	378728	17.645 ng/ml
Target Compounds			
1) t 2-Methylpentane	5.190	40119	1.598 ng/ml
2) t 2,2,4-Trimethylpentane	7.893	35476	1.648 ng/ml
3) t n-Heptane	8.204	18817	0.622 ng/mlm
4) t Benzene	8.368	22856	0.598 ng/mlm
6) t Toluene	11.051	55597	1.486 ng/ml
7) t Ethylbenzene	13.460	18963	0.524 ng/ml
8) t m-Xylene	13.589	37204	1.023 ng/ml
9) t O-Xylene	14.311	36944	1.070 ng/mlm
10) t 1,2,4-Trimethylbenzene	16.568	26637	0.938 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB051121\
Data File : FB025757.D
Signal(s) : FID2B.CH
Acq On : 11 May 2021 14:26
Operator : DD/AJ
Sample : M2262-03
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 8 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: May 12 01:11:11 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB050521.M
Quant Title :
QLast Update : Thu May 06 15:01:51 2021
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

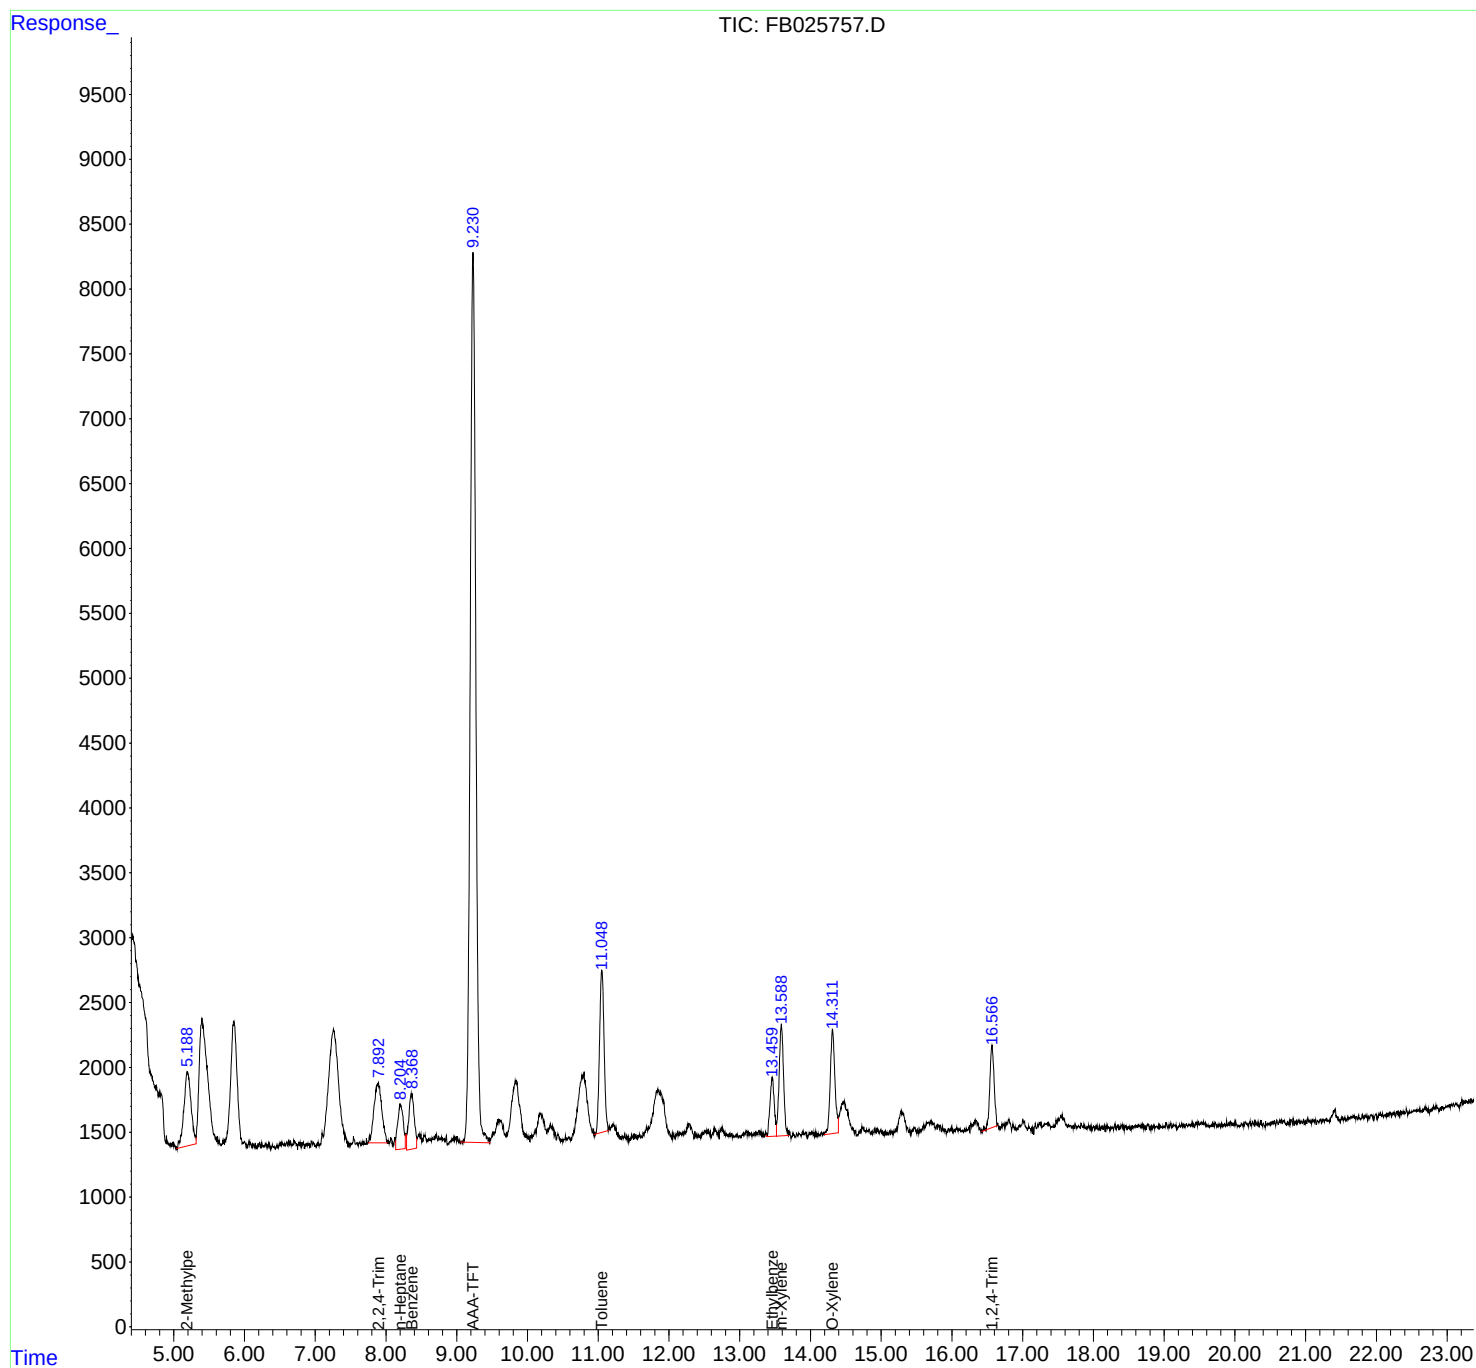

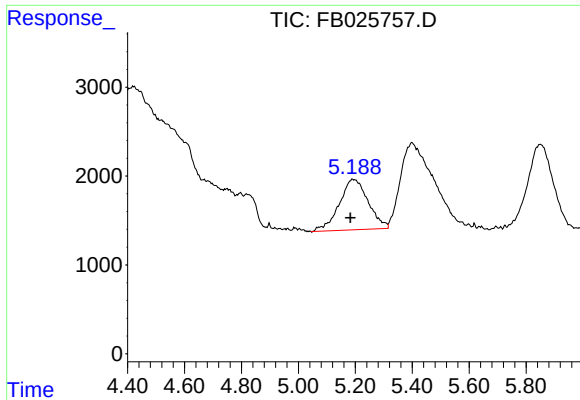


#1 2-Methylpentane

R.T.: 5.190 min
Delta R.T.: 0.007 min
Response: 40119
Conc: 1.60 ng/ml

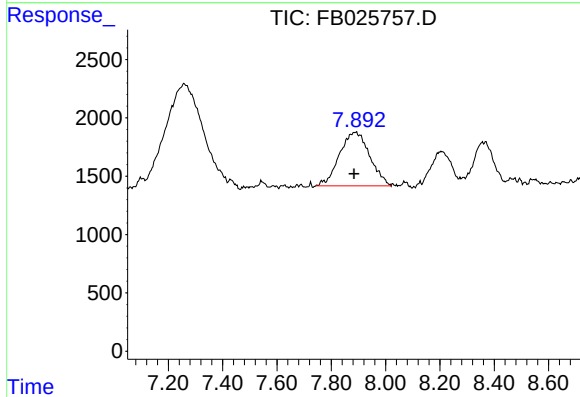


#2 2,2,4-Trimethylpentane

R.T.: 7.893 min
Delta R.T.: 0.009 min
Response: 35476
Conc: 1.65 ng/ml

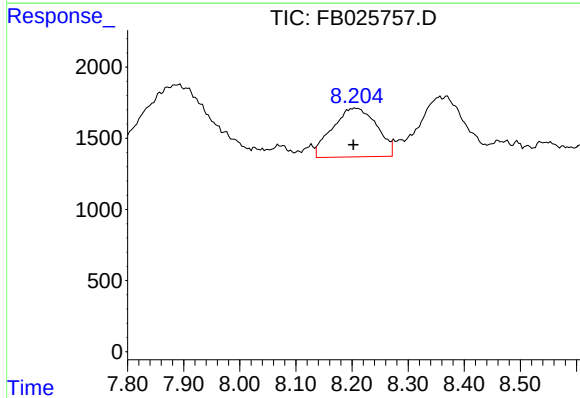


#3 n-Heptane

R.T.: 8.204 min
Delta R.T.: 0.000 min
Response: 18817
Conc: 0.62 ng/ml m

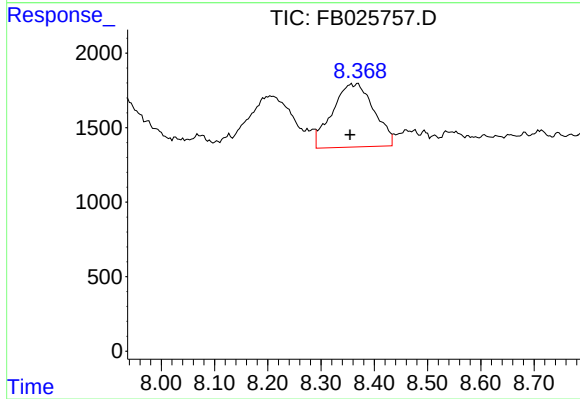


#4 Benzene

R.T.: 8.368 min
Delta R.T.: 0.014 min
Response: 22856
Conc: 0.60 ng/ml m

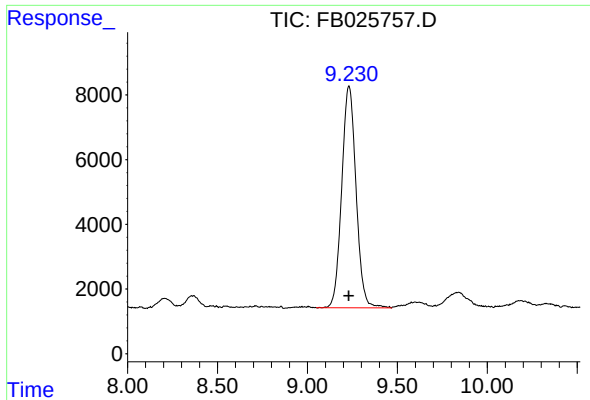


#5 AAA-TFT

R.T.: 9.231 min
Delta R.T.: 0.002 min
Response: 378728
Conc: 17.64 ng/ml

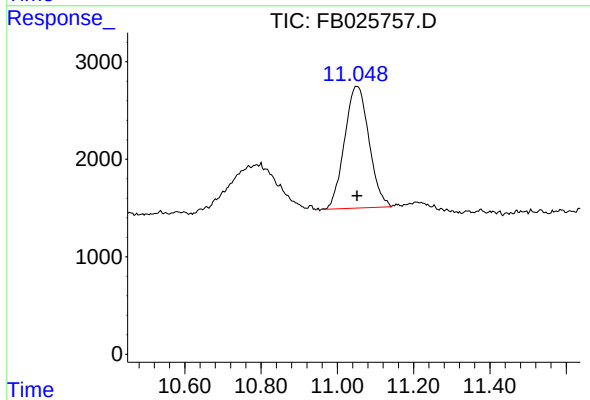


#6 Toluene

R.T.: 11.051 min
Delta R.T.: 0.000 min
Response: 55597
Conc: 1.49 ng/ml

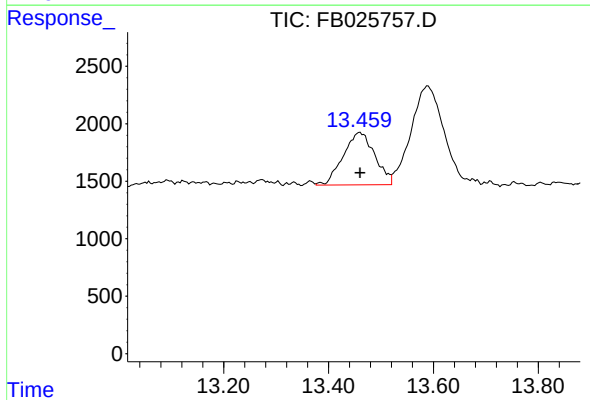


#7 Ethylbenzene

R.T.: 13.460 min
Delta R.T.: 0.000 min
Response: 18963
Conc: 0.52 ng/ml

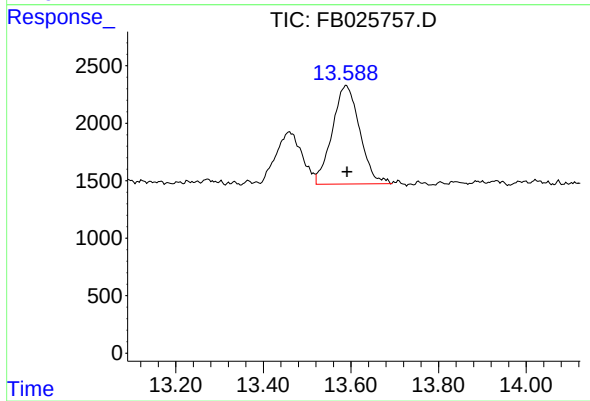

#8 m-Xylene

R.T.: 13.589 min
Delta R.T.: -0.002 min
Response: 37204
Conc: 1.02 ng/ml

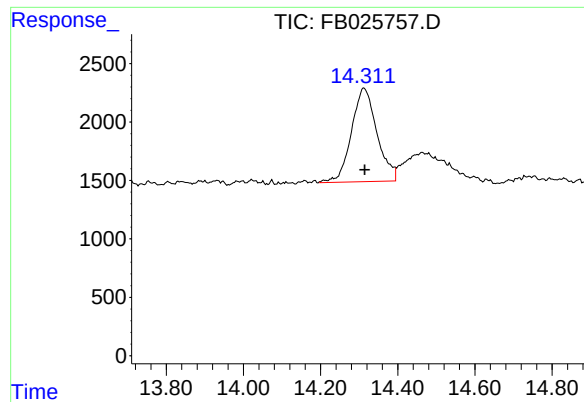


#9 O-Xylene

R.T.: 14.311 min

Delta R.T.: -0.004 min

Response: 36944

Conc: 1.07 ng/ml m

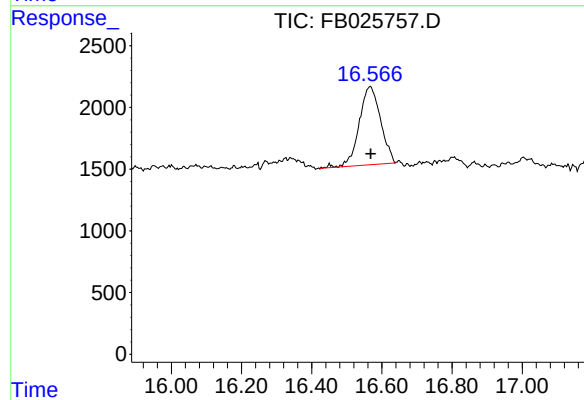

#10 1,2,4-Trimethylbenzene

R.T.: 16.568 min

Delta R.T.: 0.000 min

Response: 26637

Conc: 0.94 ng/ml