

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB051220\
 Data File : FB024324.D
 Signal(s) : FID2B.CH
 Acq On : 12 May 2020 8:00
 Operator : DD/AJ
 Sample : BSF0512S1
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0512S1

Integration File: Calibration.e
 Quant Time: May 13 02:45:58 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051120.M
 Quant Title :
 QLast Update : Mon May 11 11:14:42 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.799	453492	20.537 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.690	923918	31.309 ng/ml
2) t 2,2,4-Trimethylpentane	7.418	1001949	32.798 ng/ml
3) t n-Heptane	7.758	329784	10.886 ng/ml
4) t Benzene	7.893	391814	10.364 ng/ml
6) t Toluene	10.630	1113839	30.738 ng/ml
7) t Ethylbenzene	13.070	347168	10.240 ng/ml
8) t m-Xylene	13.203	672772	20.387 ng/ml
9) t O-Xylene	13.931	657908	20.388 ng/ml
10) t 1,2,4-Trimethylbenzene	16.209	550649	20.417 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB051220\
Data File : FB024324.D
Signal(s) : FID2B.CH
Acq On : 12 May 2020 8:00
Operator : DD/AJ
Sample : BSF0512S1
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0512S1

Integration File: Calibration.e
Quant Time: May 13 02:45:58 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051120.M
Quant Title :
QLast Update : Mon May 11 11:14:42 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

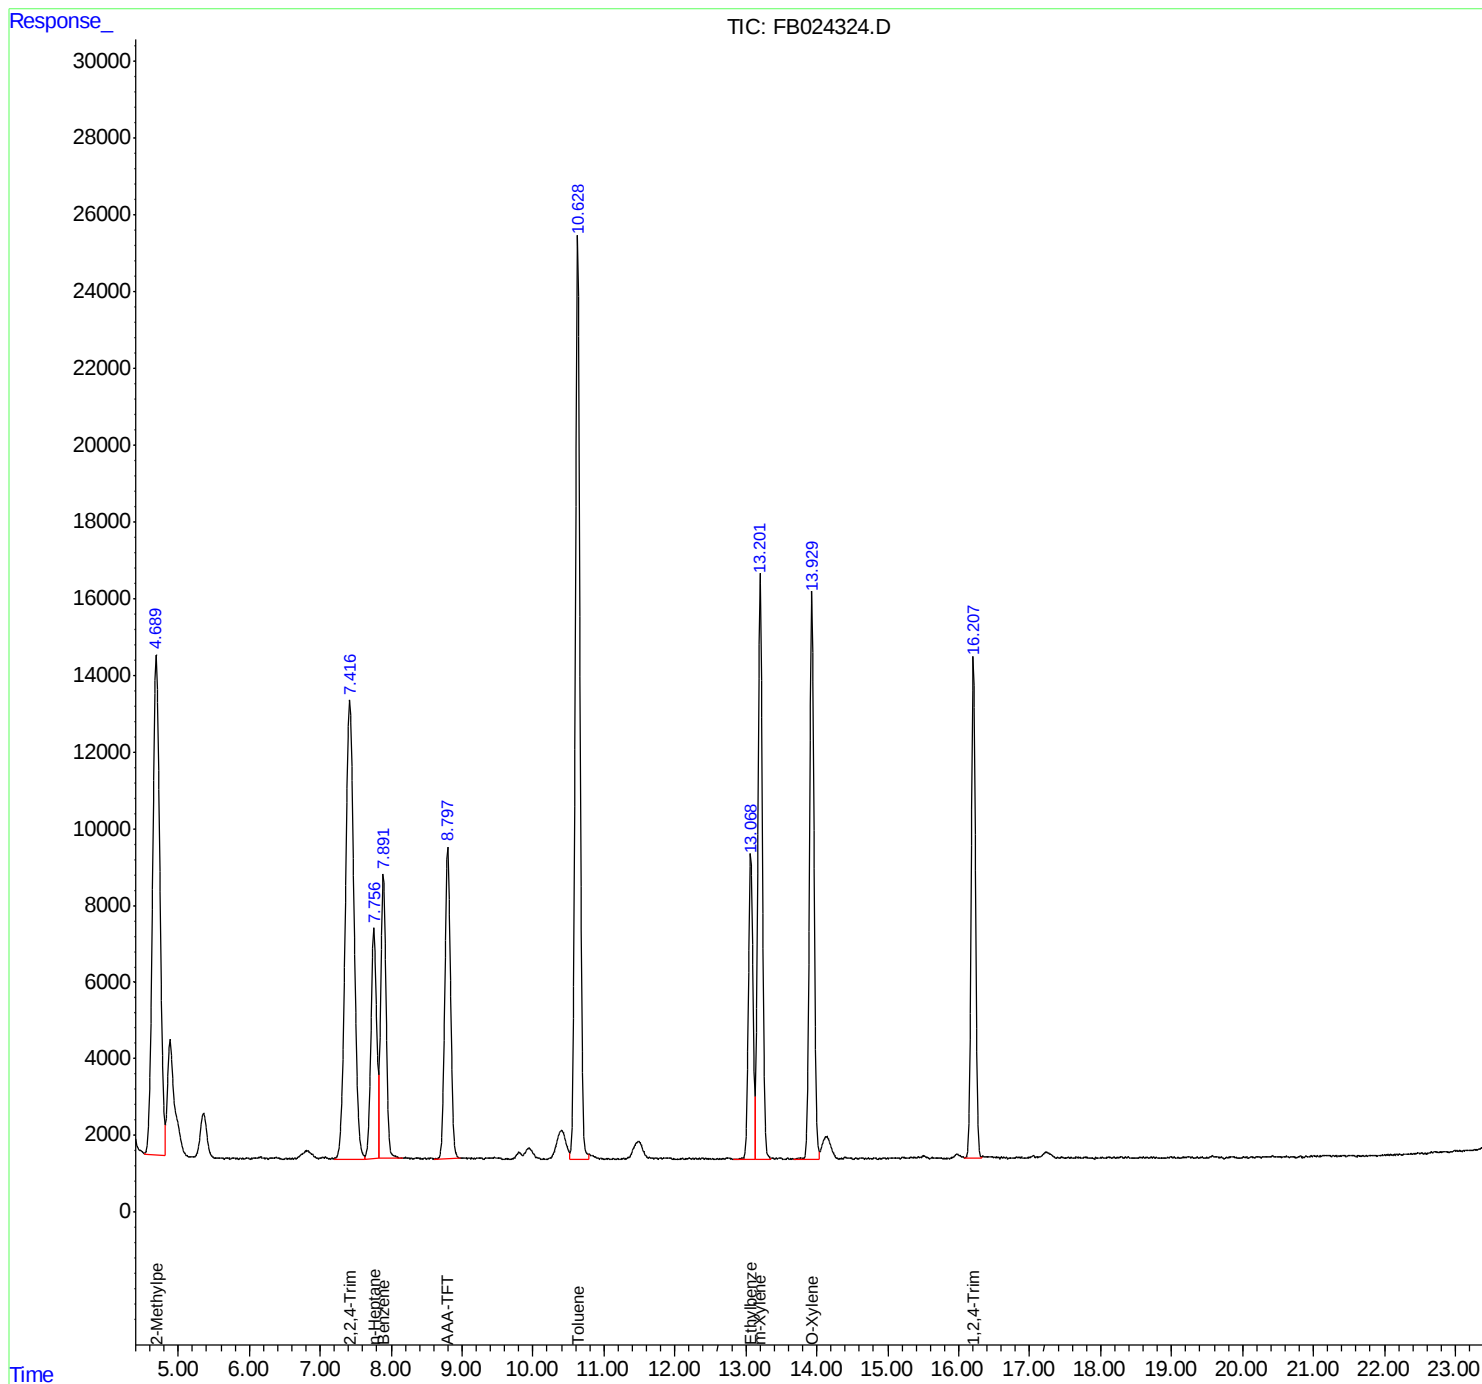


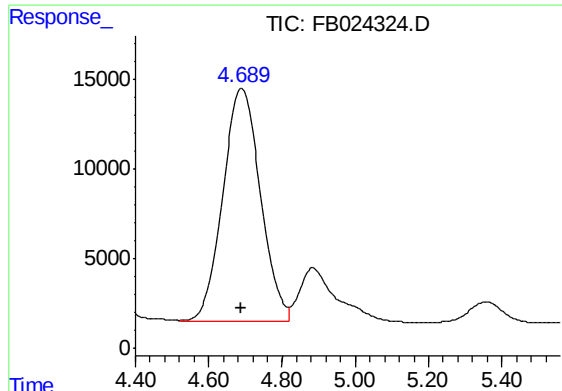

#1 2-Methylpentane


R.T.: 4.690 min
Delta R.T.: 0.001 min
Response: 923918
Conc: 31.31 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0512S1

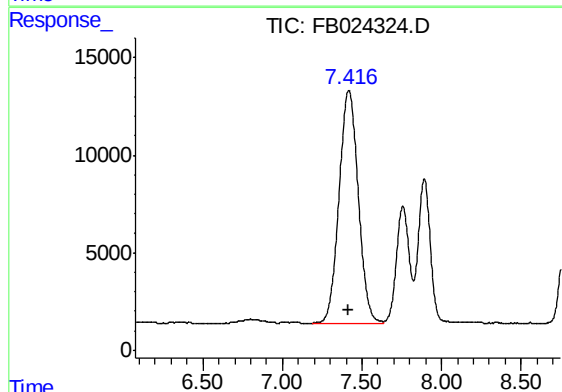


#2 2,2,4-Trimethylpentane

R.T.: 7.418 min
Delta R.T.: 0.000 min
Response: 1001949
Conc: 32.80 ng/ml

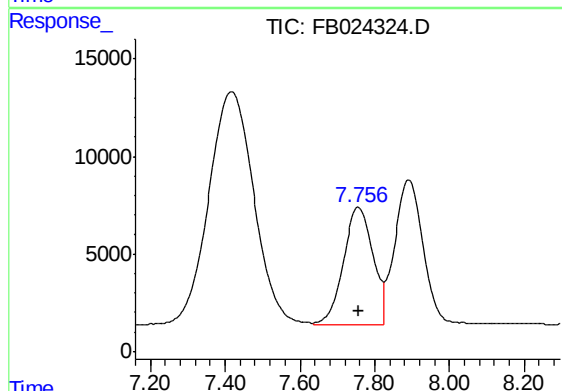


#3 n-Heptane

R.T.: 7.758 min
Delta R.T.: 0.000 min
Response: 329784
Conc: 10.89 ng/ml

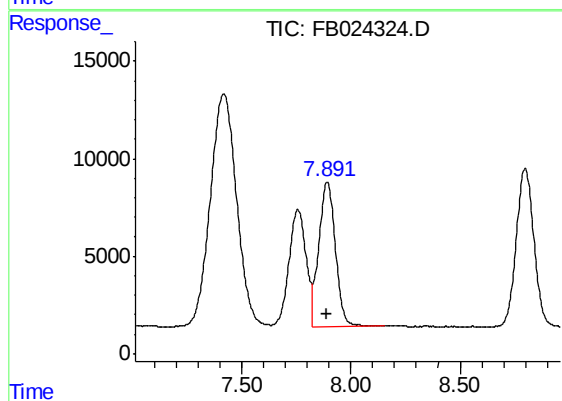

#4 Benzene


R.T.: 7.893 min
Delta R.T.: 0.000 min
Response: 391814
Conc: 10.36 ng/ml

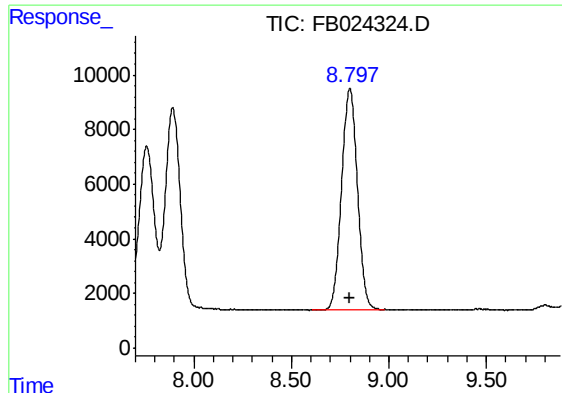

#5 AAA-TFT


R.T.: 8.799 min
Delta R.T.: 0.000 min
Response: 453492
Conc: 20.54 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0512S1

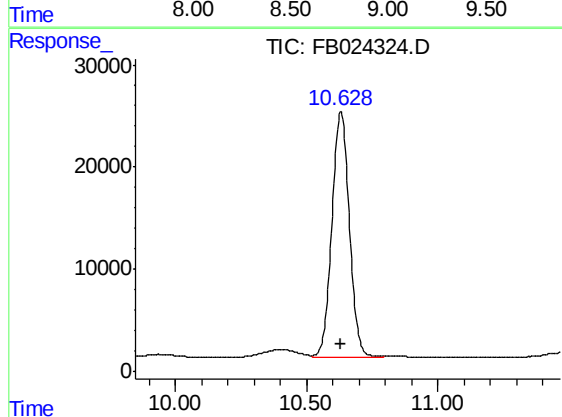


#6 Toluene

R.T.: 10.630 min
Delta R.T.: 0.000 min
Response: 1113839
Conc: 30.74 ng/ml

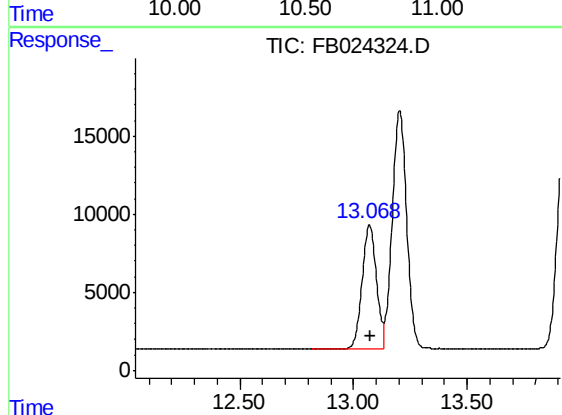


#7 Ethylbenzene

R.T.: 13.070 min
Delta R.T.: -0.002 min
Response: 347168
Conc: 10.24 ng/ml

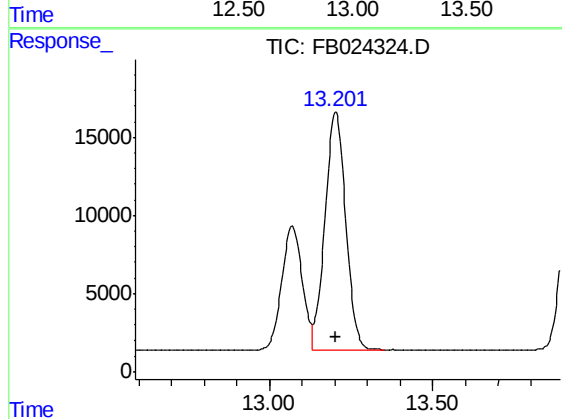

#8 m-Xylene


R.T.: 13.203 min
Delta R.T.: -0.001 min
Response: 672772
Conc: 20.39 ng/ml

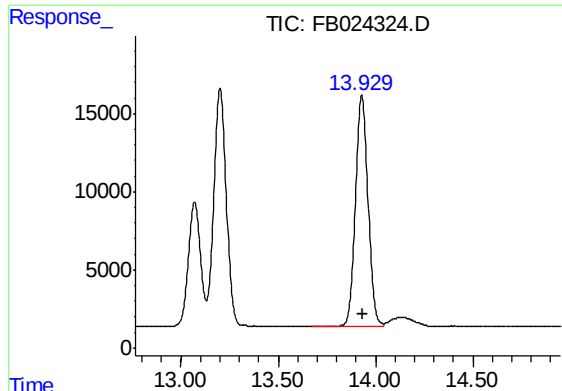

#9 O-Xylene

R.T.: 13.931 min
Delta R.T.: -0.001 min
Response: 657908
Conc: 20.39 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0512S1

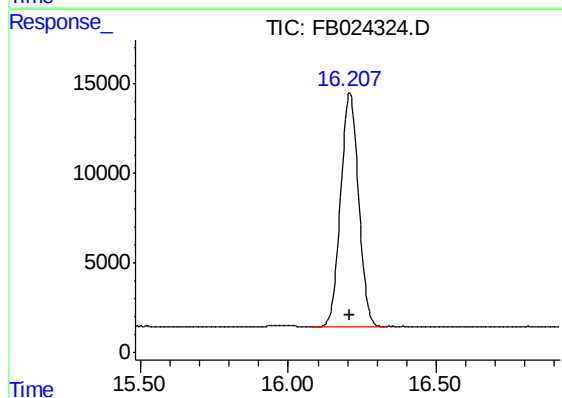

#10 1,2,4-Trimethylbenzene

R.T.: 16.209 min
Delta R.T.: -0.001 min
Response: 550649
Conc: 20.42 ng/ml