

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB0511220\
 Data File : FB024332.D
 Signal(s) : FID2B.CH
 Acq On : 12 May 2020 15:19
 Operator : DD/AJ
 Sample : L2502-01
 Misc : 5.00g/5.00ml DI WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 PL-01-050820

Integration File: Calibration.e
 Quant Time: May 13 02:47:30 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051120.M
 Quant Title :
 QLast Update : Mon May 11 11:14:42 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.800	442577	20.043 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.684	4134	0.140 ng/ml
2) t 2,2,4-Trimethylpentane	7.417	2347	0.077 ng/ml
6) t Toluene	10.630	28879	0.797 ng/ml
7) t Ethylbenzene	13.030	95237	2.809 ng/ml
8) t m-Xylene	13.201	19514	0.591 ng/ml
9) t o-Xylene	13.928	8370	0.259 ng/ml
10) t 1,2,4-Trimethylbenzene	16.218	54254	2.012 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB051220\
Data File : FB024332.D
Signal(s) : FID2B.CH
Acq On : 12 May 2020 15:19
Operator : DD/AJ
Sample : L2502-01
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
PL-01-050820

Integration File: Calibration.e
Quant Time: May 13 02:47:30 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051120.M
Quant Title :
QLast Update : Mon May 11 11:14:42 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

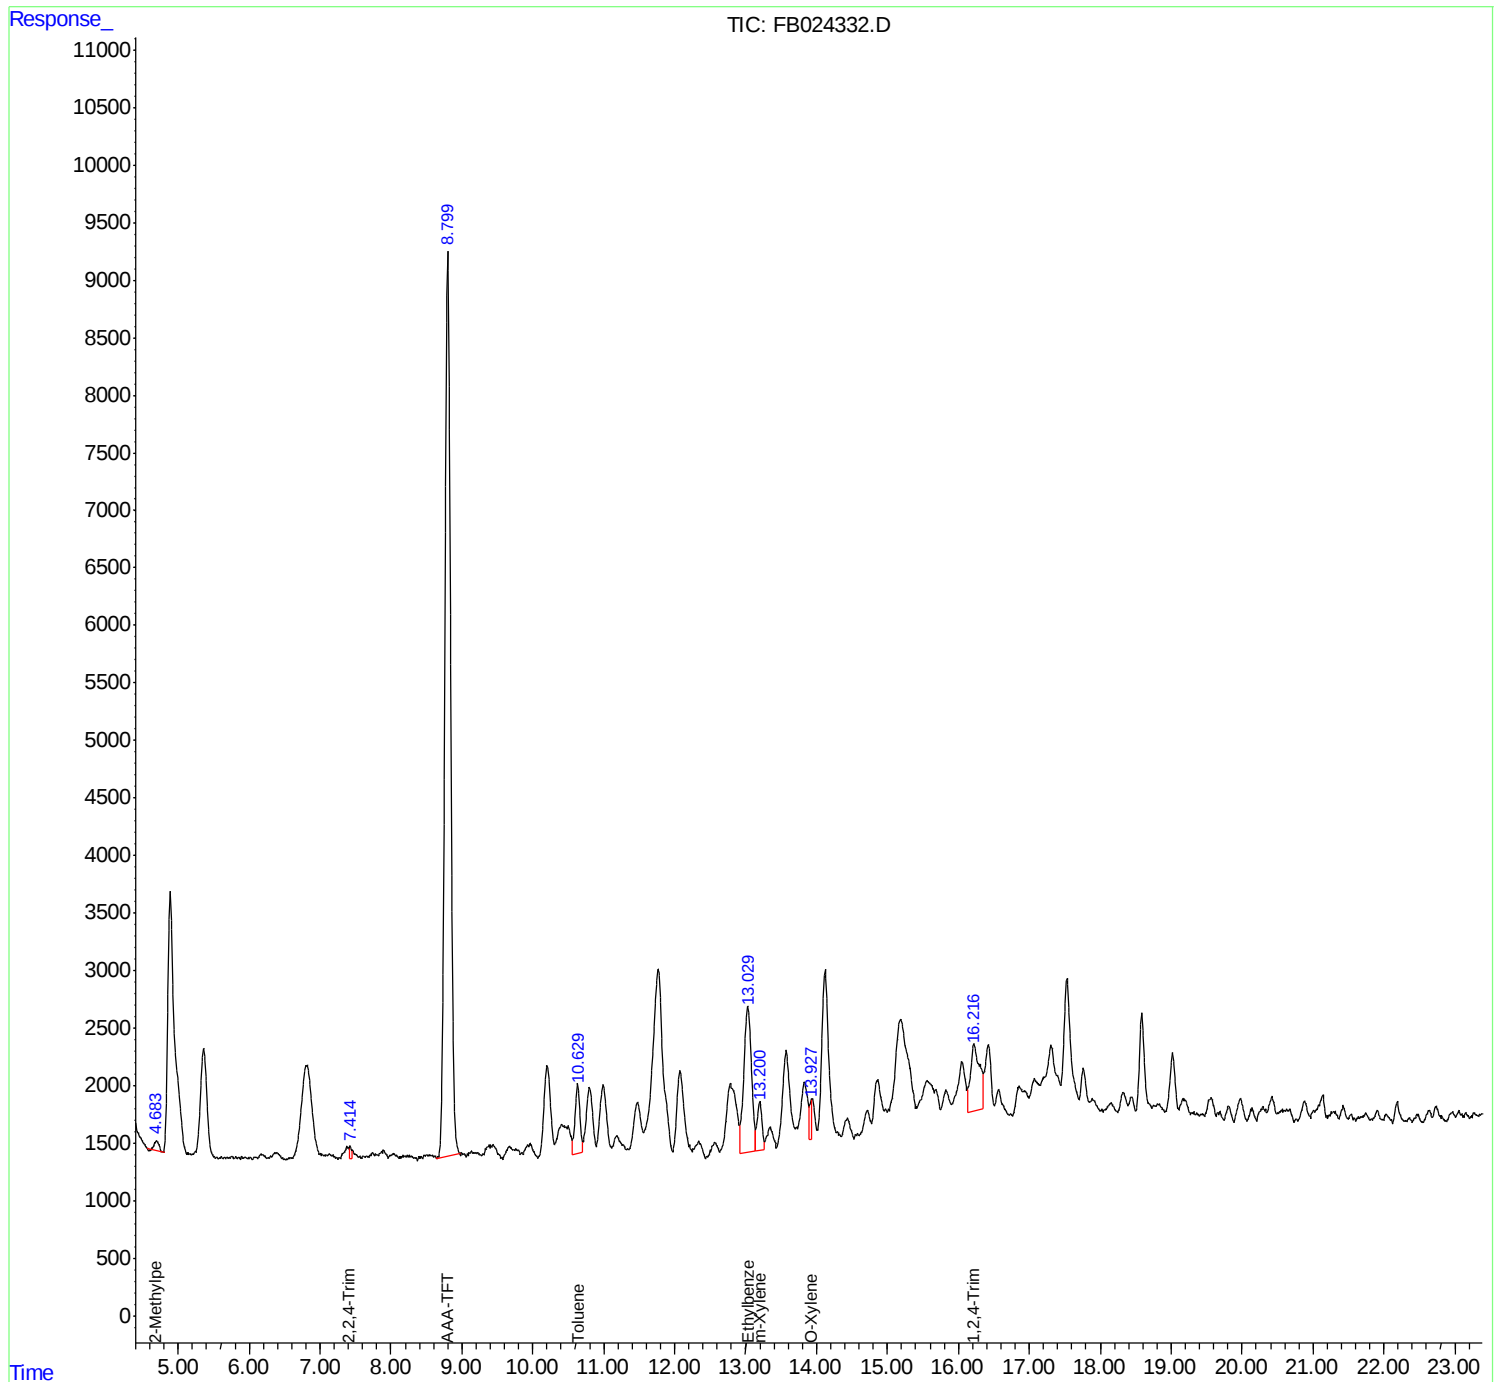


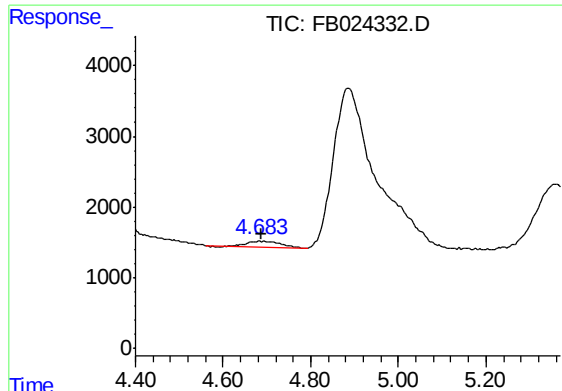

#1 2-Methylpentane


R.T.: 4.684 min
Delta R.T.: -0.005 min
Response: 4134
Conc: 0.14 ng/ml

Instrument :
FID_B
ClientSampleId :
PL-01-050820

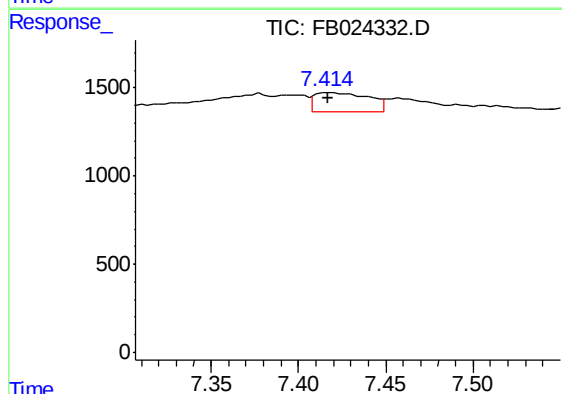


#2 2,2,4-Trimethylpentane

R.T.: 7.417 min
Delta R.T.: 0.000 min
Response: 2347
Conc: 0.08 ng/ml

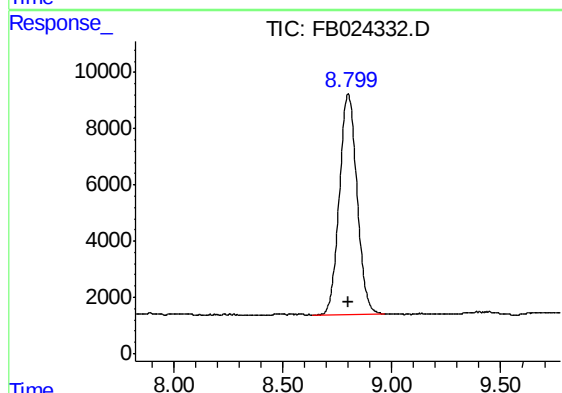


#5 AAA-TFT

R.T.: 8.800 min
Delta R.T.: 0.001 min
Response: 442577
Conc: 20.04 ng/ml

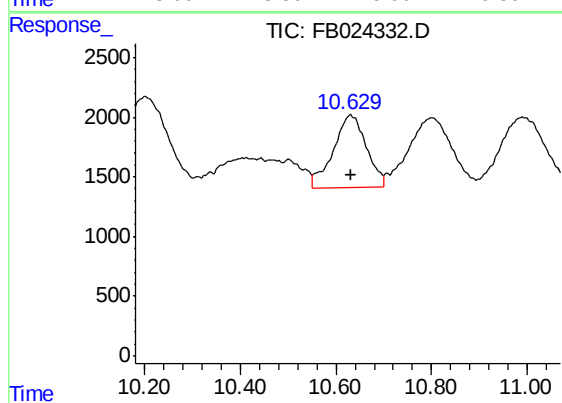

#6 Toluene


R.T.: 10.630 min
Delta R.T.: 0.000 min
Response: 28879
Conc: 0.80 ng/ml

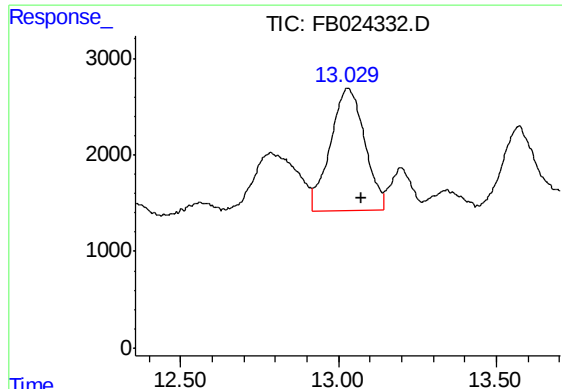

#7 Ethylbenzene


R.T.: 13.030 min
Delta R.T.: -0.041 min
Response: 95237
Conc: 2.81 ng/ml

Instrument :
FID_B
ClientSampleId :
PL-01-050820

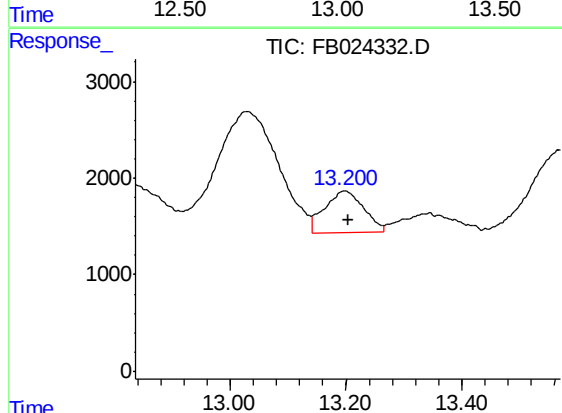


#8 m-Xylene

R.T.: 13.201 min
Delta R.T.: -0.004 min
Response: 19514
Conc: 0.59 ng/ml

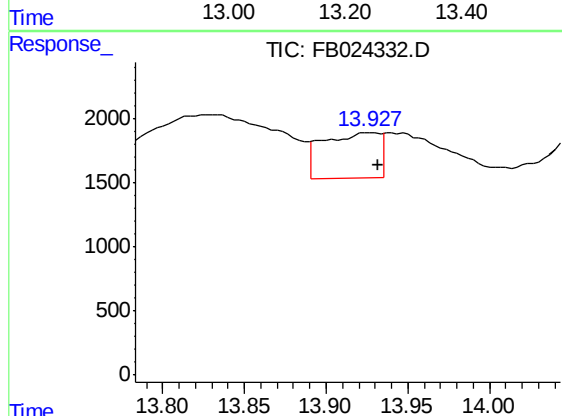

#9 o-Xylene

R.T.: 13.928 min
Delta R.T.: -0.004 min
Response: 8370
Conc: 0.26 ng/ml

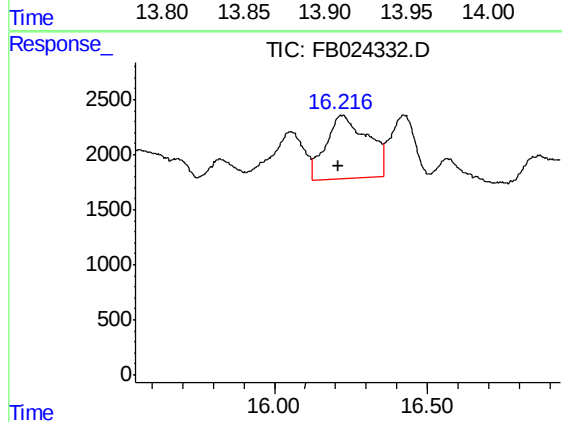

#10 1,2,4-Trimethylbenzene

R.T.: 16.218 min
Delta R.T.: 0.008 min
Response: 54254
Conc: 2.01 ng/ml