

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB0511220\
Data File : FB024333.D
Signal(s) : FID2B.CH
Acq On : 12 May 2020 15:49
Operator : DD/AJ
Sample : L2575-01
Misc : 5.06g/5.00ml DI WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
TP-28

Integration File: Calibration.e
Quant Time: May 13 02:47:40 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051120.M
Quant Title :
QLast Update : Mon May 11 11:14:42 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.800	505864	22.909 ng/ml
Target Compounds			
6) t Toluene	10.630	17975	0.496 ng/ml
7) t Ethylbenzene	13.070	4695	0.138 ng/ml
8) t m-Xylene	13.203	18493	0.560 ng/ml
9) t O-Xylene	13.931	5846	0.181 ng/ml
10) t 1,2,4-Trimethylbenzene	16.214	7933	0.294 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB051220\
Data File : FB024333.D
Signal(s) : FID2B.CH
Acq On : 12 May 2020 15:49
Operator : DD/AJ
Sample : L2575-01
Misc : 5.06g/5.00ml DI WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
TP-28

Integration File: Calibration.e
Quant Time: May 13 02:47:40 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051120.M
Quant Title :
QLast Update : Mon May 11 11:14:42 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

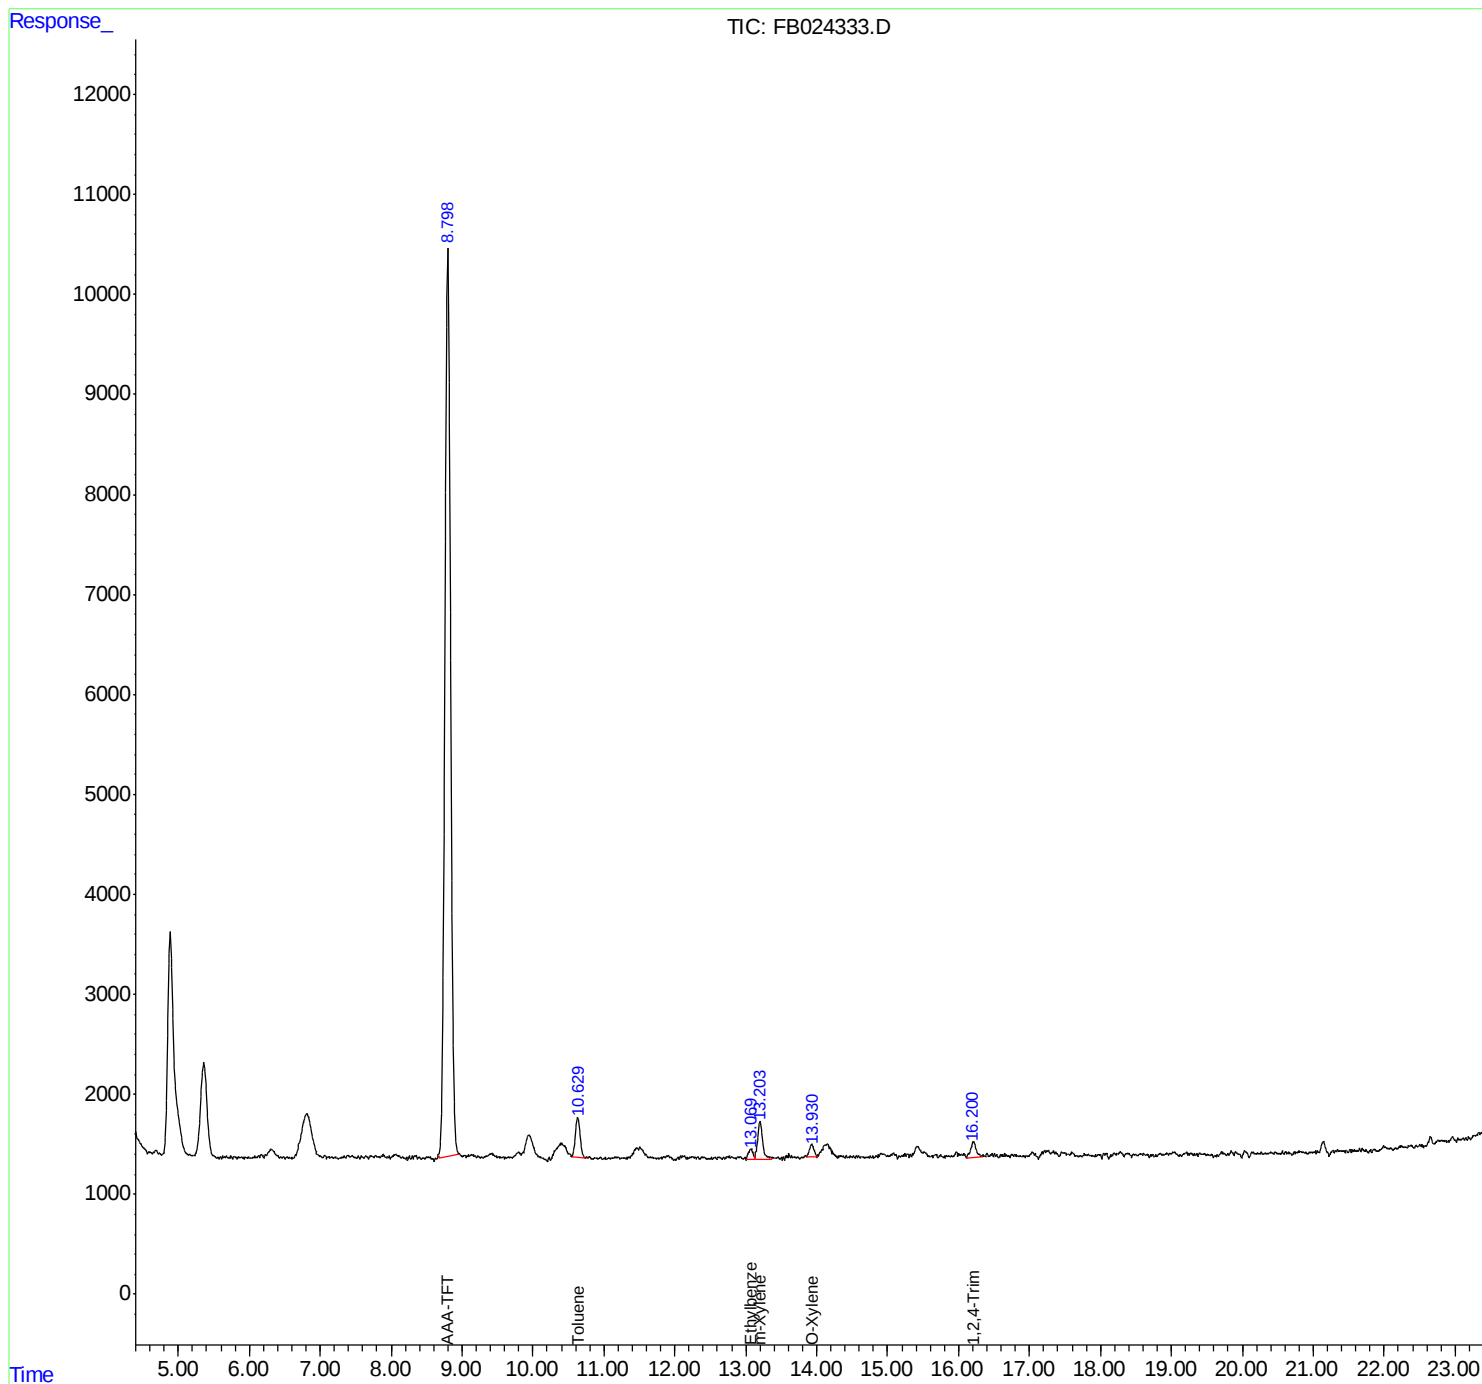


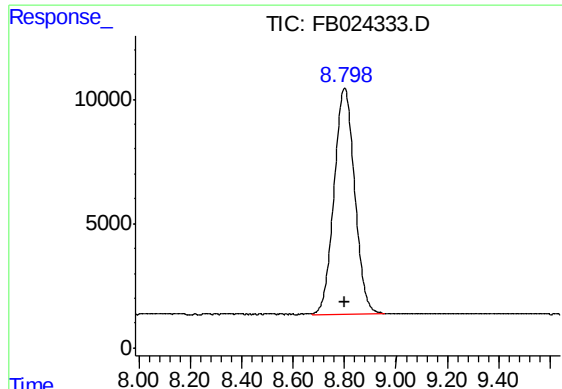

#5 AAA-TFT


R.T.: 8.800 min
Delta R.T.: 0.001 min
Response: 505864
Conc: 22.91 ng/ml

Instrument :
FID_B
ClientSampleId :
TP-28

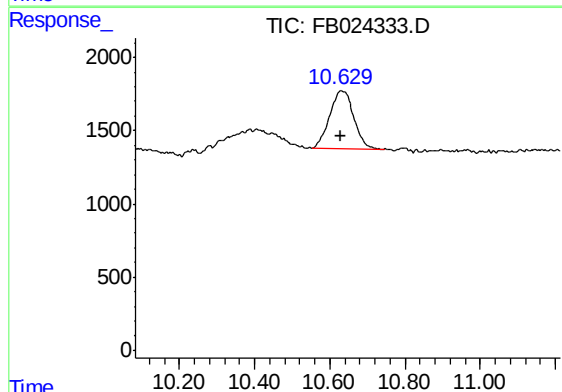


#6 Toluene

R.T.: 10.630 min
Delta R.T.: 0.000 min
Response: 17975
Conc: 0.50 ng/ml

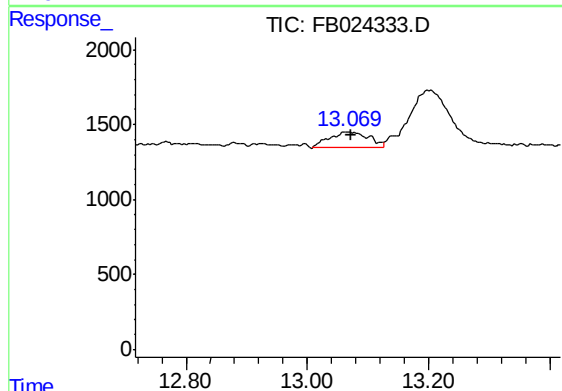


#7 Ethylbenzene

R.T.: 13.070 min
Delta R.T.: -0.001 min
Response: 4695
Conc: 0.14 ng/ml

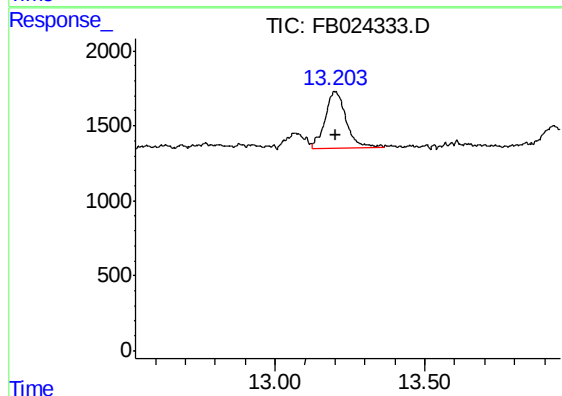

#8 m-Xylene


R.T.: 13.203 min
Delta R.T.: -0.001 min
Response: 18493
Conc: 0.56 ng/ml

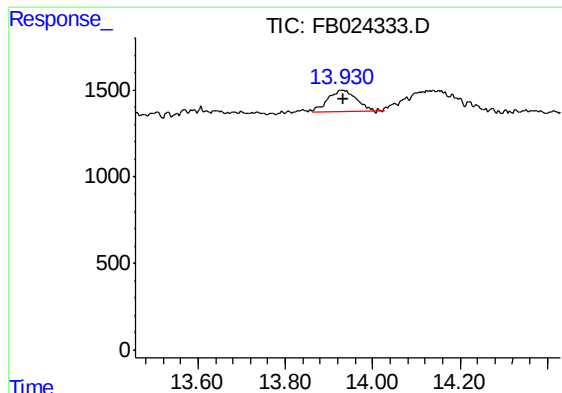

#9 O-Xylene

R.T.: 13.931 min
Delta R.T.: 0.000 min
Response: 5846
Conc: 0.18 ng/ml

Instrument :
FID_B
ClientSampleId :
TP-28

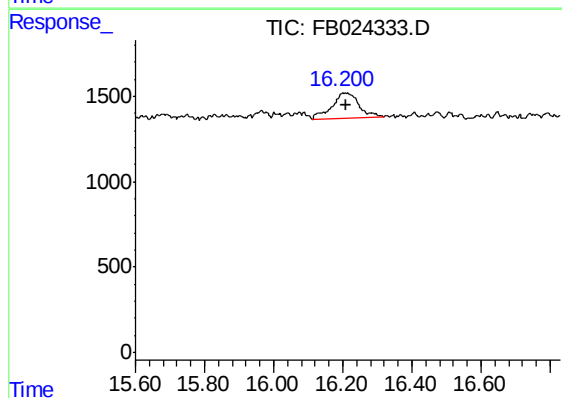

#10 1,2,4-Trimethylbenzene

R.T.: 16.214 min
Delta R.T.: 0.005 min
Response: 7933
Conc: 0.29 ng/ml