

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB0511220\
Data File : FB024335.D
Signal(s) : FID2B.CH
Acq On : 12 May 2020 16:50
Operator : DD/AJ
Sample : L2575-09
Misc : 5.03g/5.00ml DI WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
TP-27

Integration File: Calibration.e
Quant Time: May 13 02:47:59 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051120.M
Quant Title :
QLast Update : Mon May 11 11:14:42 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.802	533040	24.139 ng/ml
Target Compounds			
6) t Toluene	10.633	16843	0.465 ng/ml
7) t Ethylbenzene	13.069	4502	0.133 ng/ml
8) t m-Xylene	13.202	7711	0.234 ng/ml
9) t O-Xylene	13.938	5310	0.165 ng/ml
10) t 1,2,4-Trimethylbenzene	16.219	7810	0.290 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB051220\
Data File : FB024335.D
Signal(s) : FID2B.CH
Acq On : 12 May 2020 16:50
Operator : DD/AJ
Sample : L2575-09
Misc : 5.03g/5.00ml DI WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
TP-27

Integration File: Calibration.e
Quant Time: May 13 02:47:59 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051120.M
Quant Title :
QLast Update : Mon May 11 11:14:42 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

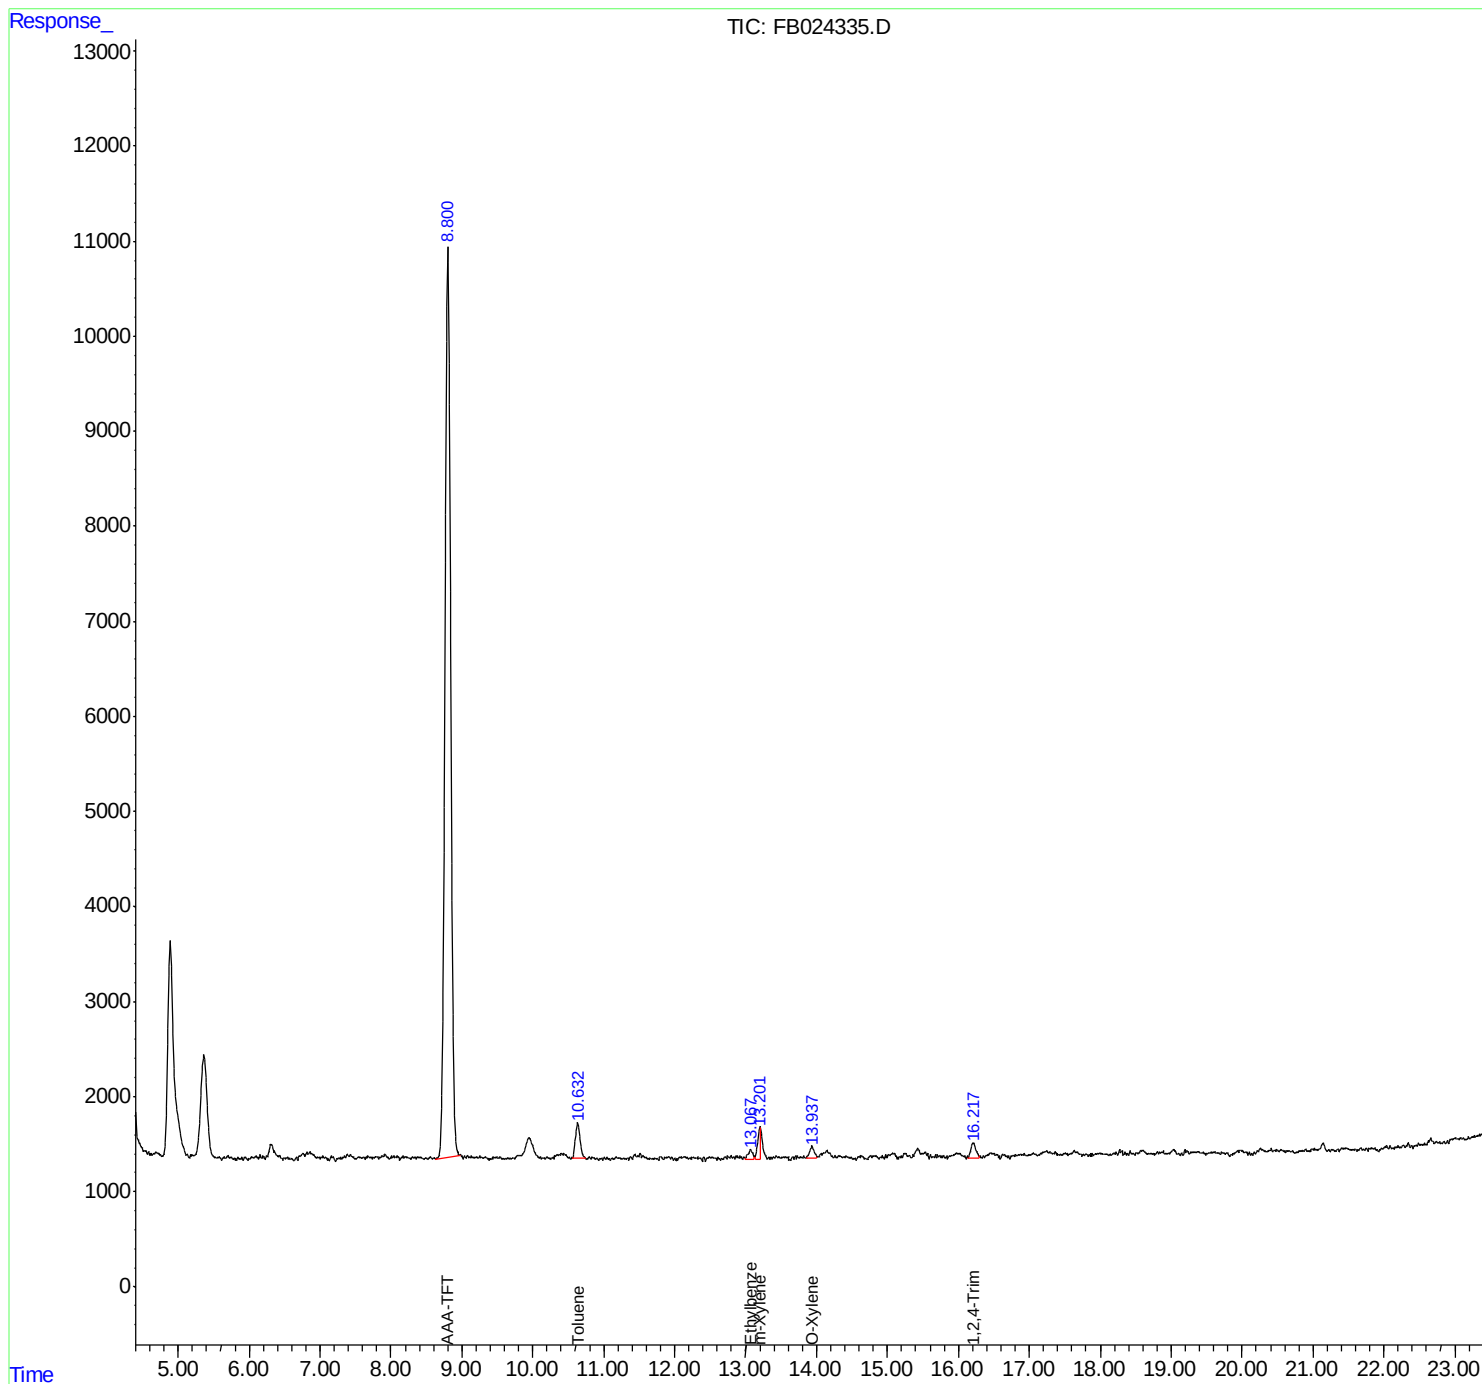


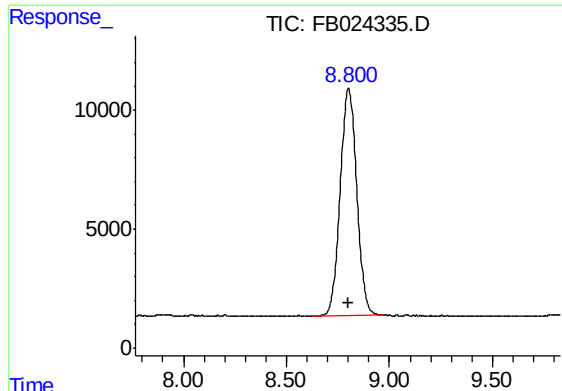

#5 AAA-TFT


R.T.: 8.802 min
Delta R.T.: 0.003 min
Response: 533040
Conc: 24.14 ng/ml

Instrument :
FID_B
ClientSampleId :
TP-27

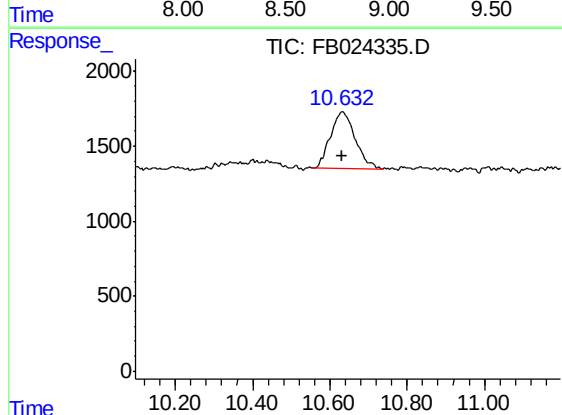


#6 Toluene

R.T.: 10.633 min
Delta R.T.: 0.002 min
Response: 16843
Conc: 0.46 ng/ml

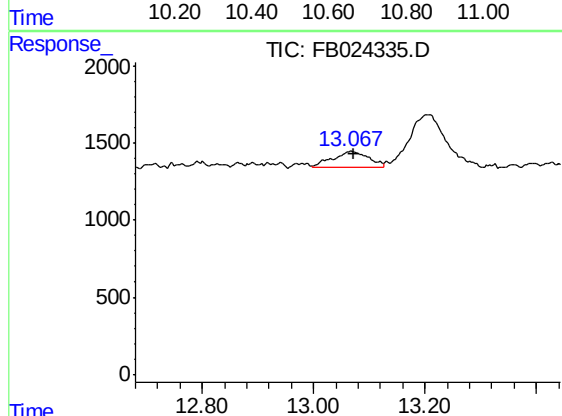


#7 Ethylbenzene

R.T.: 13.069 min
Delta R.T.: -0.002 min
Response: 4502
Conc: 0.13 ng/ml

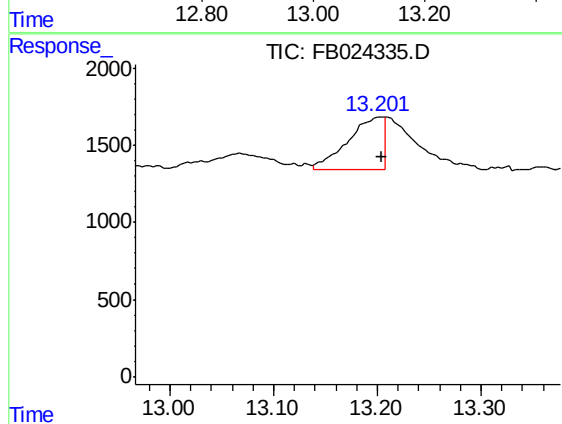

#8 m-Xylene


R.T.: 13.202 min
Delta R.T.: -0.002 min
Response: 7711
Conc: 0.23 ng/ml

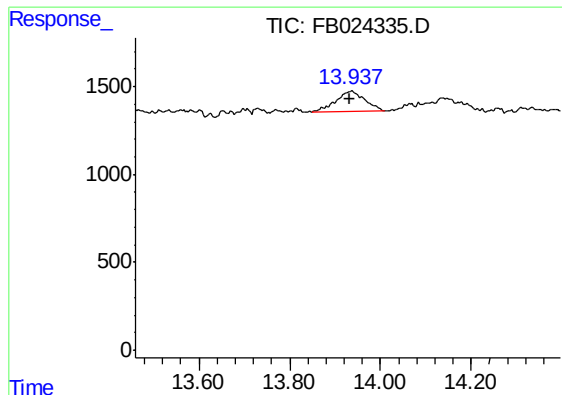

#9 O-Xylene

R.T.: 13.938 min
Delta R.T.: 0.006 min
Response: 5310
Conc: 0.16 ng/ml

Instrument :
FID_B
ClientSampleId :
TP-27

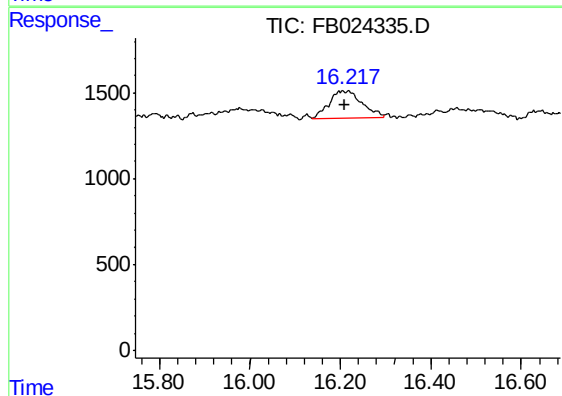

#10 1,2,4-Trimethylbenzene

R.T.: 16.219 min
Delta R.T.: 0.009 min
Response: 7810
Conc: 0.29 ng/ml