

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB051220\
 Data File : FB024338.D
 Signal(s) : FID2B.CH
 Acq On : 12 May 2020 18:23
 Operator : DD/AJ
 Sample : L2595-02MS
 Misc : 5.03g/5.00ml DI WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 JHDS-SOUTH-DMS

Integration File: Calibration.e
 Quant Time: May 13 02:48:27 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051120.M
 Quant Title :
 QLast Update : Mon May 11 11:14:42 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.801	429532	19.452 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.693	887385	30.071 ng/ml
2) t 2,2,4-Trimethylpentane	7.421	920843	30.143 ng/ml
3) t n-Heptane	7.759	306429	10.115 ng/ml
4) t Benzene	7.894	383322	10.139 ng/ml
6) t Toluene	10.632	1100916	30.381 ng/ml
7) t Ethylbenzene	13.072	322567	9.515 ng/ml
8) t m-Xylene	13.205	644109	19.519 ng/ml
9) t O-Xylene	13.933	624186	19.343 ng/ml
10) t 1,2,4-Trimethylbenzene	16.211	523018	19.393 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB051220\
Data File : FB024338.D
Signal(s) : FID2B.CH
Acq On : 12 May 2020 18:23
Operator : DD/AJ
Sample : L2595-02MS
Misc : 5.03g/5.00ml DI WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
JHDS-SOUTH-DMS

Integration File: Calibration.e
Quant Time: May 13 02:48:27 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051120.M
Quant Title :
QLast Update : Mon May 11 11:14:42 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

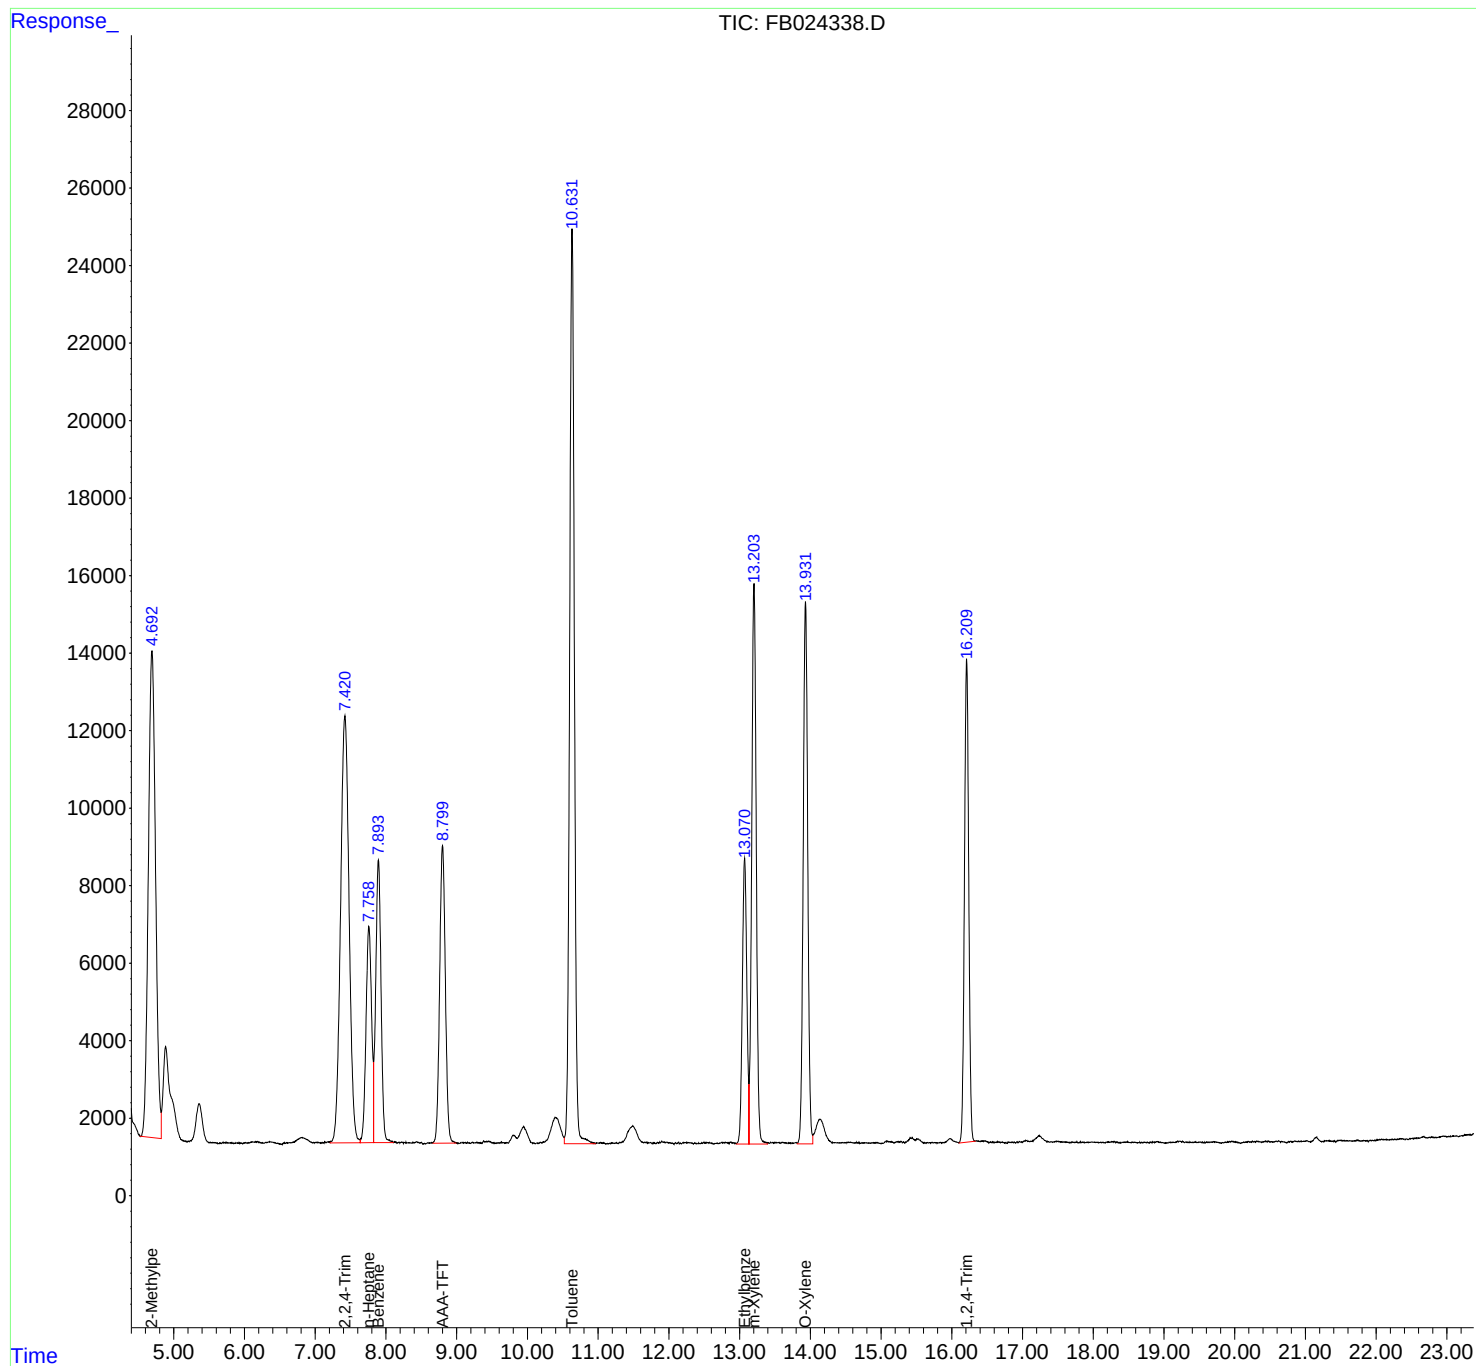


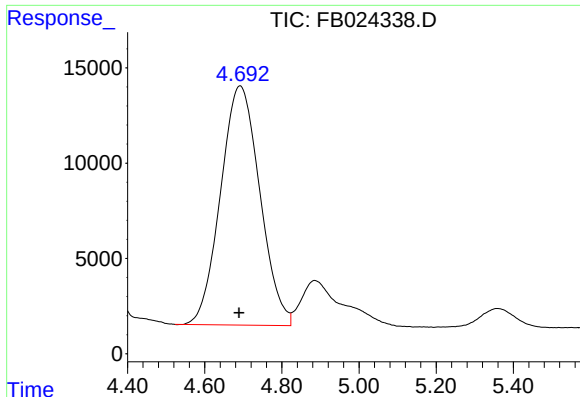

#1 2-Methylpentane


R.T.: 4.693 min
Delta R.T.: 0.004 min
Response: 887385
Conc: 30.07 ng/ml

Instrument :
FID_B
ClientSampleId :
JHDS-SOUTH-DMS

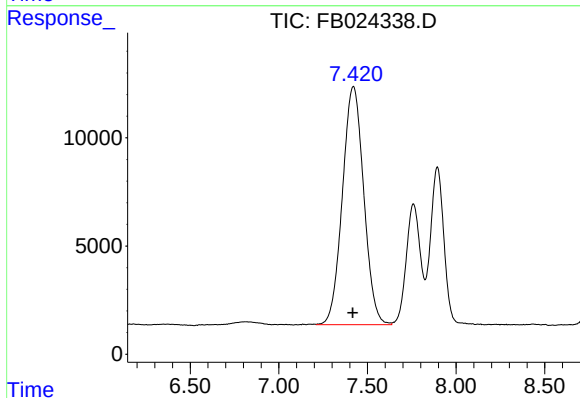


#2 2,2,4-Trimethylpentane

R.T.: 7.421 min
Delta R.T.: 0.004 min
Response: 920843
Conc: 30.14 ng/ml

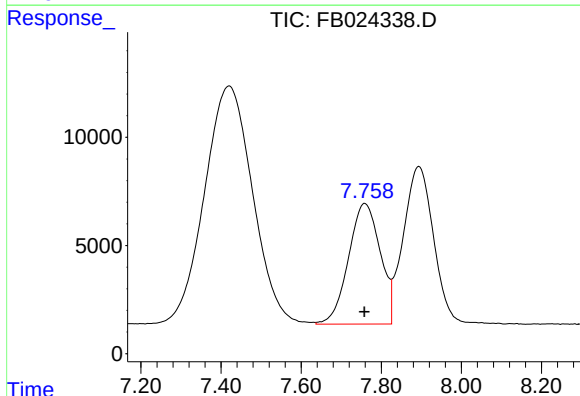


#3 n-Heptane

R.T.: 7.759 min
Delta R.T.: 0.001 min
Response: 306429
Conc: 10.11 ng/ml

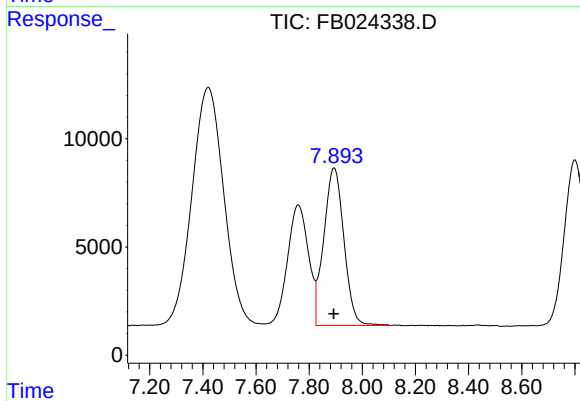

#4 Benzene


R.T.: 7.894 min
Delta R.T.: 0.002 min
Response: 383322
Conc: 10.14 ng/ml

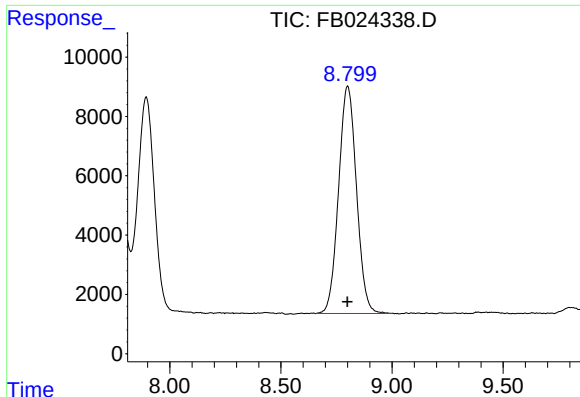

#5 AAA-TFT


R.T.: 8.801 min
Delta R.T.: 0.001 min
Response: 429532
Conc: 19.45 ng/ml

Instrument :
FID_B
ClientSampleId :
JHDS-SOUTH-DMS

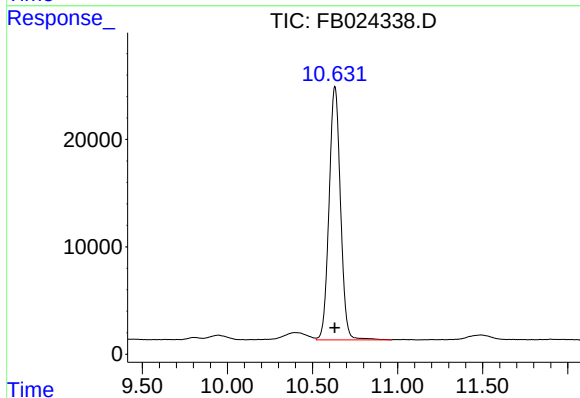


#6 Toluene

R.T.: 10.632 min
Delta R.T.: 0.001 min
Response: 1100916
Conc: 30.38 ng/ml

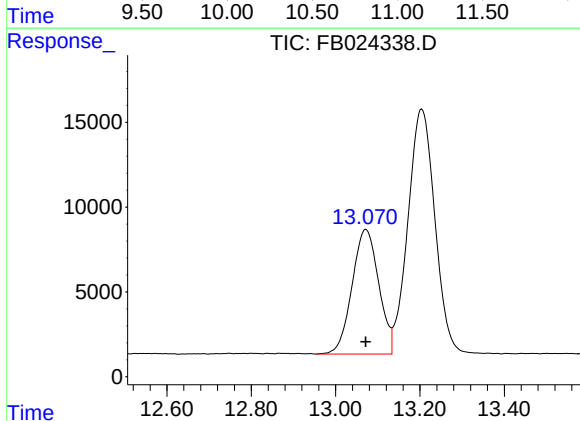


#7 Ethylbenzene

R.T.: 13.072 min
Delta R.T.: 0.000 min
Response: 322567
Conc: 9.51 ng/ml

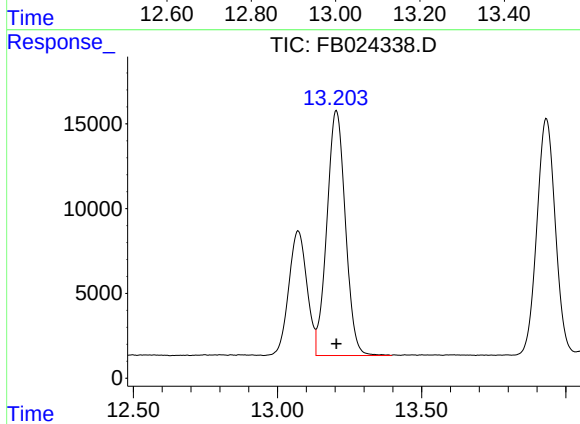

#8 m-Xylene


R.T.: 13.205 min
Delta R.T.: 0.000 min
Response: 644109
Conc: 19.52 ng/ml

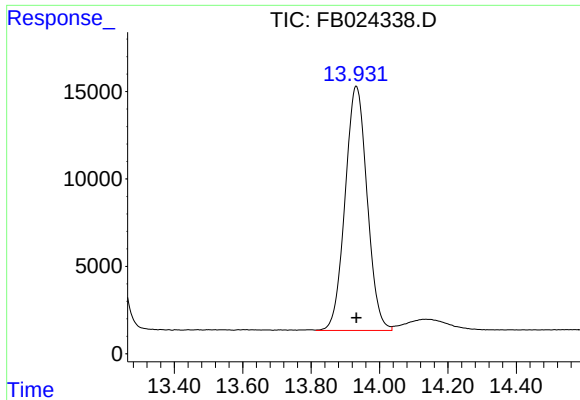

#9 O-Xylene

R.T.: 13.933 min
Delta R.T.: 0.000 min
Response: 624186
Conc: 19.34 ng/ml

Instrument :
FID_B
ClientSampleId :
JHDS-SOUTH-DMS

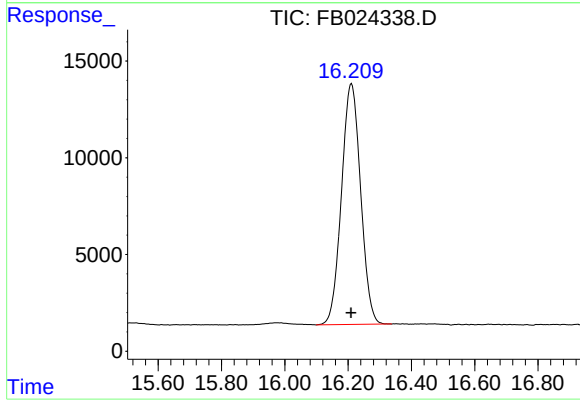

#10 1,2,4-Trimethylbenzene

R.T.: 16.211 min
Delta R.T.: 0.001 min
Response: 523018
Conc: 19.39 ng/ml