

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB051225\
Data File : FB031701.D
Signal(s) : FID2B.CH
Acq On : 12 May 2025 15:23
Operator : YP/AJ
Sample : VBF0512S2 50X
Misc : 5.00G/5.00 ML MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
VBF0512S2

Integration File: Calibration.e
Quant Time: May 13 03:01:05 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB042325.M
Quant Title :
QLast Update : Wed Apr 23 13:48:24 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.793	470315	20.508 ng/ml
Target Compounds				
6) t	Toluene	10.614	400	0.010 ng/ml
8) t	m-Xylene	13.193	8273	0.212 ng/ml
9) t	O-Xylene	13.920	4375	0.119 ng/ml
10) t	1,2,4-Trimethylbenzene	16.194	5420	0.201 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB051225\
Data File : FB031701.D
Signal(s) : FID2B.CH
Acq On : 12 May 2025 15:23
Operator : YP/AJ
Sample : VBF0512S2 50X
Misc : 5.00G/5.00 ML MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
VBF0512S2

Integration File: Calibration.e
Quant Time: May 13 03:01:05 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB042325.M
Quant Title :
QLast Update : Wed Apr 23 13:48:24 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

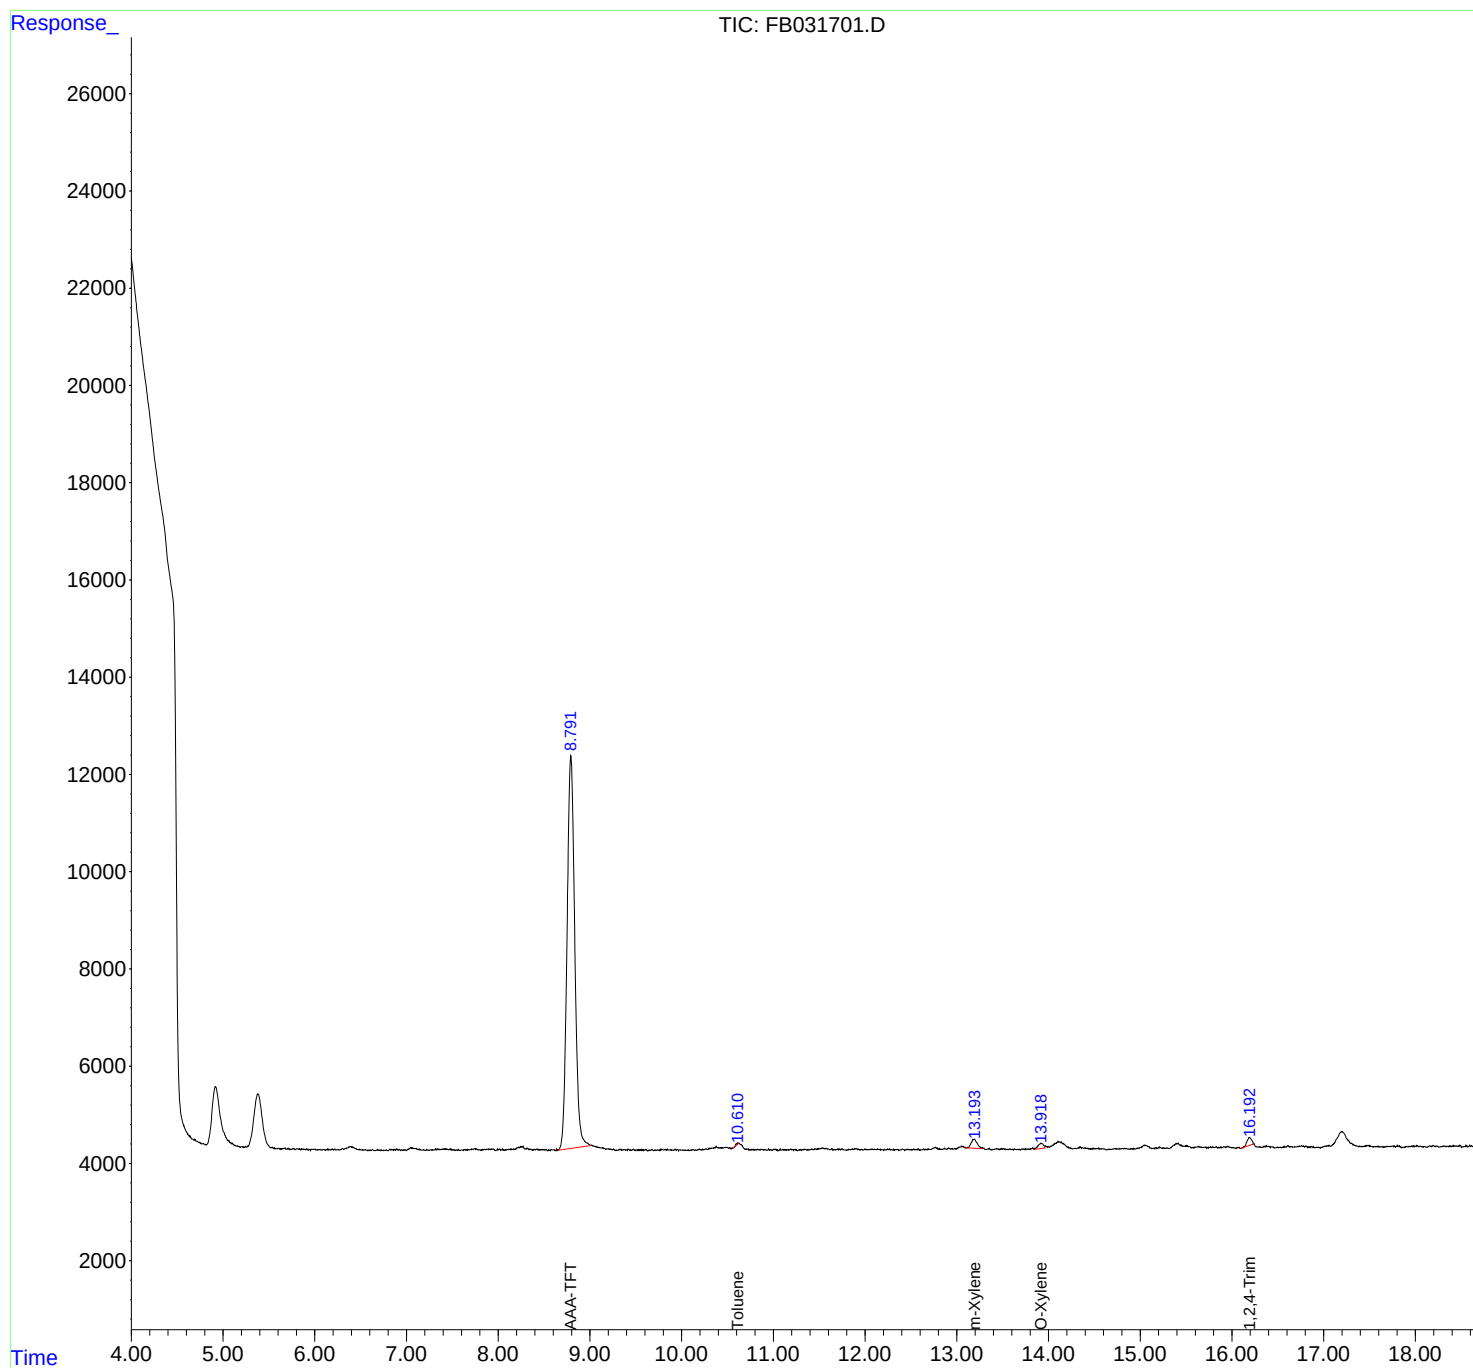


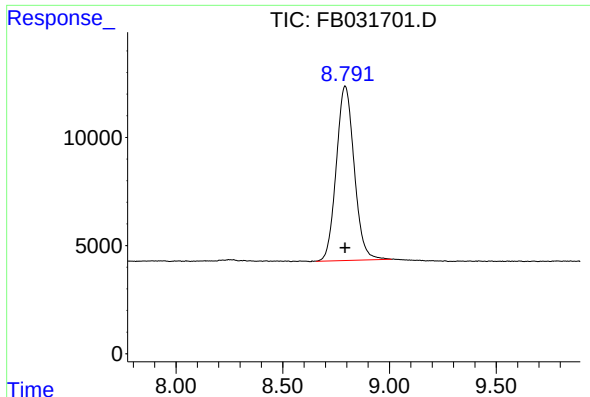

#5 AAA-TFT


R.T.: 8.793 min
Delta R.T.: 0.000 min
Response: 470315
Conc: 20.51 ng/ml

Instrument :
FID_B
ClientSampleId :
VBF0512S2

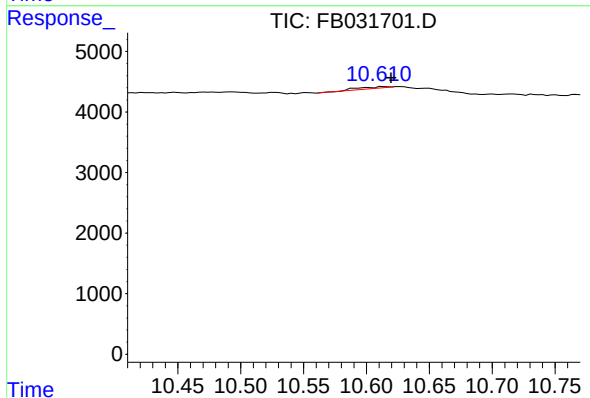


#6 Toluene

R.T.: 10.614 min
Delta R.T.: -0.006 min
Response: 400
Conc: 0.01 ng/ml

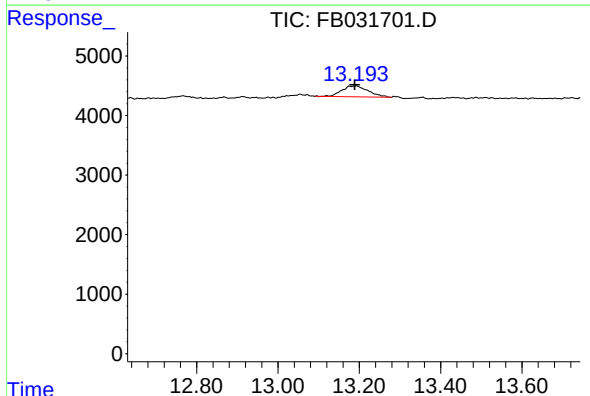


#8 m-Xylene

R.T.: 13.193 min
Delta R.T.: 0.005 min
Response: 8273
Conc: 0.21 ng/ml

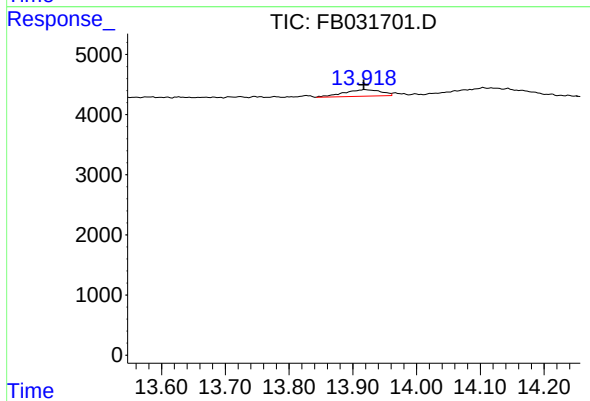

#9 O-Xylene

R.T.: 13.920 min
Delta R.T.: 0.003 min
Response: 4375
Conc: 0.12 ng/ml

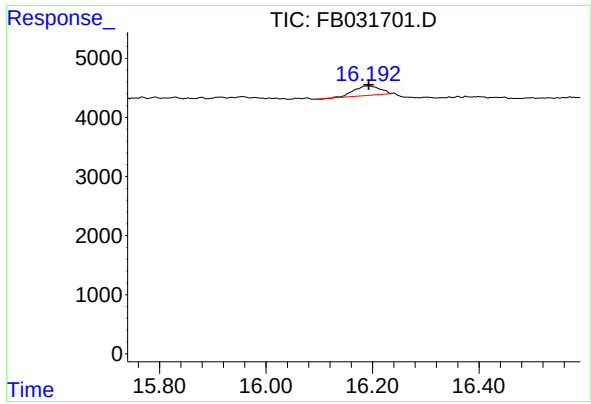

#10 1,2,4-Trimethylbenzene

R.T.: 16.194 min
Delta R.T.: 0.000 min
Response: 5420
Conc: 0.20 ng/ml

Instrument :
FID_B
ClientSampleId :
VBF0512S2