

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB051225\
Data File : FB031703.D
Signal(s) : FID2B.CH
Acq On : 12 May 2025 17:12
Operator : YP/AJ
Sample : Q1982-01
Misc : 5.22G/5.00 ML DI WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
TP-1

Integration File: Calibration.e
Quant Time: May 13 03:01:25 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB042325.M
Quant Title :
QLast Update : Wed Apr 23 13:48:24 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.795	121078	5.280 ng/ml
Target Compounds			
6) t Toluene	10.617	6892	0.173 ng/ml
8) t m-Xylene	13.191	6416	0.164 ng/ml
9) t O-Xylene	13.927	7926	0.215 ng/ml
10) t 1,2,4-Trimethylbenzene	16.196	14414	0.534 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB051225\
Data File : FB031703.D
Signal(s) : FID2B.CH
Acq On : 12 May 2025 17:12
Operator : YP/AJ
Sample : Q1982-01
Misc : 5.22G/5.00 ML DI WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
TP-1

Integration File: Calibration.e
Quant Time: May 13 03:01:25 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB042325.M
Quant Title :
QLast Update : Wed Apr 23 13:48:24 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

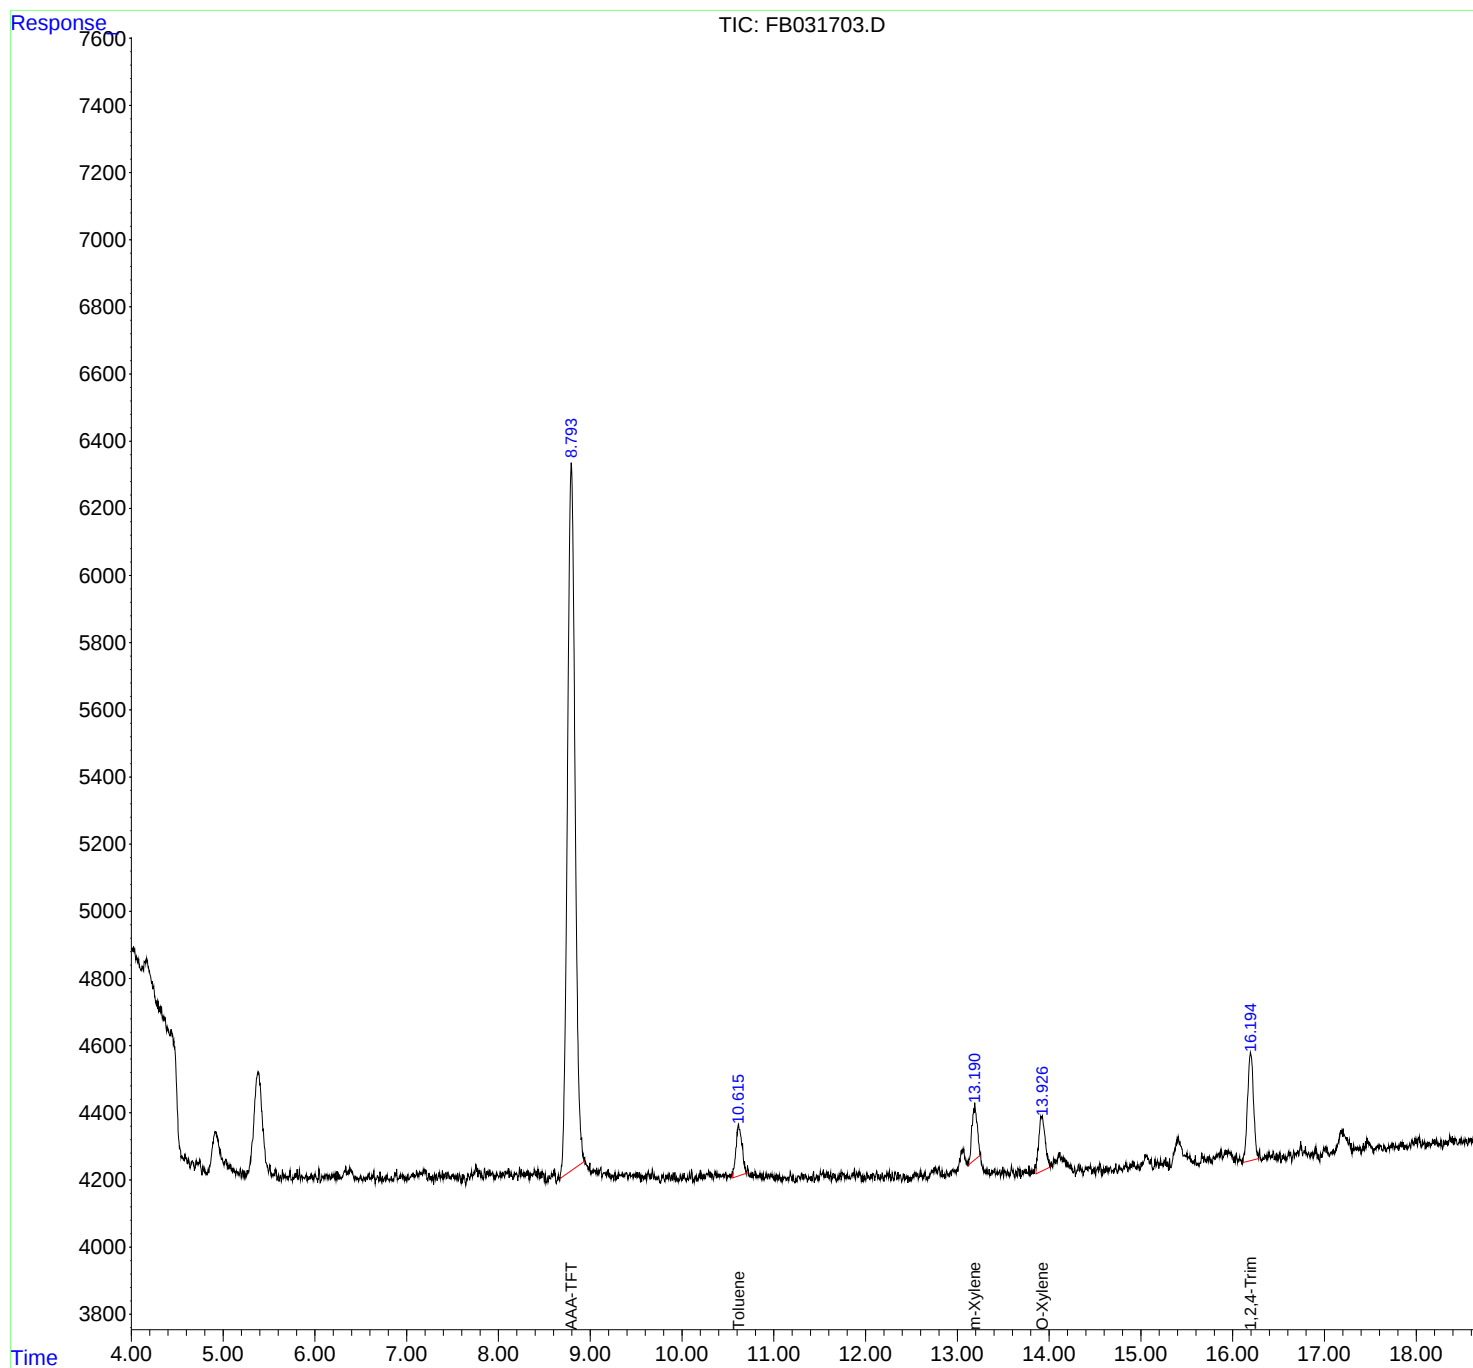


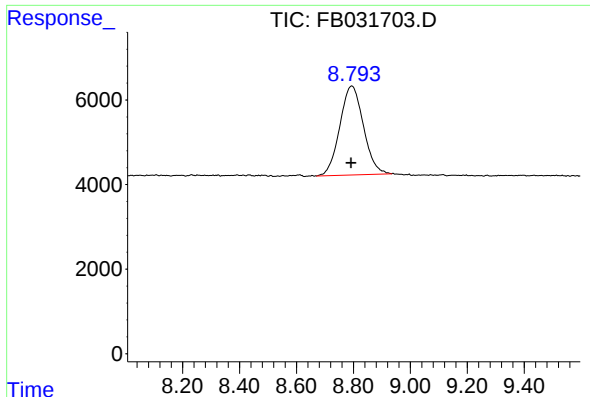

#5 AAA-TFT


R.T.: 8.795 min
Delta R.T.: 0.003 min
Response: 121078
Conc: 5.28 ng/ml

Instrument :
FID_B
ClientSampleId :
TP-1

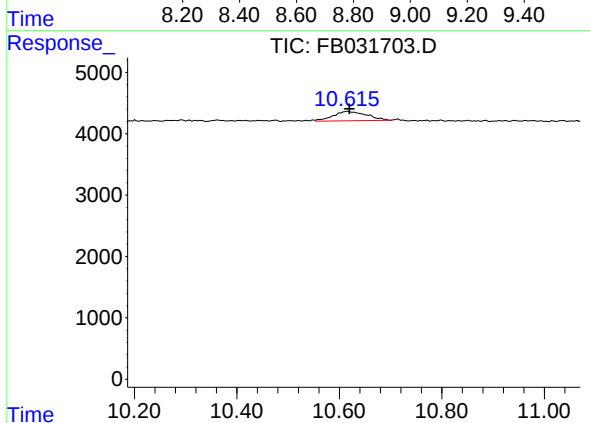


#6 Toluene

R.T.: 10.617 min
Delta R.T.: -0.003 min
Response: 6892
Conc: 0.17 ng/ml

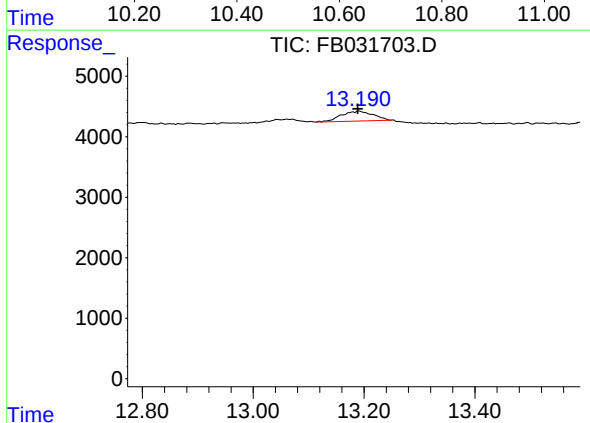


#8 m-Xylene

R.T.: 13.191 min
Delta R.T.: 0.002 min
Response: 6416
Conc: 0.16 ng/ml

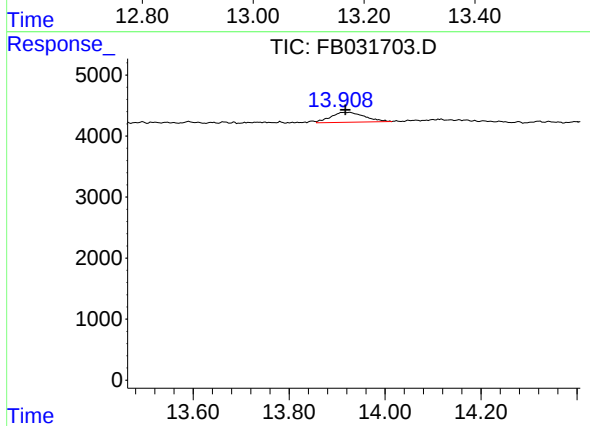

#9 O-Xylene

R.T.: 13.927 min
Delta R.T.: 0.010 min
Response: 7926
Conc: 0.22 ng/ml

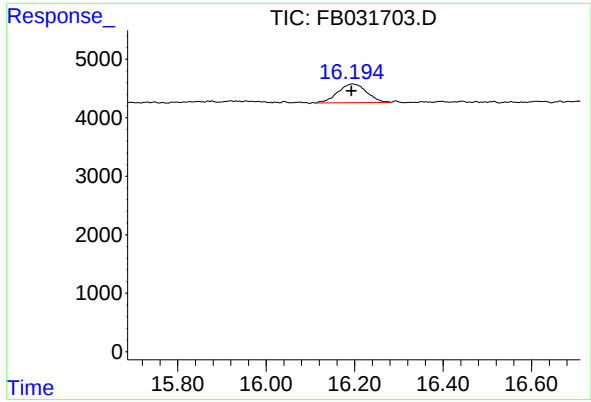

#10 1,2,4-Trimethylbenzene

R.T.: 16.196 min
Delta R.T.: 0.003 min
Response: 14414
Conc: 0.53 ng/ml

Instrument :
FID_B
ClientSampleId :
TP-1