

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB051319\
 Data File : FB021028.D
 Signal(s) : FID2B.CH
 Acq On : 13 May 2019 10:51
 Operator : MJ/SJ
 Sample : BSF0513S1
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: May 14 01:55:01 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB042919.M
 Quant Title :
 QLast Update : Mon Apr 29 15:53:58 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.992	365869	20.395 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.855	1186748	26.309 ng/ml
2) t 2,2,4-Trimethylpentane	7.608	1129847	27.105 ng/ml
3) t n-Heptane	7.948	351804	8.886 ng/ml
4) t Benzene	8.084	379071	9.061 ng/ml
6) t Toluene	10.837	752151	27.152 ng/ml
7) t Ethylbenzene	13.287	250630	8.936 ng/ml
8) t m-Xylene	13.420	539060	18.138 ng/ml
9) t O-Xylene	14.151	556941	17.968 ng/ml
10) t 1,2,4-Trimethylbenzene	16.436	564985	18.217 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB051319\
Data File : FB021028.D
Signal(s) : FID2B.CH
Acq On : 13 May 2019 10:51
Operator : MJ/SJ
Sample : BSF0513S1
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: May 14 01:55:01 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB042919.M
Quant Title :
QLast Update : Mon Apr 29 15:53:58 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

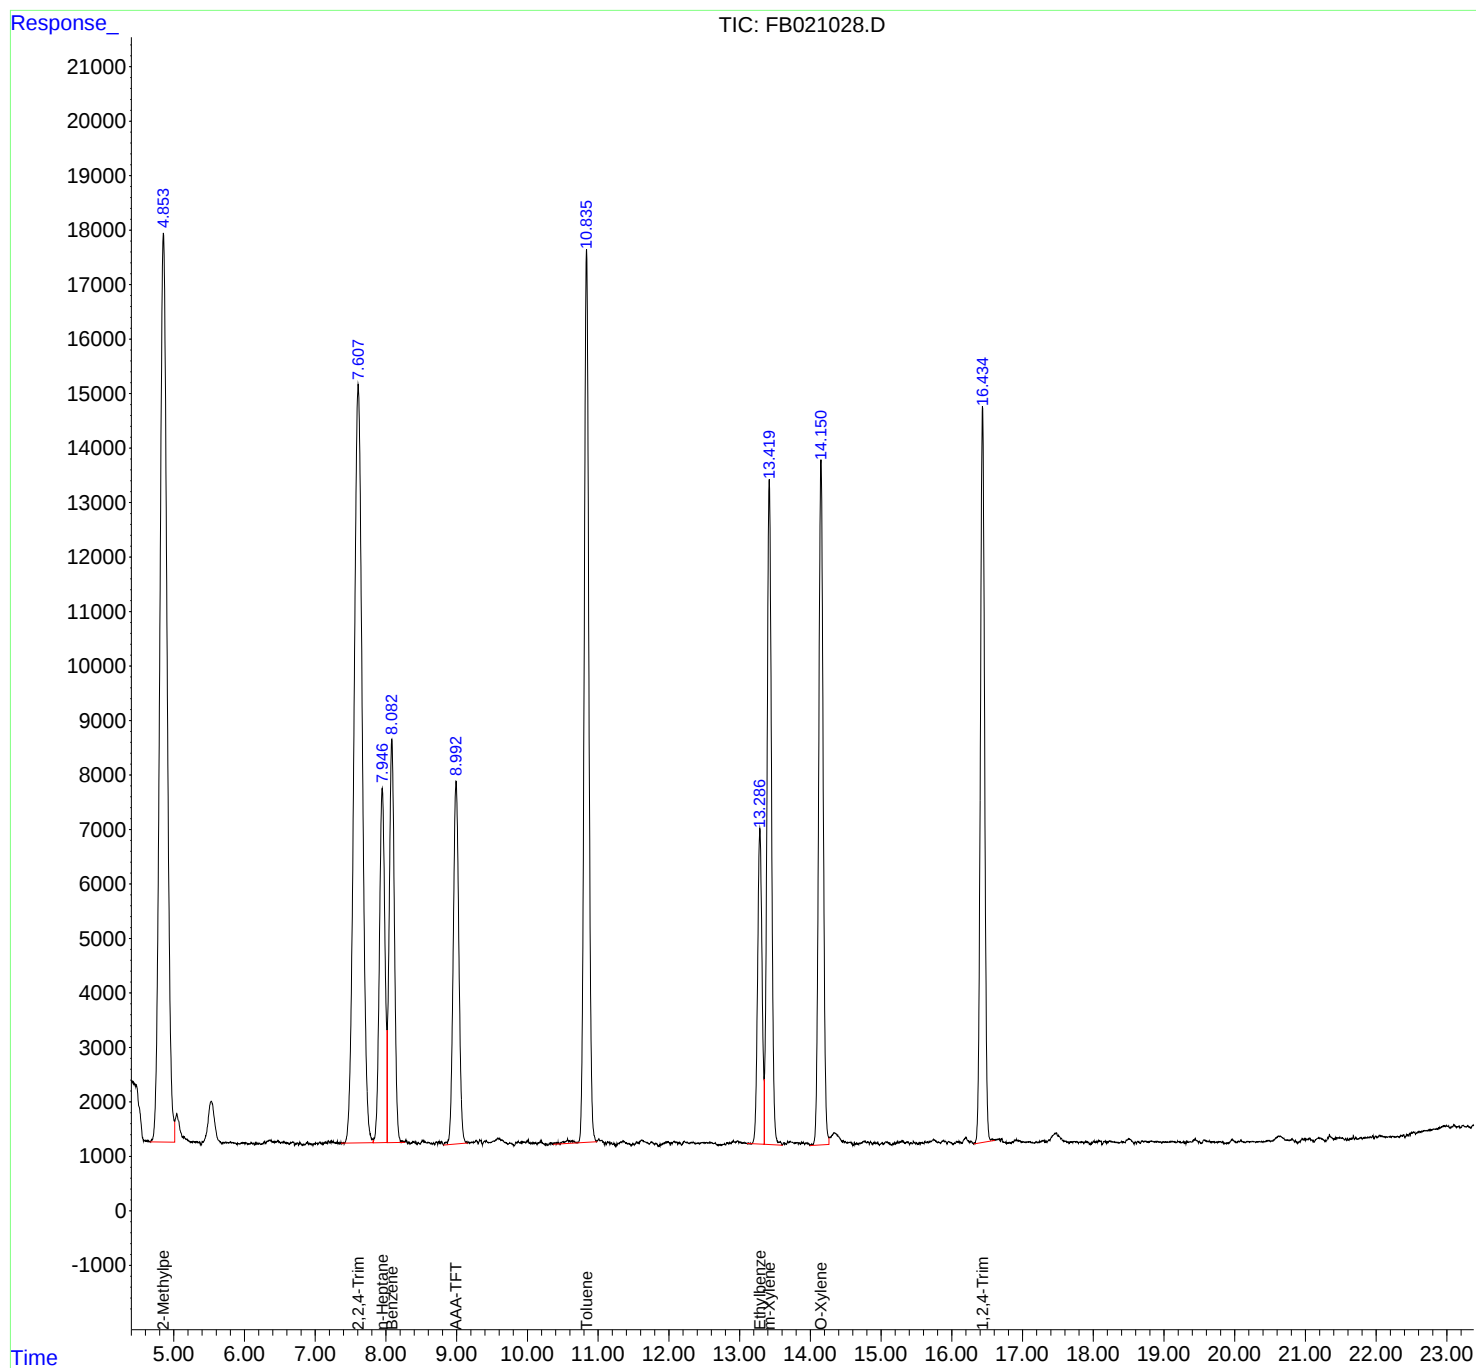

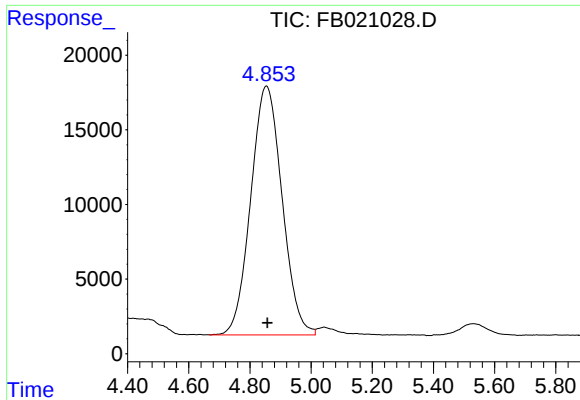


#1 2-Methylpentane

R.T.: 4.855 min
Delta R.T.: -0.002 min
Response: 1186748
Conc: 26.31 ng/ml

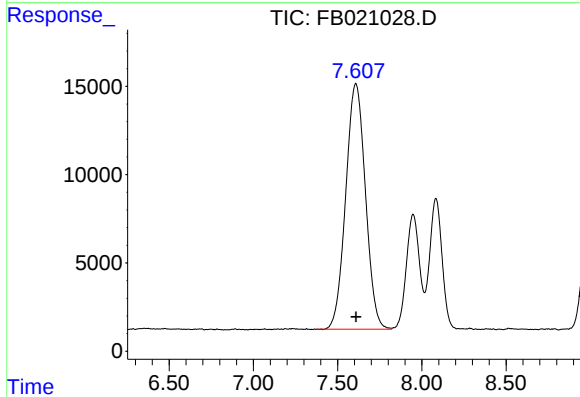


#2 2,2,4-Trimethylpentane

R.T.: 7.608 min
Delta R.T.: 0.000 min
Response: 1129847
Conc: 27.11 ng/ml

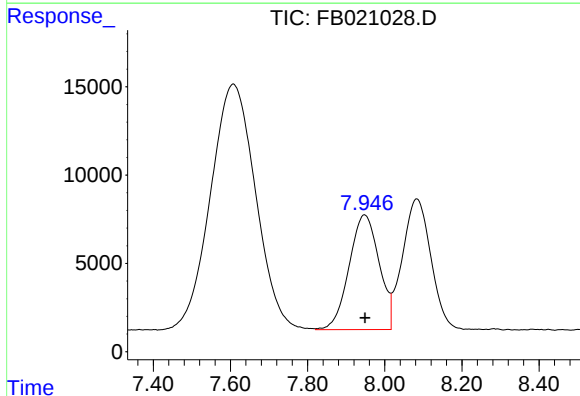


#3 n-Heptane

R.T.: 7.948 min
Delta R.T.: 0.000 min
Response: 351804
Conc: 8.89 ng/ml

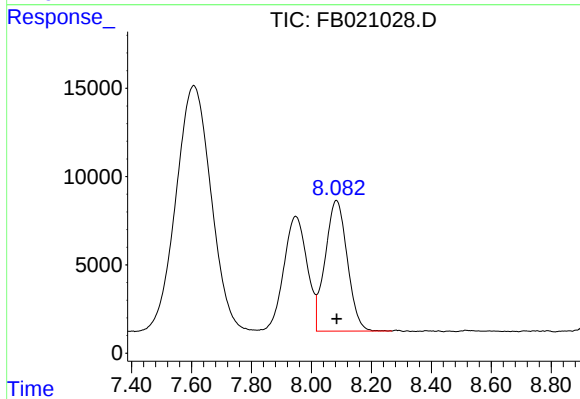


#4 Benzene

R.T.: 8.084 min
Delta R.T.: 0.000 min
Response: 379071
Conc: 9.06 ng/ml

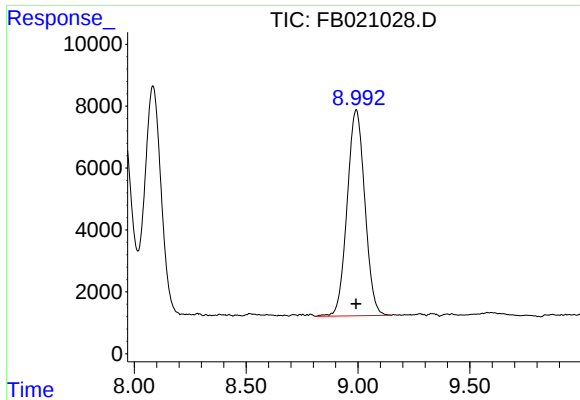


#5 AAA-TFT

R.T.: 8.992 min
Delta R.T.: 0.000 min
Response: 365869
Conc: 20.39 ng/ml

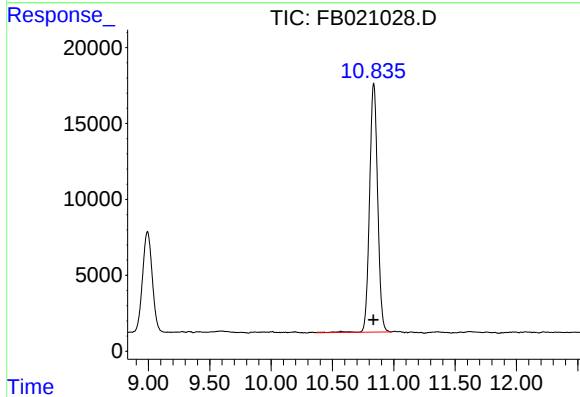


#6 Toluene

R.T.: 10.837 min
Delta R.T.: 0.000 min
Response: 752151
Conc: 27.15 ng/ml

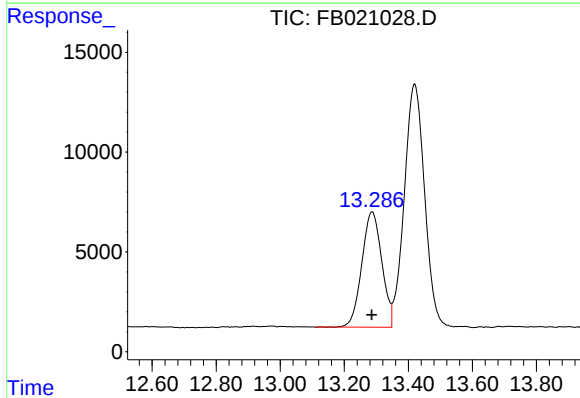


#7 Ethylbenzene

R.T.: 13.287 min
Delta R.T.: 0.002 min
Response: 250630
Conc: 8.94 ng/ml

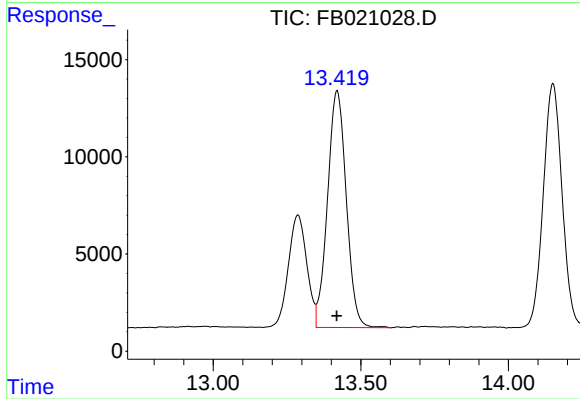


#8 m-Xylene

R.T.: 13.420 min
Delta R.T.: 0.001 min
Response: 539060
Conc: 18.14 ng/ml

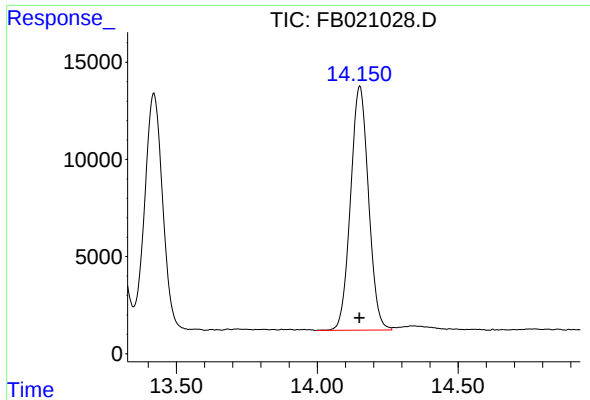

#9 O-Xylene

R.T.: 14.151 min
Delta R.T.: 0.002 min
Response: 556941
Conc: 17.97 ng/ml

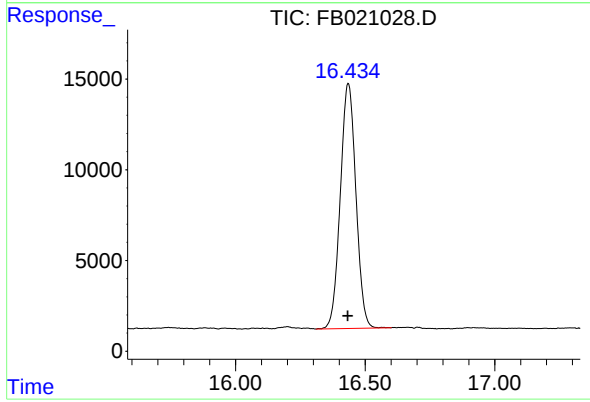

#10 1,2,4-Trimethylbenzene

R.T.: 16.436 min
Delta R.T.: 0.002 min
Response: 564985
Conc: 18.22 ng/ml