

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB051320\
 Data File : FB024346.D
 Signal(s) : FID2B.CH
 Acq On : 13 May 2020 12:13
 Operator : DD/AJ
 Sample : L2505-02
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: May 14 04:28:44 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051120.M
 Quant Title :
 QLast Update : Mon May 11 11:14:42 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.795	487115	22.059 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.688	2760	0.094 ng/ml
4) t Benzene	7.887	1155	0.031 ng/ml
6) t Toluene	10.625	26037	0.719 ng/ml
7) t Ethylbenzene	13.062	6222	0.184 ng/ml
8) t m-Xylene	13.200	15633	0.474 ng/ml
9) t O-Xylene	13.928	9534	0.295 ng/ml
10) t 1,2,4-Trimethylbenzene	16.209	4202	0.156 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB051320\
Data File : FB024346.D
Signal(s) : FID2B.CH
Acq On : 13 May 2020 12:13
Operator : DD/AJ
Sample : L2505-02
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: May 14 04:28:44 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051120.M
Quant Title :
QLast Update : Mon May 11 11:14:42 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

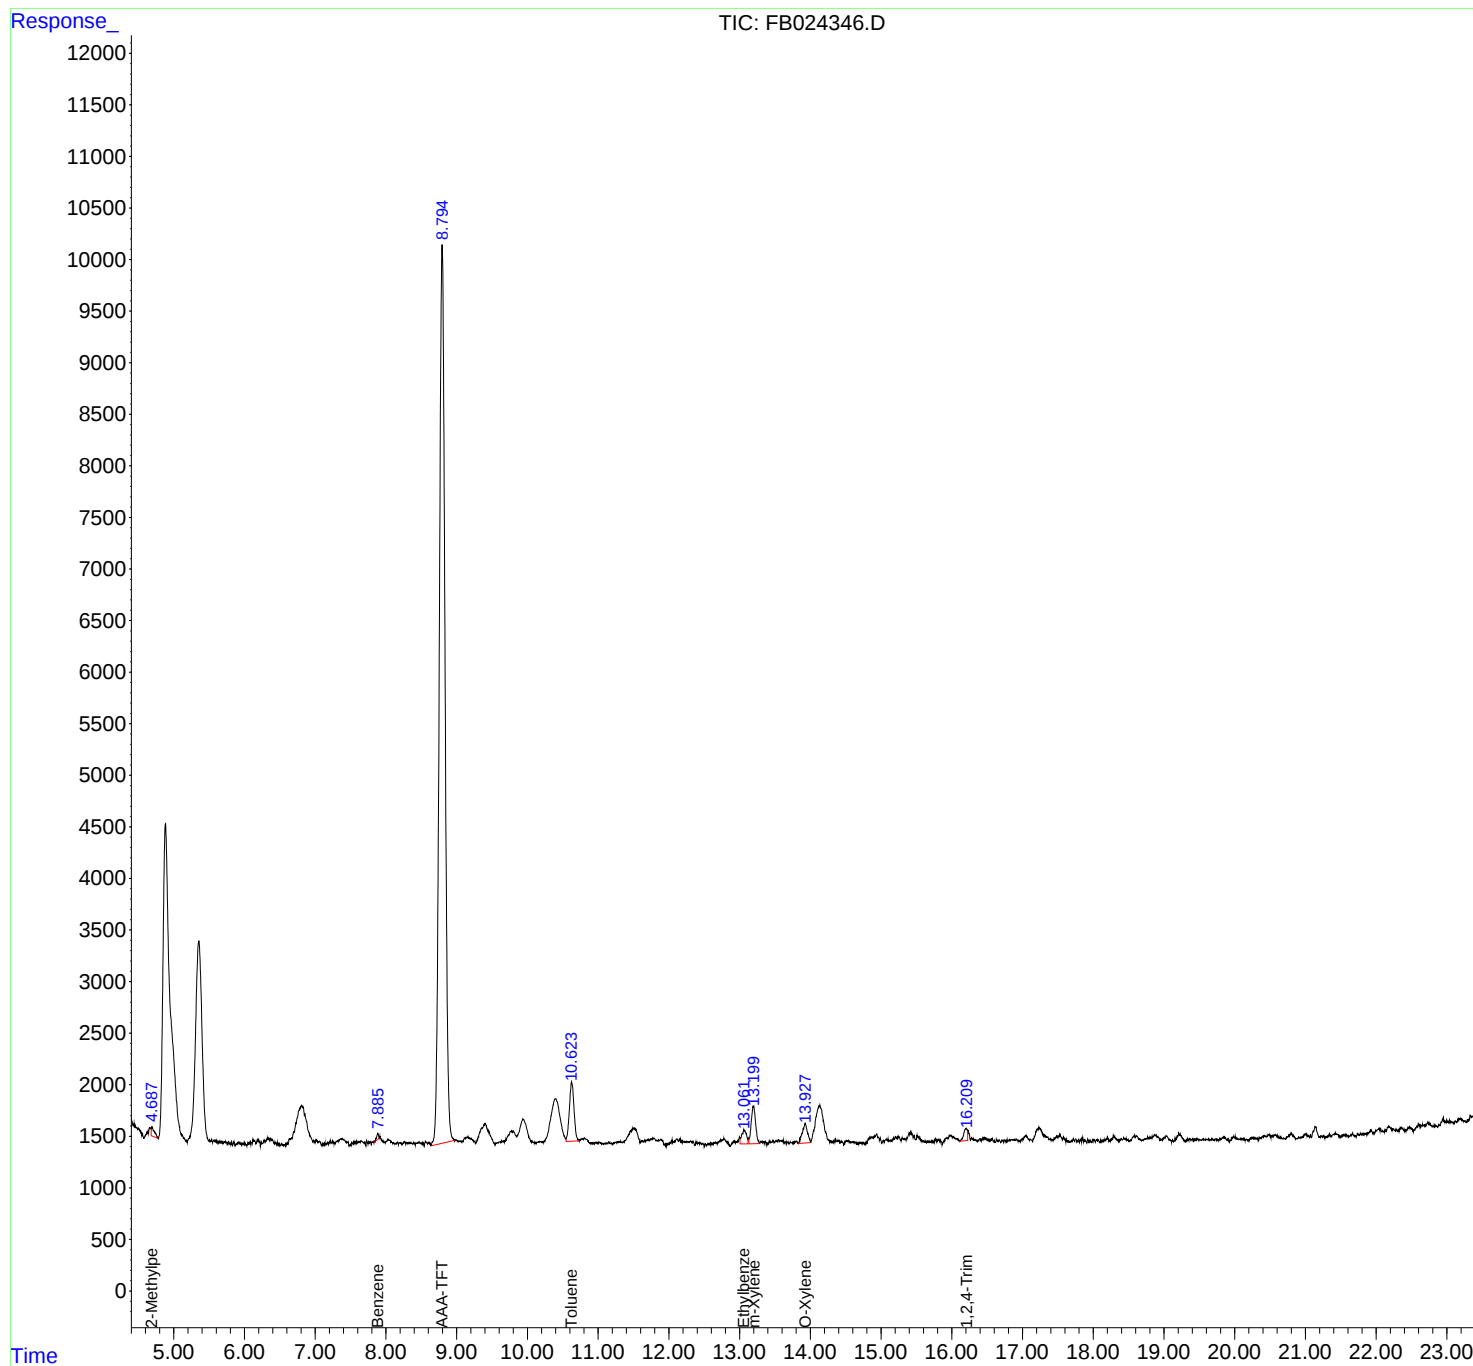


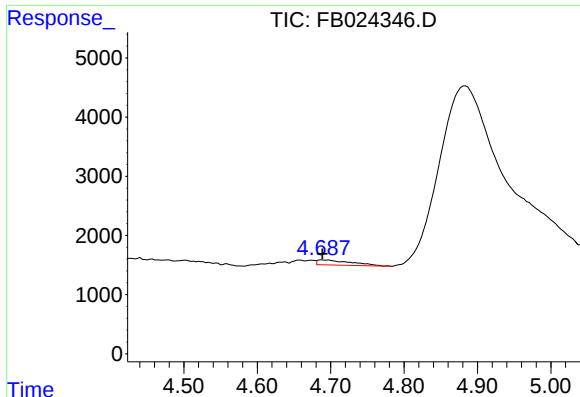

#1 2-Methylpentane


R.T.: 4.688 min
Delta R.T.: 0.000 min
Response: 2760
Conc: 0.09 ng/ml

Instrument :
FID_B
ClientSampleId :

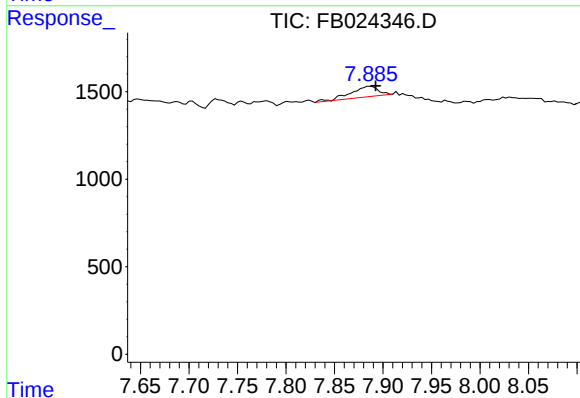


#4 Benzene

R.T.: 7.887 min
Delta R.T.: -0.006 min
Response: 1155
Conc: 0.03 ng/ml

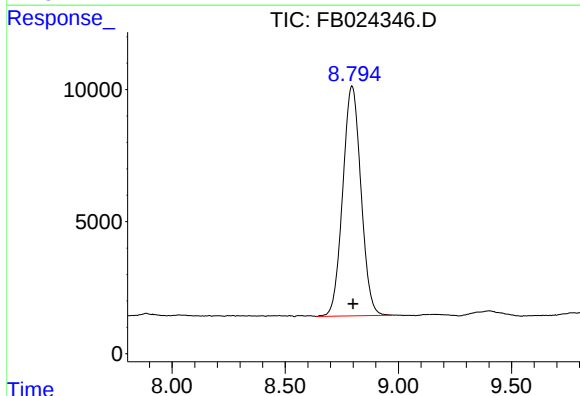


#5 AAA-TFT

R.T.: 8.795 min
Delta R.T.: -0.004 min
Response: 487115
Conc: 22.06 ng/ml

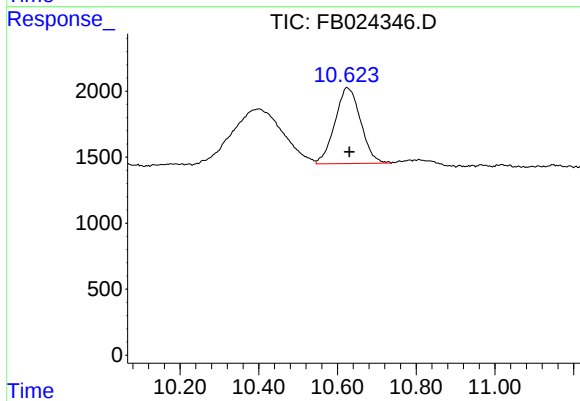

#6 Toluene


R.T.: 10.625 min
Delta R.T.: -0.006 min
Response: 26037
Conc: 0.72 ng/ml

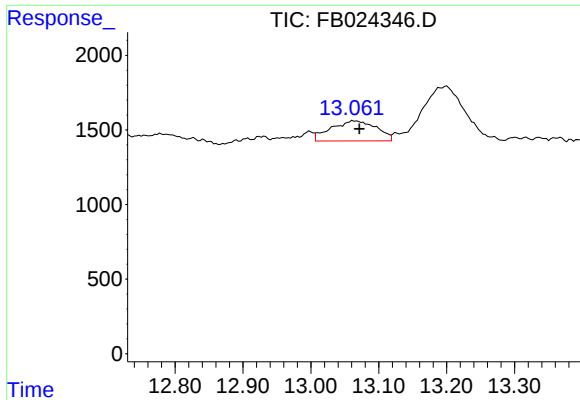

#7 Ethylbenzene


R.T.: 13.062 min
Delta R.T.: -0.009 min
Response: 6222
Conc: 0.18 ng/ml

Instrument :
FID_B
ClientSampleId :

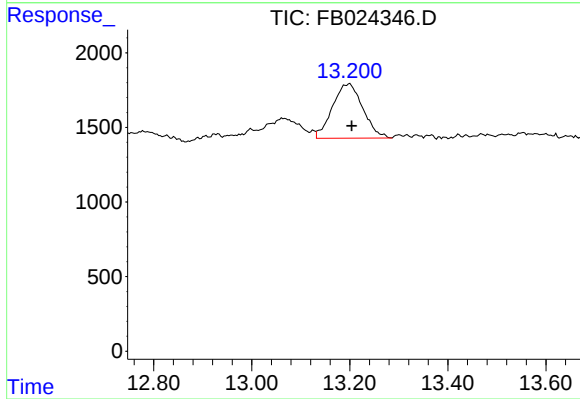


#8 m-Xylene

R.T.: 13.200 min
Delta R.T.: -0.004 min
Response: 15633
Conc: 0.47 ng/ml

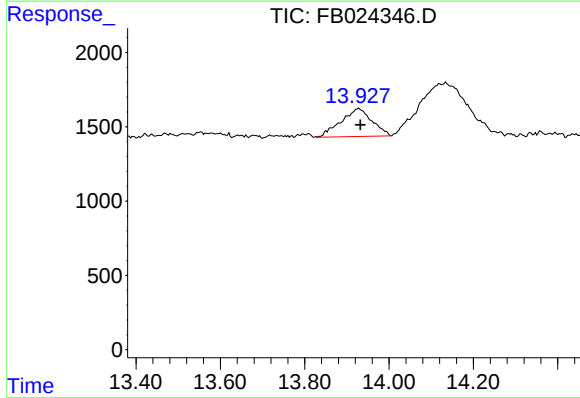

#9 o-Xylene

R.T.: 13.928 min
Delta R.T.: -0.004 min
Response: 9534
Conc: 0.30 ng/ml

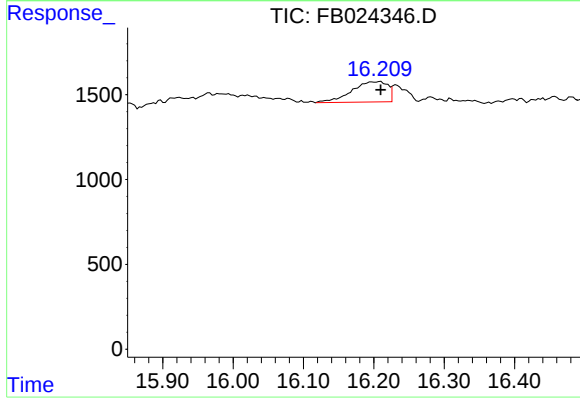

#10 1,2,4-Trimethylbenzene

R.T.: 16.209 min
Delta R.T.: 0.000 min
Response: 4202
Conc: 0.16 ng/ml