

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB051320\
 Data File : FB024351.D
 Signal(s) : FID2B.CH
 Acq On : 13 May 2020 15:52
 Operator : DD/AJ
 Sample : L2182-01
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: May 14 04:29:20 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051120.M
 Quant Title :
 QLast Update : Mon May 11 11:14:42 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.795	426148	19.299 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.689	53916	1.827 ng/ml
2) t 2,2,4-Trimethylpentane	7.417	25979	0.850 ng/ml
3) t n-Heptane	7.749	16894	0.558 ng/ml
4) t Benzene	7.890	19307	0.511 ng/ml
6) t Toluene	10.627	90449	2.496 ng/ml
7) t Ethylbenzene	13.070	25455	0.751 ng/ml
8) t m-Xylene	13.199	62905	1.906 ng/ml
9) t O-Xylene	13.935	72535	2.248 ng/ml
10) t 1,2,4-Trimethylbenzene	16.207	37037	1.373 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB051320\
Data File : FB024351.D
Signal(s) : FID2B.CH
Acq On : 13 May 2020 15:52
Operator : DD/AJ
Sample : L2182-01
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: May 14 04:29:20 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051120.M
Quant Title :
QLast Update : Mon May 11 11:14:42 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

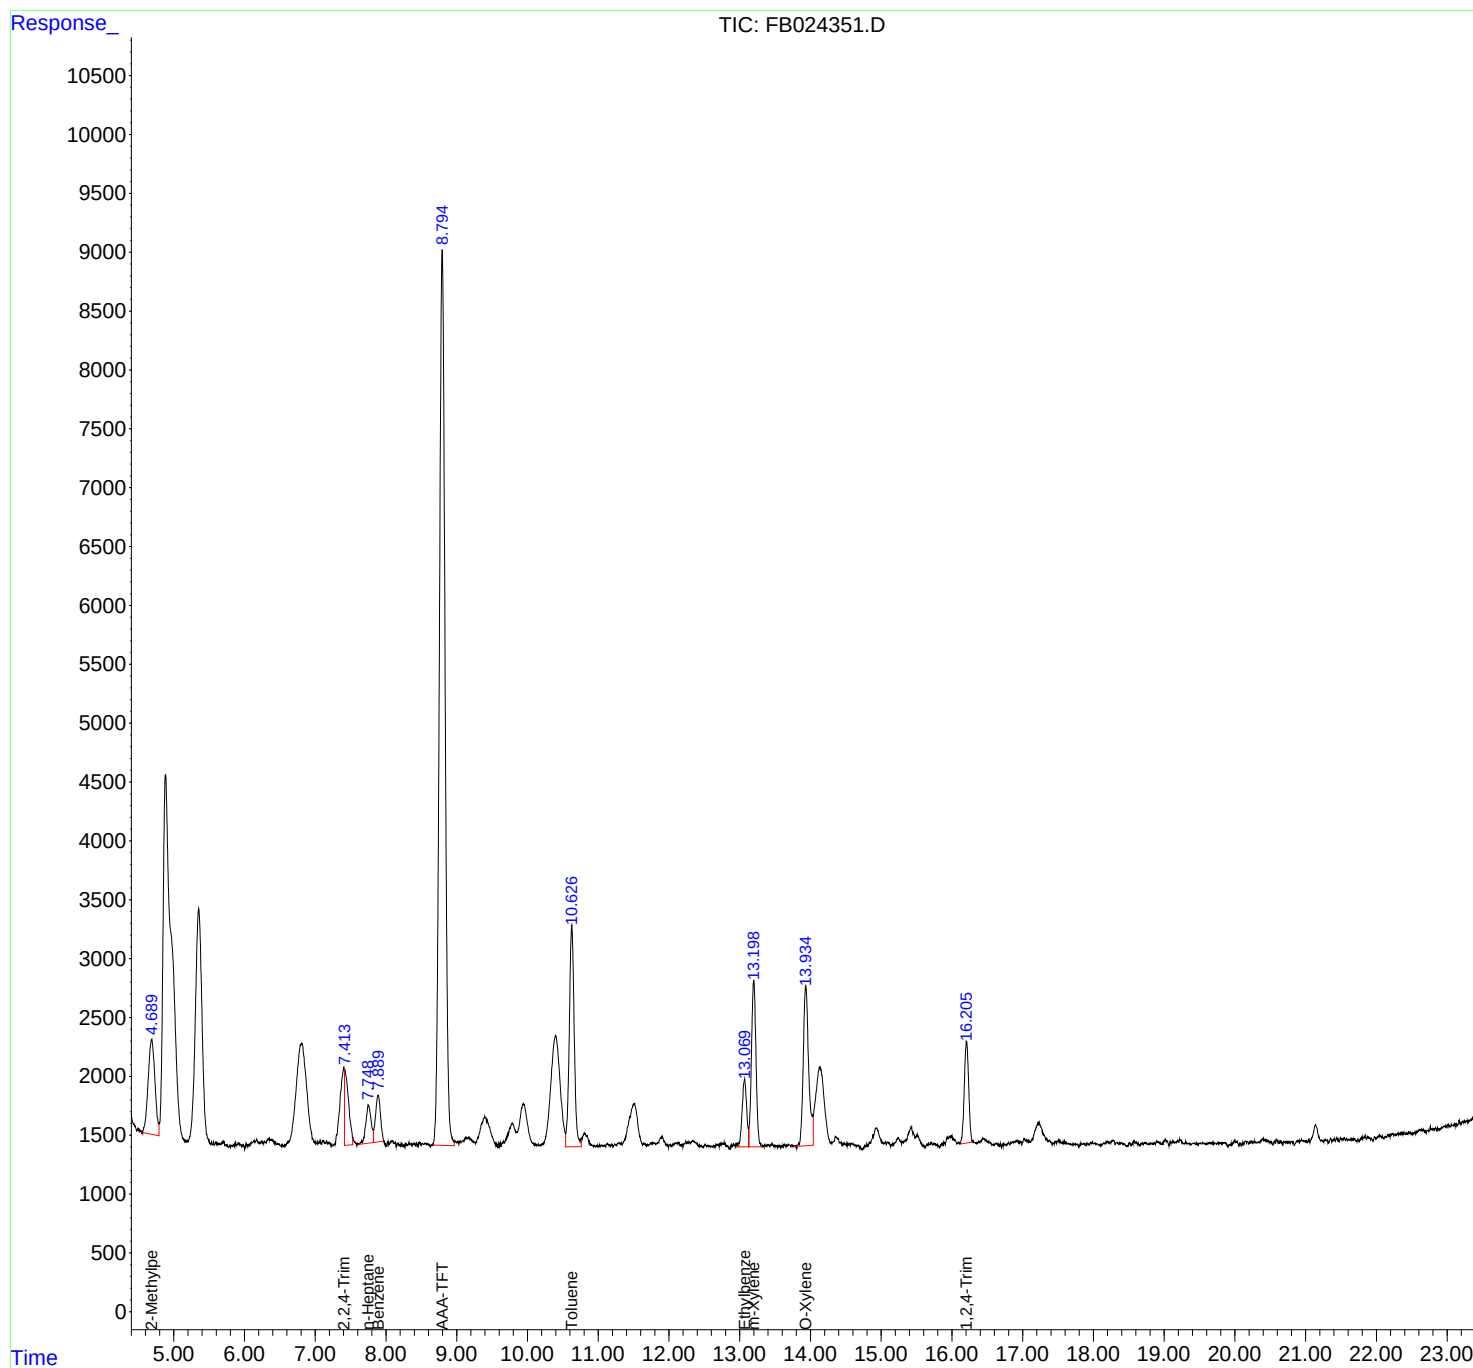


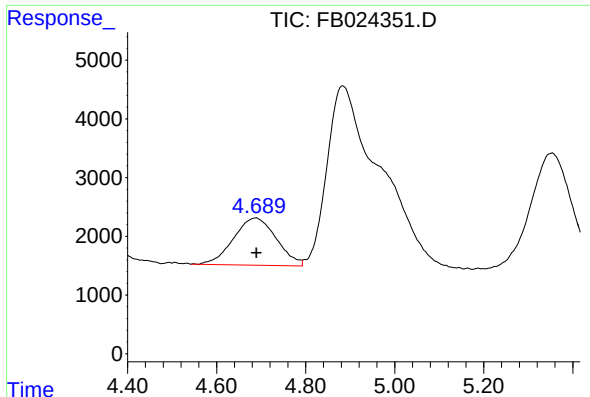

#1 2-Methylpentane


R.T.: 4.689 min
Delta R.T.: 0.000 min
Response: 53916
Conc: 1.83 ng/ml

Instrument :
FID_B
ClientSampleId :

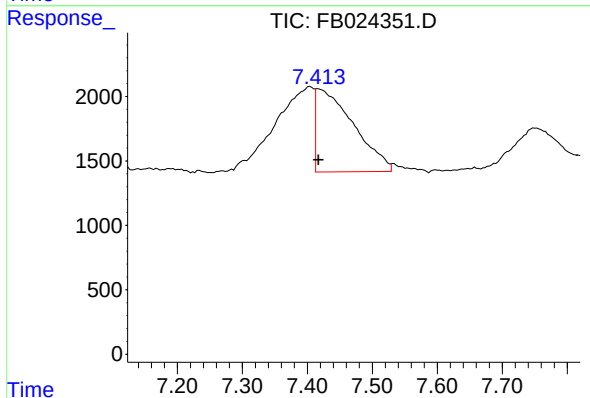


#2 2,2,4-Trimethylpentane

R.T.: 7.417 min
Delta R.T.: 0.000 min
Response: 25979
Conc: 0.85 ng/ml

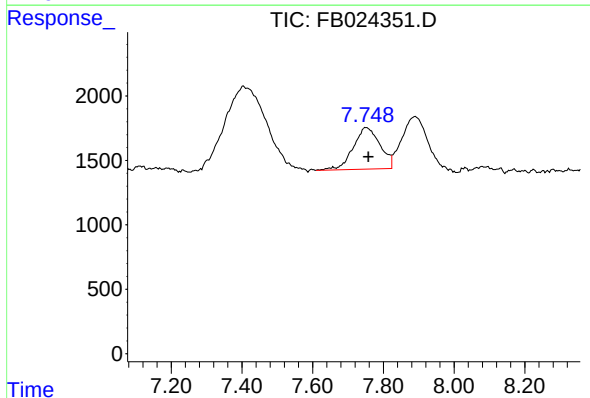


#3 n-Heptane

R.T.: 7.749 min
Delta R.T.: -0.008 min
Response: 16894
Conc: 0.56 ng/ml

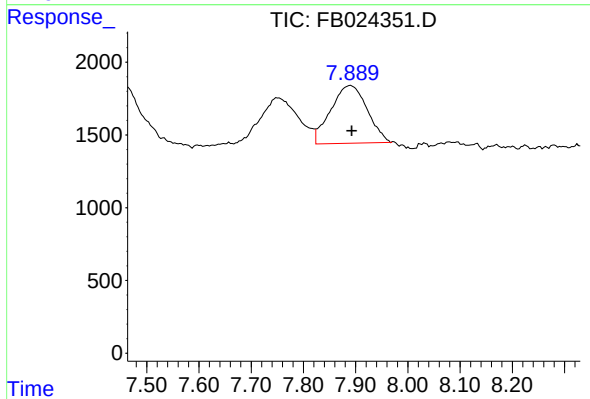

#4 Benzene


R.T.: 7.890 min
Delta R.T.: -0.002 min
Response: 19307
Conc: 0.51 ng/ml

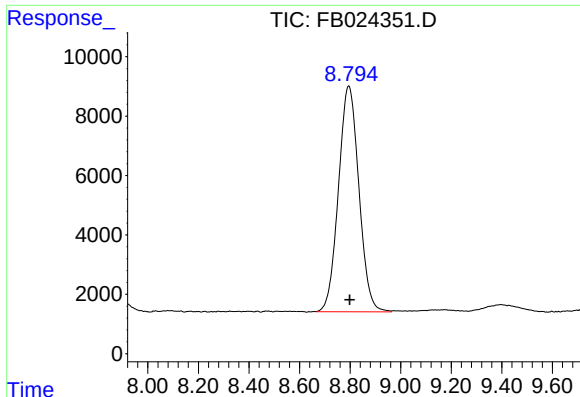

#5 AAA-TFT


R.T.: 8.795 min
Delta R.T.: -0.004 min
Response: 426148
Conc: 19.30 ng/ml

Instrument :
FID_B
ClientSampleId :

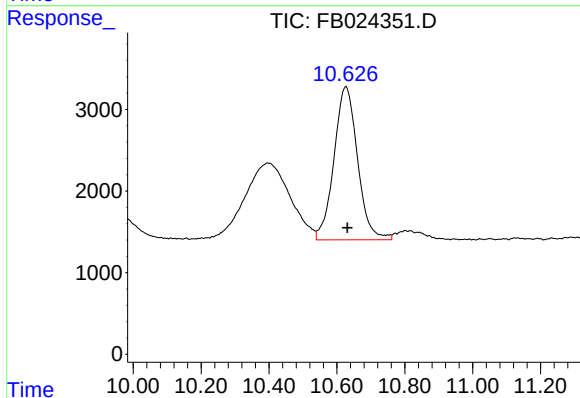


#6 Toluene

R.T.: 10.627 min
Delta R.T.: -0.004 min
Response: 90449
Conc: 2.50 ng/ml

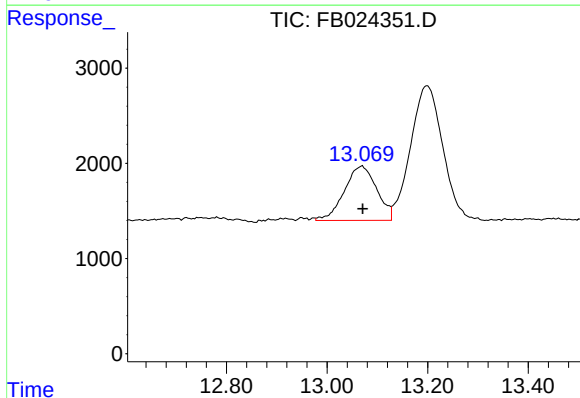


#7 Ethylbenzene

R.T.: 13.070 min
Delta R.T.: -0.001 min
Response: 25455
Conc: 0.75 ng/ml

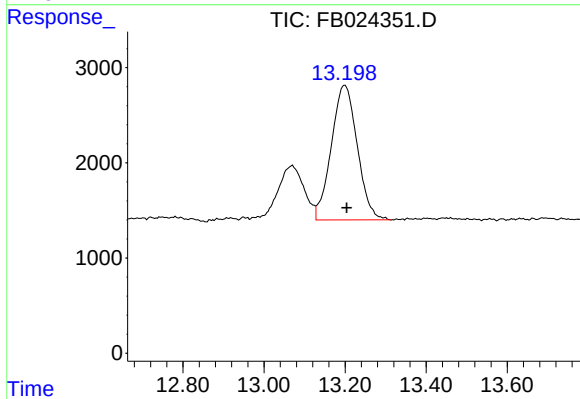

#8 m-Xylene


R.T.: 13.199 min
Delta R.T.: -0.005 min
Response: 62905
Conc: 1.91 ng/ml

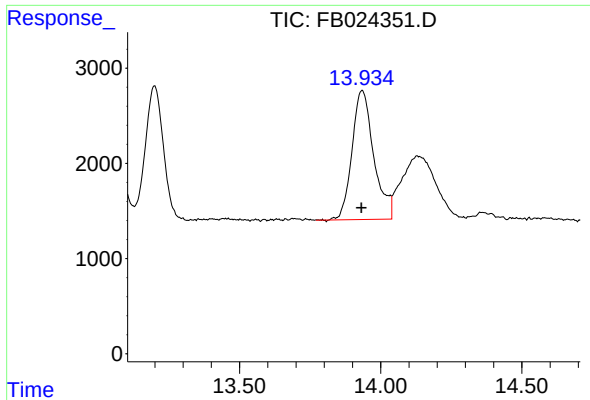

#9 O-Xylene

R.T.: 13.935 min
Delta R.T.: 0.003 min
Response: 72535
Conc: 2.25 ng/ml

Instrument :
FID_B
ClientSampleId :

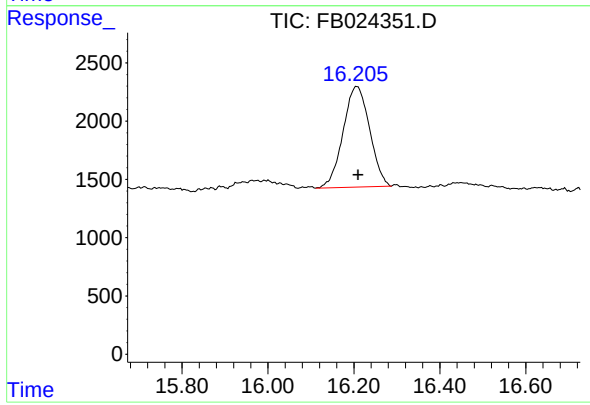

#10 1,2,4-Trimethylbenzene

R.T.: 16.207 min
Delta R.T.: -0.002 min
Response: 37037
Conc: 1.37 ng/ml