

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB051320\
 Data File : FB024343.D
 Signal(s) : FID2B.CH
 Acq On : 13 May 2020 10:21
 Operator : DD/AJ
 Sample : BSF0513S1
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0513S1

Integration File: Calibration.e
 Quant Time: May 14 04:28:22 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051120.M
 Quant Title :
 QLast Update : Mon May 11 11:14:42 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.796	466108	21.108 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.688	915502	31.023 ng/ml
2) t 2,2,4-Trimethylpentane	7.415	973237	31.858 ng/ml
3) t n-Heptane	7.755	321371	10.608 ng/ml
4) t Benzene	7.889	387262	10.244 ng/ml
6) t Toluene	10.626	1111251	30.667 ng/ml
7) t Ethylbenzene	13.067	327865	9.671 ng/ml
8) t m-Xylene	13.200	650101	19.700 ng/ml
9) t O-Xylene	13.927	628153	19.465 ng/ml
10) t 1,2,4-Trimethylbenzene	16.205	530083	19.655 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB051320\
Data File : FB024343.D
Signal(s) : FID2B.CH
Acq On : 13 May 2020 10:21
Operator : DD/AJ
Sample : BSF0513S1
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0513S1

Integration File: Calibration.e
Quant Time: May 14 04:28:22 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051120.M
Quant Title :
QLast Update : Mon May 11 11:14:42 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

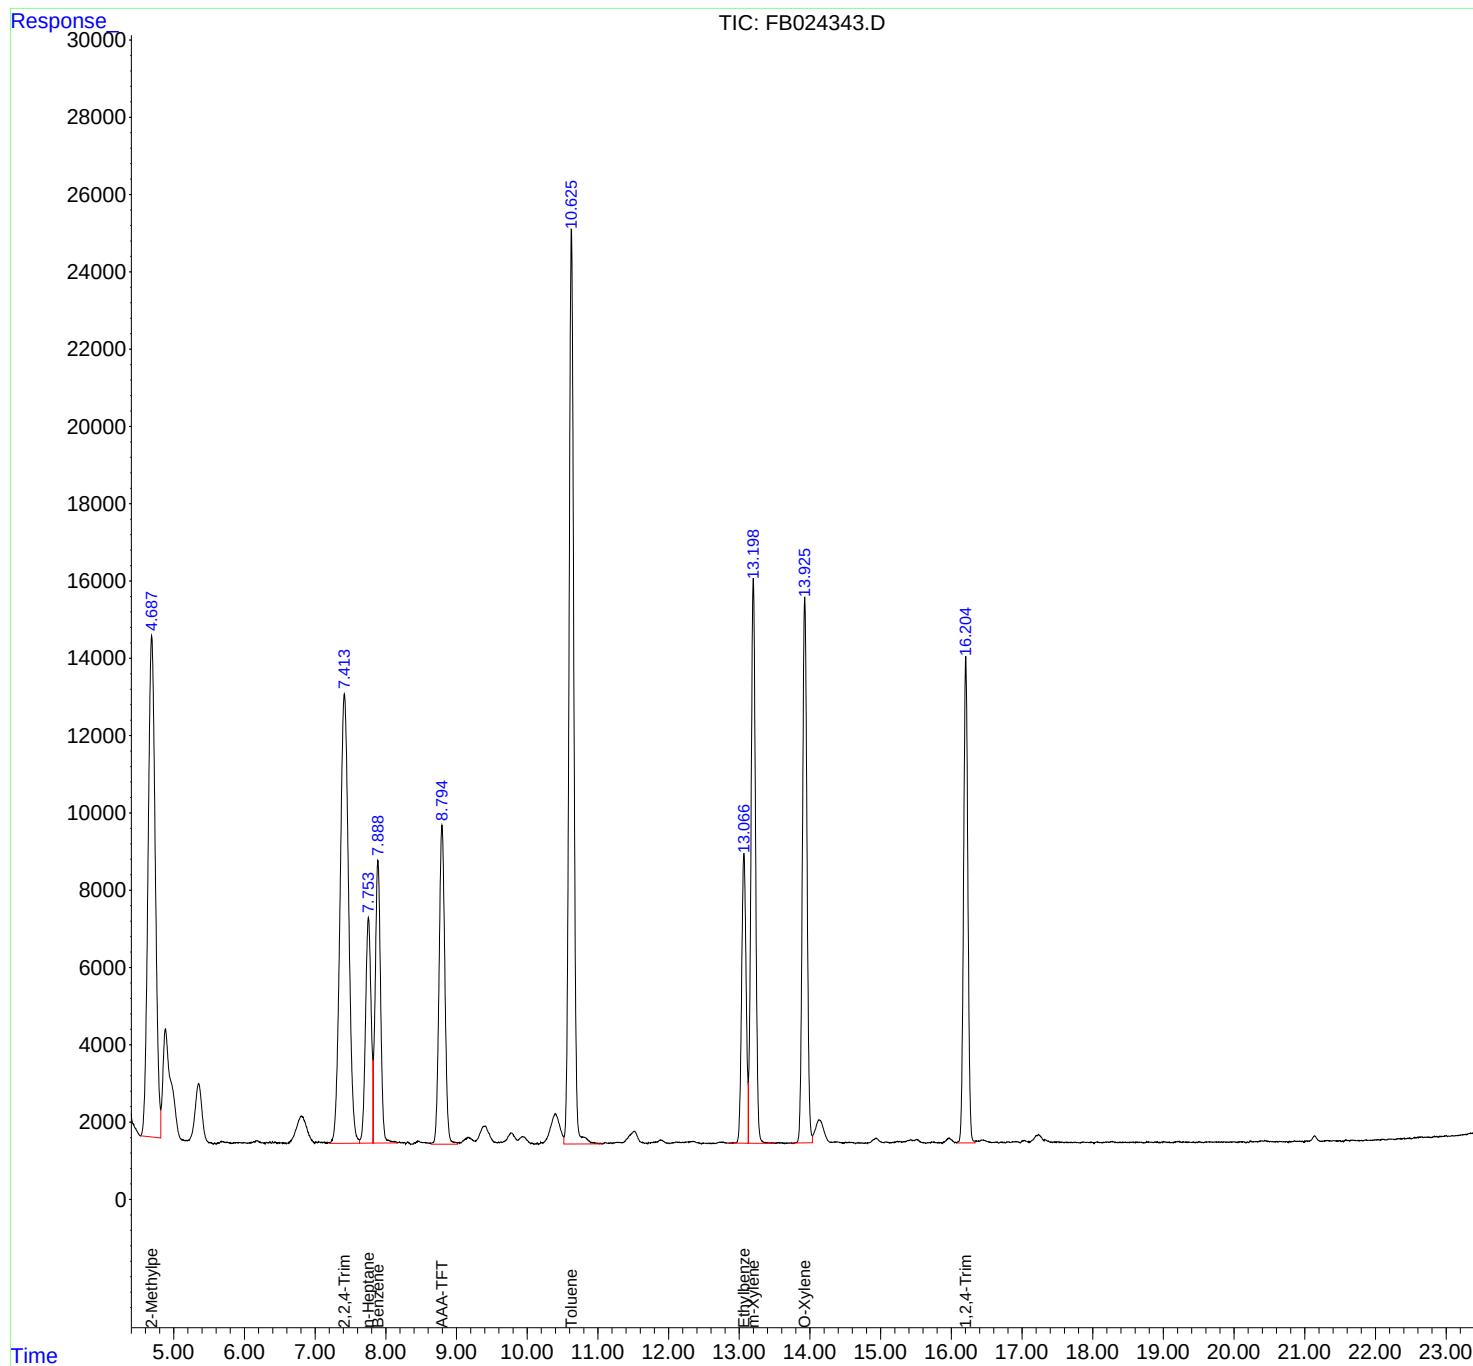


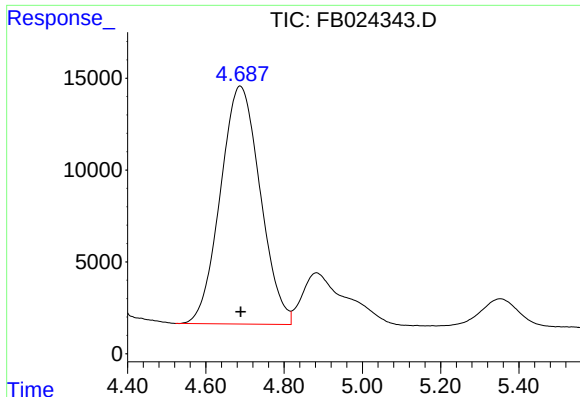

#1 2-Methylpentane


R.T.: 4.688 min
Delta R.T.: 0.000 min
Response: 915502
Conc: 31.02 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0513S1

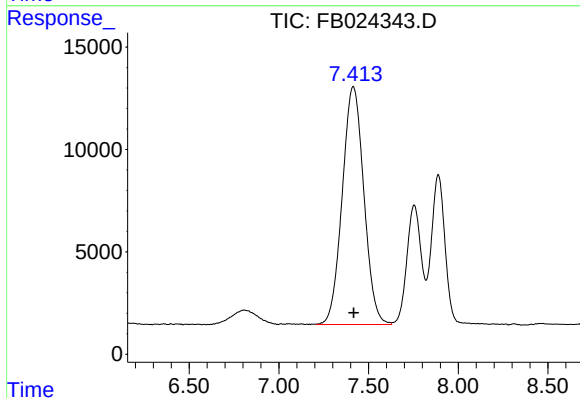


#2 2,2,4-Trimethylpentane

R.T.: 7.415 min
Delta R.T.: -0.002 min
Response: 973237
Conc: 31.86 ng/ml

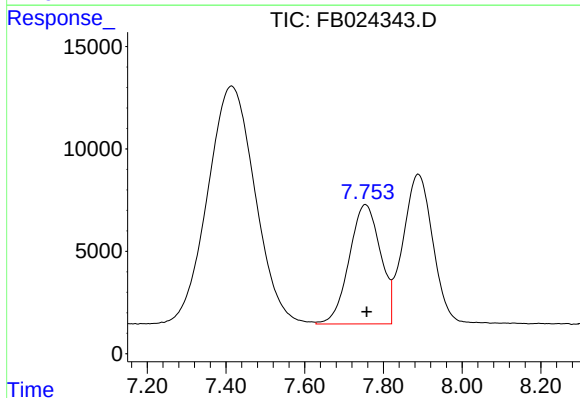


#3 n-Heptane

R.T.: 7.755 min
Delta R.T.: -0.003 min
Response: 321371
Conc: 10.61 ng/ml

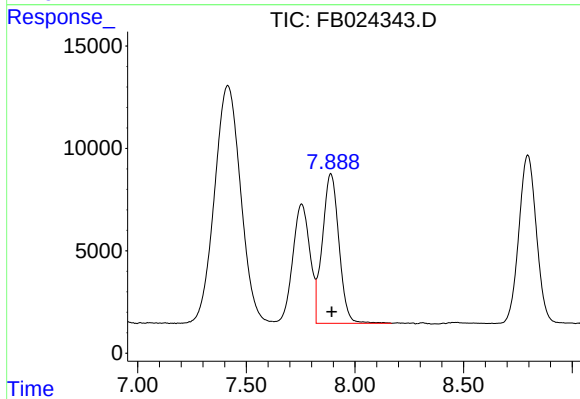

#4 Benzene


R.T.: 7.889 min
Delta R.T.: -0.004 min
Response: 387262
Conc: 10.24 ng/ml

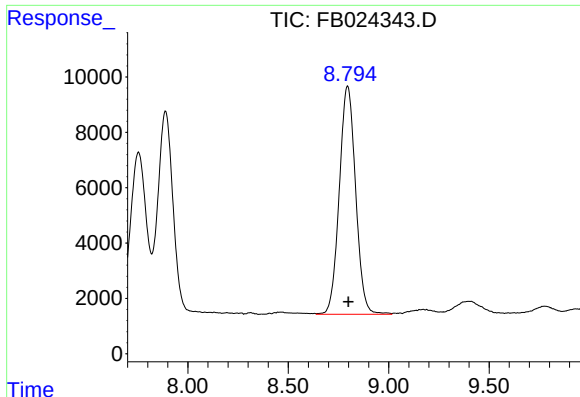

#5 AAA-TFT


R.T.: 8.796 min
Delta R.T.: -0.004 min
Response: 466108
Conc: 21.11 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0513S1

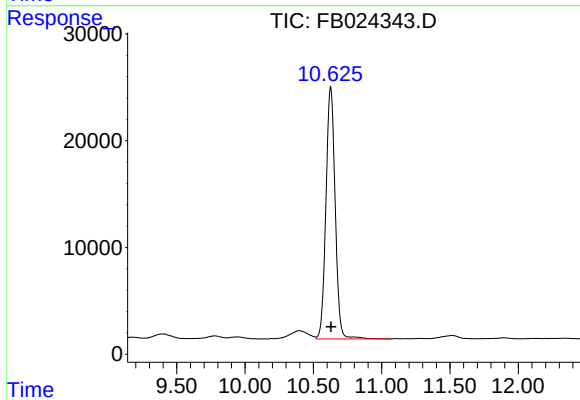


#6 Toluene

R.T.: 10.626 min
Delta R.T.: -0.004 min
Response: 1111251
Conc: 30.67 ng/ml

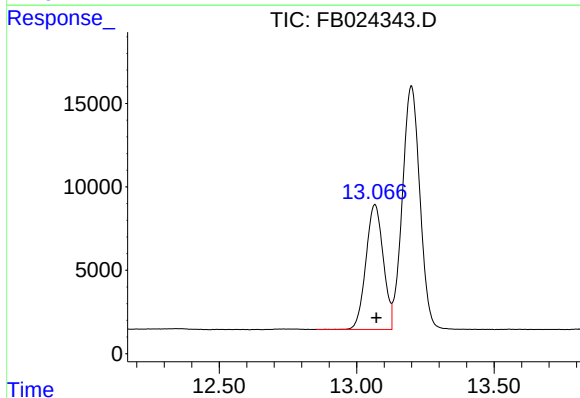


#7 Ethylbenzene

R.T.: 13.067 min
Delta R.T.: -0.005 min
Response: 327865
Conc: 9.67 ng/ml

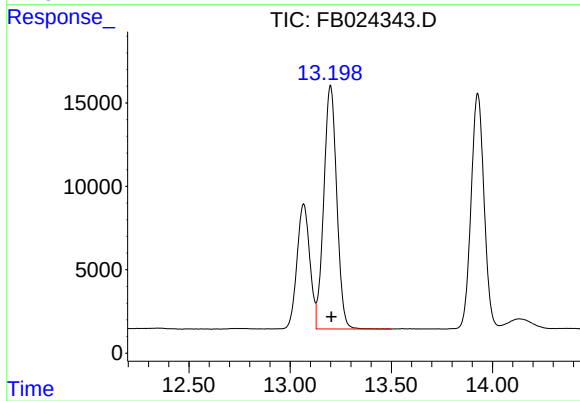

#8 m-Xylene


R.T.: 13.200 min
Delta R.T.: -0.005 min
Response: 650101
Conc: 19.70 ng/ml

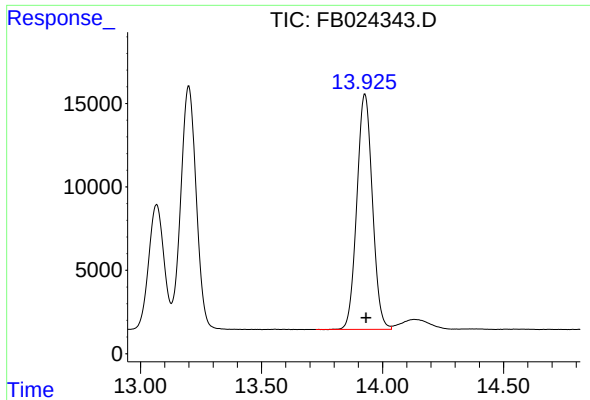

#9 O-Xylene

R.T.: 13.927 min
Delta R.T.: -0.005 min
Response: 628153
Conc: 19.47 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0513S1

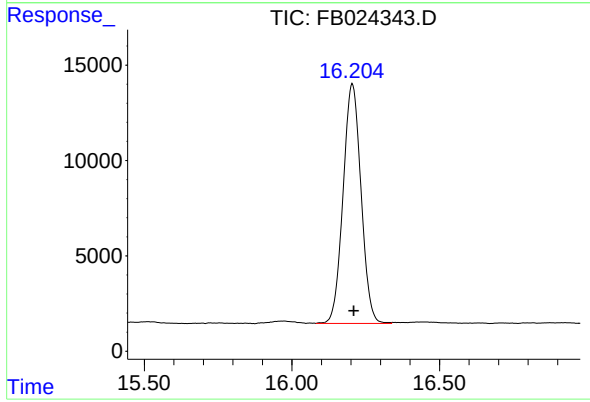

#10 1,2,4-Trimethylbenzene

R.T.: 16.205 min
Delta R.T.: -0.005 min
Response: 530083
Conc: 19.65 ng/ml