

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB051320\
 Data File : FB024348.D
 Signal(s) : FID2B.CH
 Acq On : 13 May 2020 13:13
 Operator : DD/AJ
 Sample : L2500-02MS
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 OK-02-051220MS

Integration File: Calibration.e
 Quant Time: May 14 04:28:58 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051120.M
 Quant Title :
 QLast Update : Mon May 11 11:14:42 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.797	494797	22.407 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.689	867668	29.402 ng/ml
2) t 2,2,4-Trimethylpentane	7.415	882287	28.881 ng/ml
3) t n-Heptane	7.756	288451	9.521 ng/ml
4) t Benzene	7.890	370093	9.789 ng/ml
6) t Toluene	10.628	1075022	29.667 ng/ml
7) t Ethylbenzene	13.068	321112	9.472 ng/ml
8) t m-Xylene	13.201	633781	19.206 ng/ml
9) t O-Xylene	13.928	620400	19.225 ng/ml
10) t 1,2,4-Trimethylbenzene	16.206	511724	18.974 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB051320\
Data File : FB024348.D
Signal(s) : FID2B.CH
Acq On : 13 May 2020 13:13
Operator : DD/AJ
Sample : L2500-02MS
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
OK-02-051220MS

Integration File: Calibration.e
Quant Time: May 14 04:28:58 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051120.M
Quant Title :
QLast Update : Mon May 11 11:14:42 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

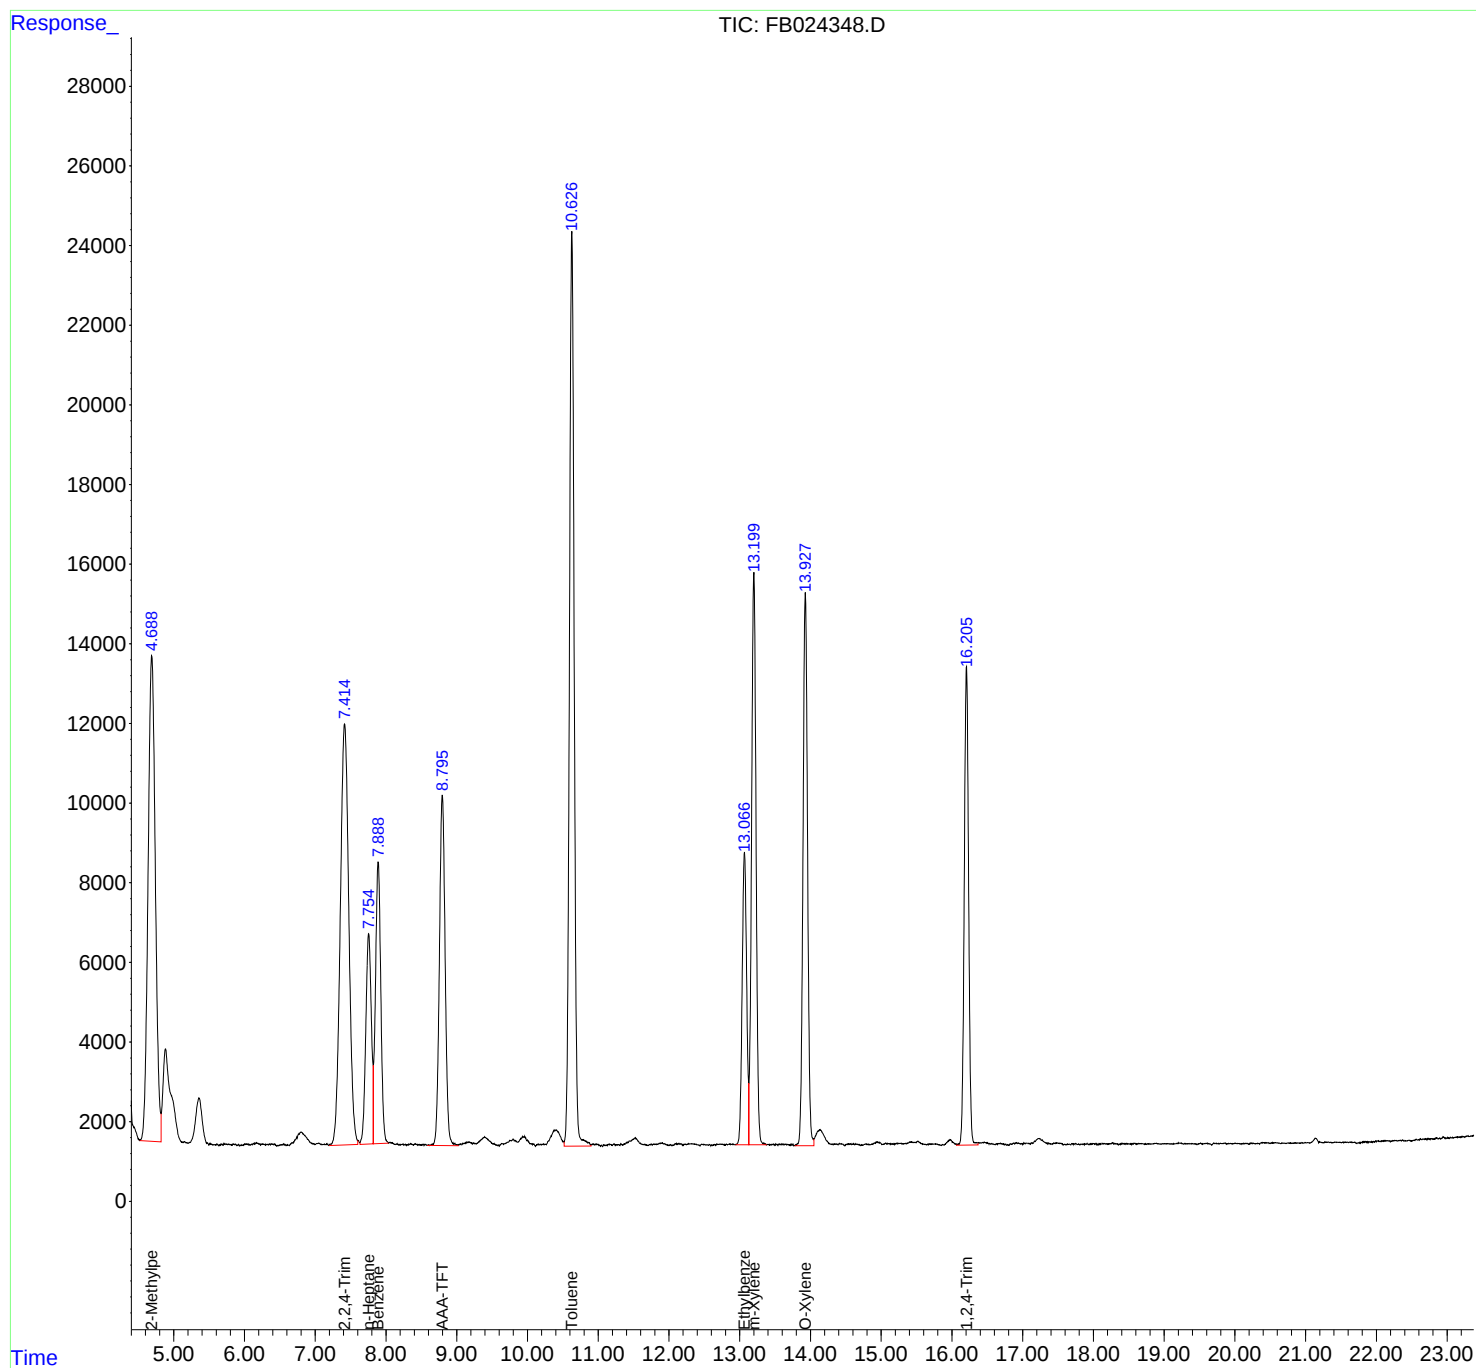


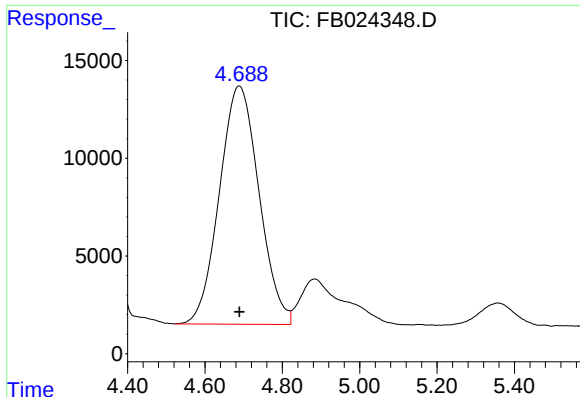

#1 2-Methylpentane


R.T.: 4.689 min
Delta R.T.: 0.000 min
Response: 867668
Conc: 29.40 ng/ml

Instrument :
FID_B
ClientSampleId :
OK-02-051220MS

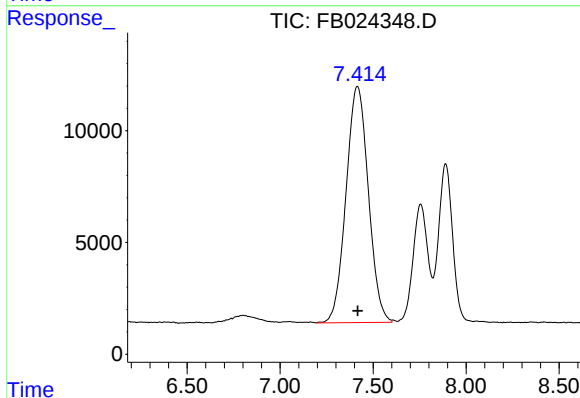


#2 2,2,4-Trimethylpentane

R.T.: 7.415 min
Delta R.T.: -0.002 min
Response: 882287
Conc: 28.88 ng/ml

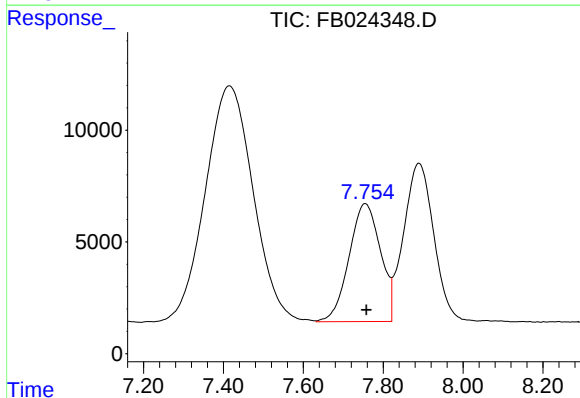


#3 n-Heptane

R.T.: 7.756 min
Delta R.T.: -0.002 min
Response: 288451
Conc: 9.52 ng/ml

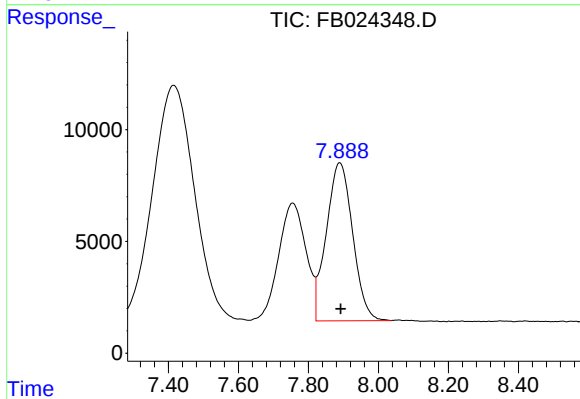

#4 Benzene


R.T.: 7.890 min
Delta R.T.: -0.003 min
Response: 370093
Conc: 9.79 ng/ml

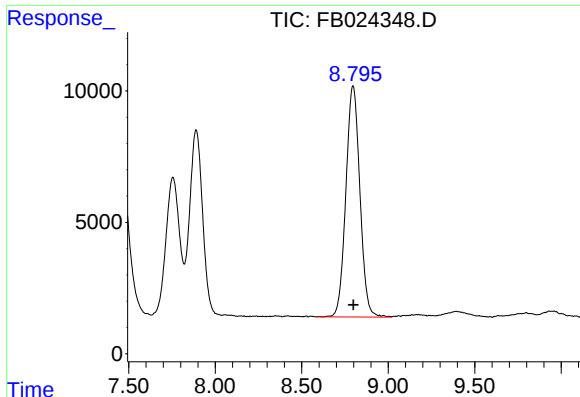

#5 AAA-TFT


R.T.: 8.797 min
Delta R.T.: -0.002 min
Response: 494797
Conc: 22.41 ng/ml

Instrument :
FID_B
ClientSampleId :
OK-02-051220MS

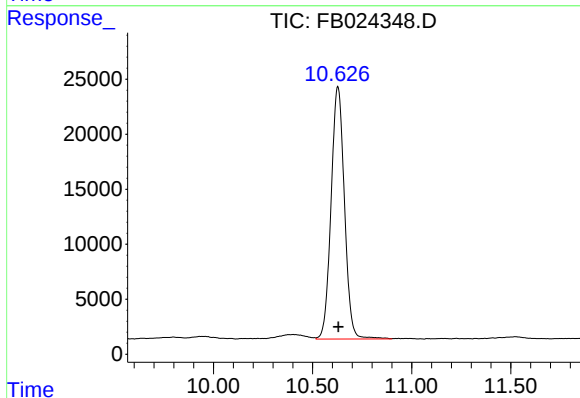


#6 Toluene

R.T.: 10.628 min
Delta R.T.: -0.003 min
Response: 1075022
Conc: 29.67 ng/ml

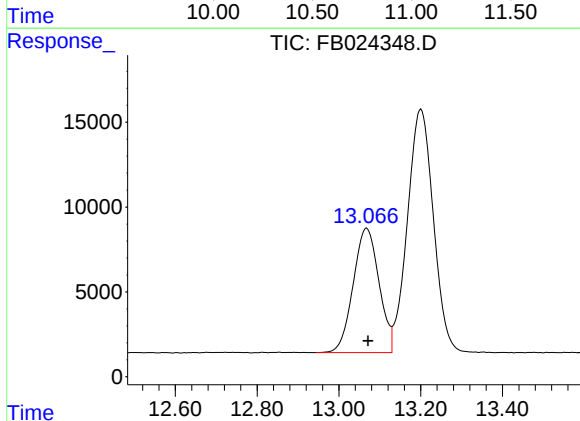


#7 Ethylbenzene

R.T.: 13.068 min
Delta R.T.: -0.003 min
Response: 321112
Conc: 9.47 ng/ml

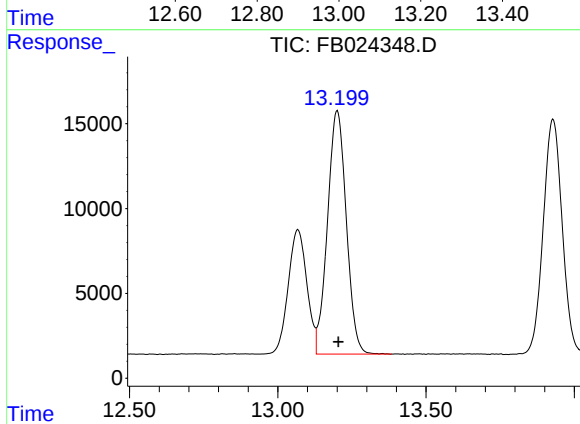

#8 m-Xylene


R.T.: 13.201 min
Delta R.T.: -0.004 min
Response: 633781
Conc: 19.21 ng/ml

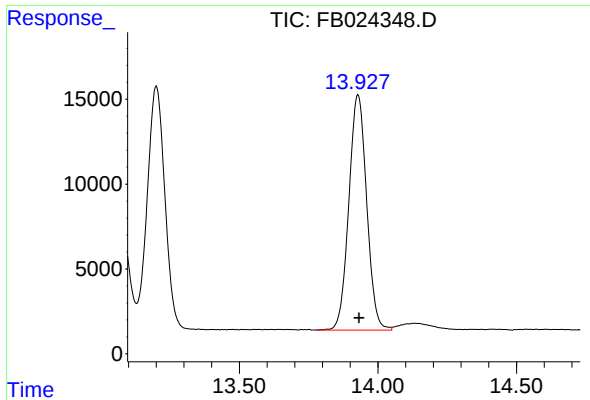

#9 O-Xylene

R.T.: 13.928 min
Delta R.T.: -0.004 min
Response: 620400
Conc: 19.23 ng/ml

Instrument :
FID_B
ClientSampleId :
OK-02-051220MS

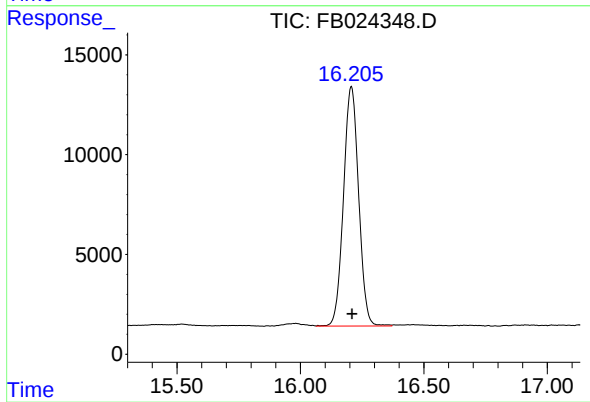

#10 1,2,4-Trimethylbenzene

R.T.: 16.206 min
Delta R.T.: -0.003 min
Response: 511724
Conc: 18.97 ng/ml