

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB051320\
 Data File : FB024349.D
 Signal(s) : FID2B.CH
 Acq On : 13 May 2020 13:43
 Operator : DD/AJ
 Sample : L2500-02MSD
 Misc : 5.03g/5.00ml DI WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 OK-02-051220MSD

Integration File: Calibration.e
 Quant Time: May 14 04:29:05 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051120.M
 Quant Title :
 QLast Update : Mon May 11 11:14:42 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.797	496119	22.467 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.689	795321	26.951 ng/ml
2) t 2,2,4-Trimethylpentane	7.416	788576	25.813 ng/ml
3) t n-Heptane	7.755	256805	8.477 ng/ml
4) t Benzene	7.891	376399	9.956 ng/ml
6) t Toluene	10.628	1041003	28.728 ng/ml
7) t Ethylbenzene	13.068	308113	9.088 ng/ml
8) t m-Xylene	13.201	606503	18.379 ng/ml
9) t O-Xylene	13.928	590986	18.314 ng/ml
10) t 1,2,4-Trimethylbenzene	16.207	469908	17.424 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB051320\
Data File : FB024349.D
Signal(s) : FID2B.CH
Acq On : 13 May 2020 13:43
Operator : DD/AJ
Sample : L2500-02MSD
Misc : 5.03g/5.00ml DI WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
OK-02-051220MSD

Integration File: Calibration.e
Quant Time: May 14 04:29:05 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051120.M
Quant Title :
QLast Update : Mon May 11 11:14:42 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

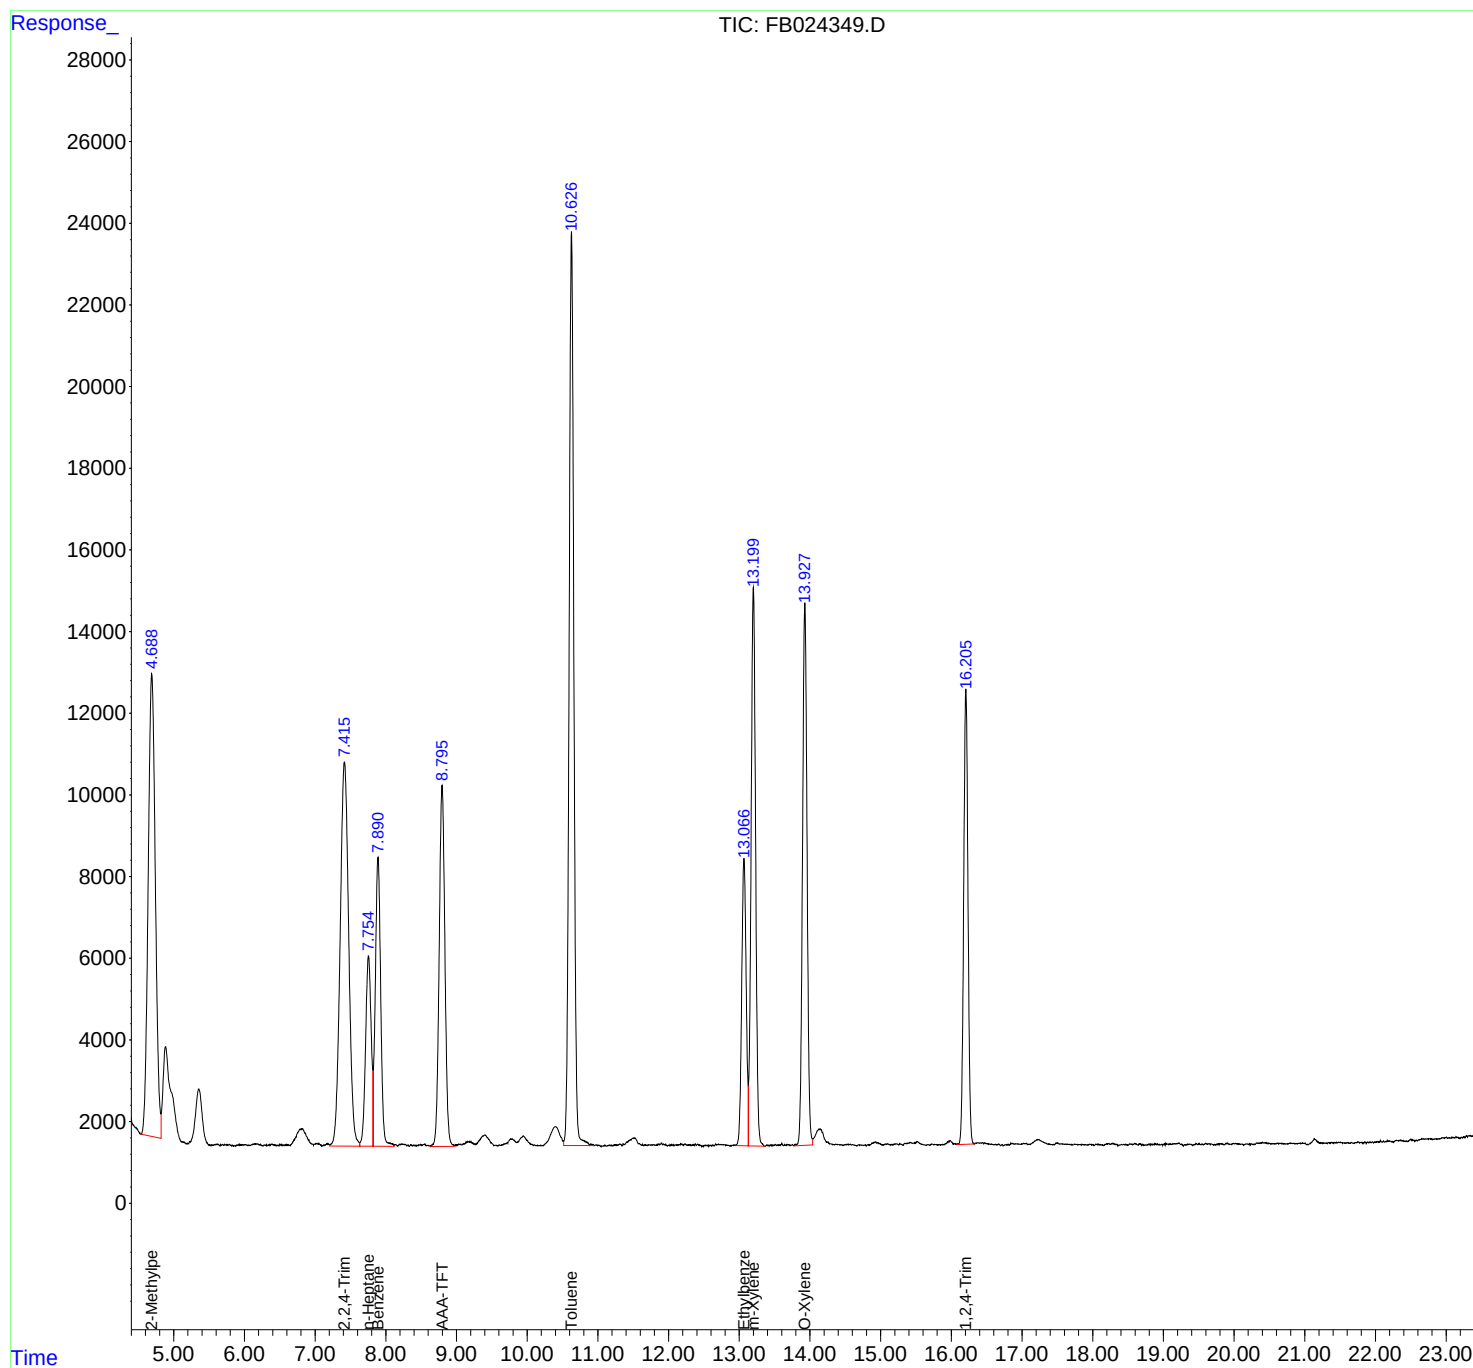


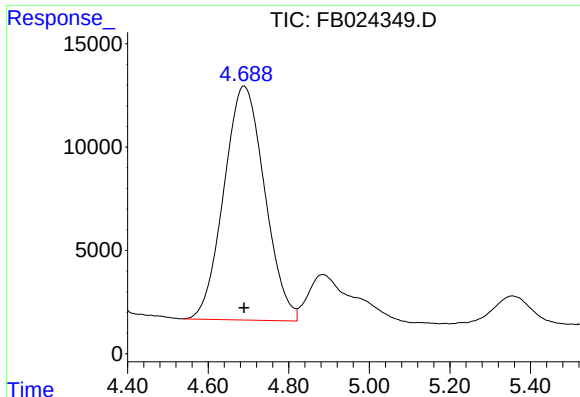

#1 2-Methylpentane


R.T.: 4.689 min
Delta R.T.: 0.000 min
Response: 795321
Conc: 26.95 ng/ml

Instrument :
FID_B
ClientSampleId :
OK-02-051220MSD

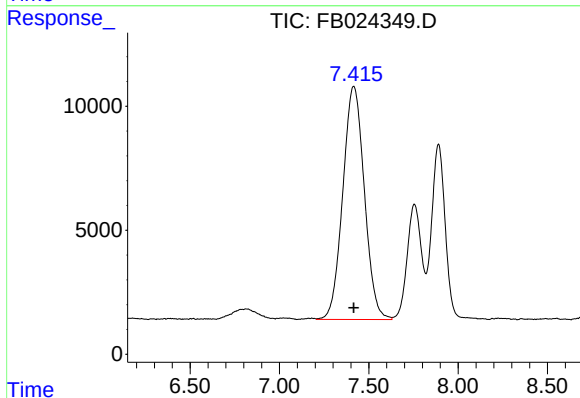


#2 2,2,4-Trimethylpentane

R.T.: 7.416 min
Delta R.T.: -0.001 min
Response: 788576
Conc: 25.81 ng/ml

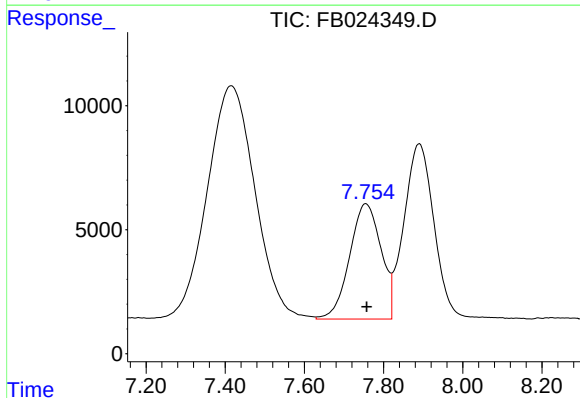


#3 n-Heptane

R.T.: 7.755 min
Delta R.T.: -0.003 min
Response: 256805
Conc: 8.48 ng/ml

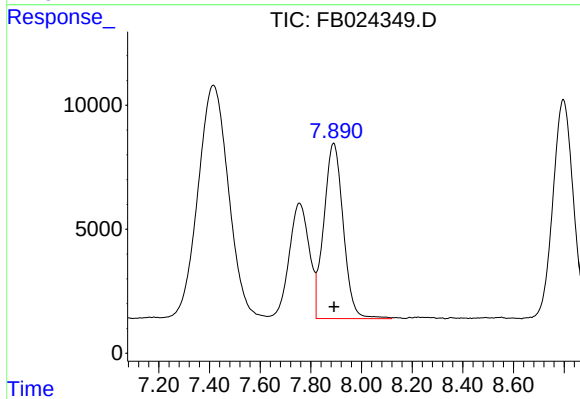

#4 Benzene


R.T.: 7.891 min
Delta R.T.: -0.002 min
Response: 376399
Conc: 9.96 ng/ml

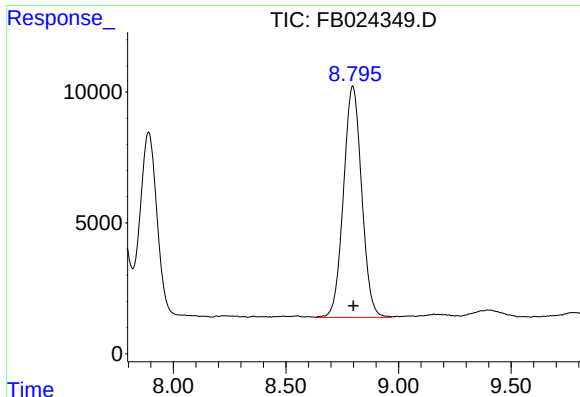

#5 AAA-TFT


R.T.: 8.797 min
Delta R.T.: -0.002 min
Response: 496119
Conc: 22.47 ng/ml

Instrument :
FID_B
ClientSampleId :
OK-02-051220MSD

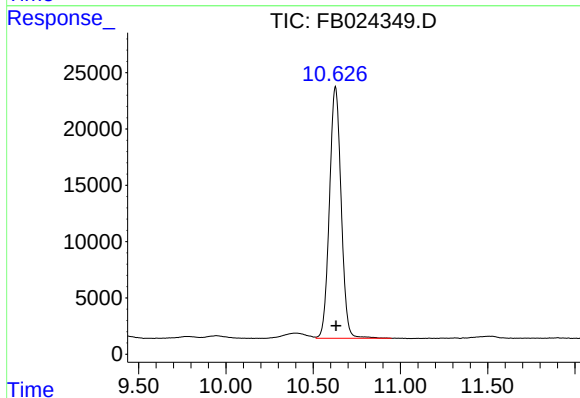


#6 Toluene

R.T.: 10.628 min
Delta R.T.: -0.003 min
Response: 1041003
Conc: 28.73 ng/ml

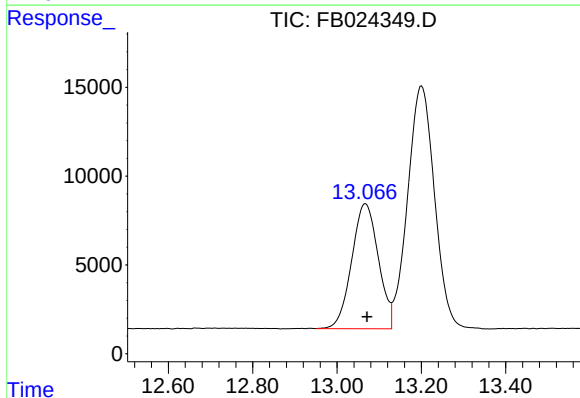


#7 Ethylbenzene

R.T.: 13.068 min
Delta R.T.: -0.004 min
Response: 308113
Conc: 9.09 ng/ml

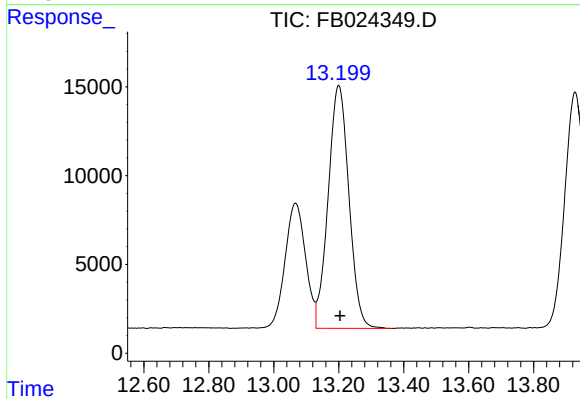

#8 m-Xylene


R.T.: 13.201 min
Delta R.T.: -0.004 min
Response: 606503
Conc: 18.38 ng/ml

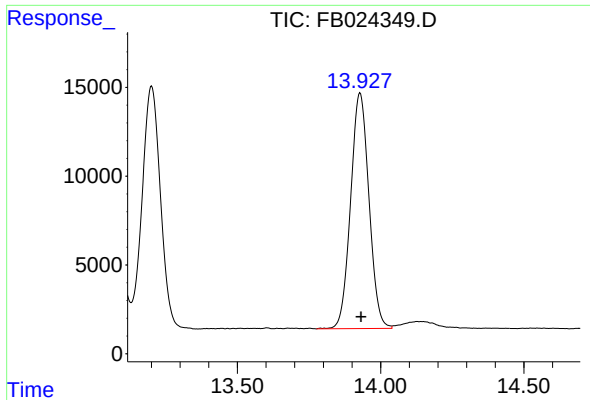

#9 O-Xylene

R.T.: 13.928 min
Delta R.T.: -0.004 min
Response: 590986
Conc: 18.31 ng/ml

Instrument :
FID_B
ClientSampleId :
OK-02-051220MSD

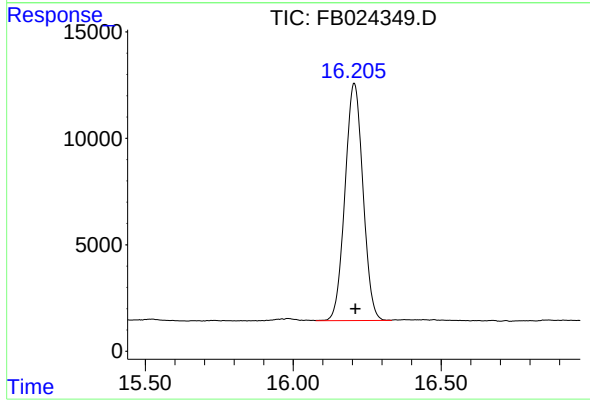

#10 1,2,4-Trimethylbenzene

R.T.: 16.207 min
Delta R.T.: -0.003 min
Response: 469908
Conc: 17.42 ng/ml