

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB051320\
 Data File : FB024354.D
 Signal(s) : FID2B.CH
 Acq On : 13 May 2020 17:24
 Operator : DD/AJ
 Sample : L2182-07
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 LOD-MDL-WATER-01-QT2-2020

Integration File: Calibration.e
 Quant Time: May 14 04:42:27 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051120.M
 Quant Title :
 QLast Update : Mon May 11 11:14:42 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.801	383262	17.356 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.689	54350	1.842 ng/ml
2) t 2,2,4-Trimethylpentane	7.419	51848	1.697 ng/ml
3) t n-Heptane	7.756	15371	0.507 ng/ml
4) t Benzene	7.902	20871	0.552 ng/ml
6) t Toluene	10.633	66342	1.831 ng/ml
7) t Ethylbenzene	13.071	24944	0.736 ng/ml
8) t m-Xylene	13.204	46085	1.397 ng/ml
9) t O-Xylene	13.936	51290	1.589 ng/ml
10) t 1,2,4-Trimethylbenzene	16.210	34455	1.278 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB051320\
Data File : FB024354.D
Signal(s) : FID2B.CH
Acq On : 13 May 2020 17:24
Operator : DD/AJ
Sample : L2182-07
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
LOD-MDL-WATER-01-QT2-2020

Integration File: Calibration.e
Quant Time: May 14 04:42:27 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051120.M
Quant Title :
QLast Update : Mon May 11 11:14:42 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

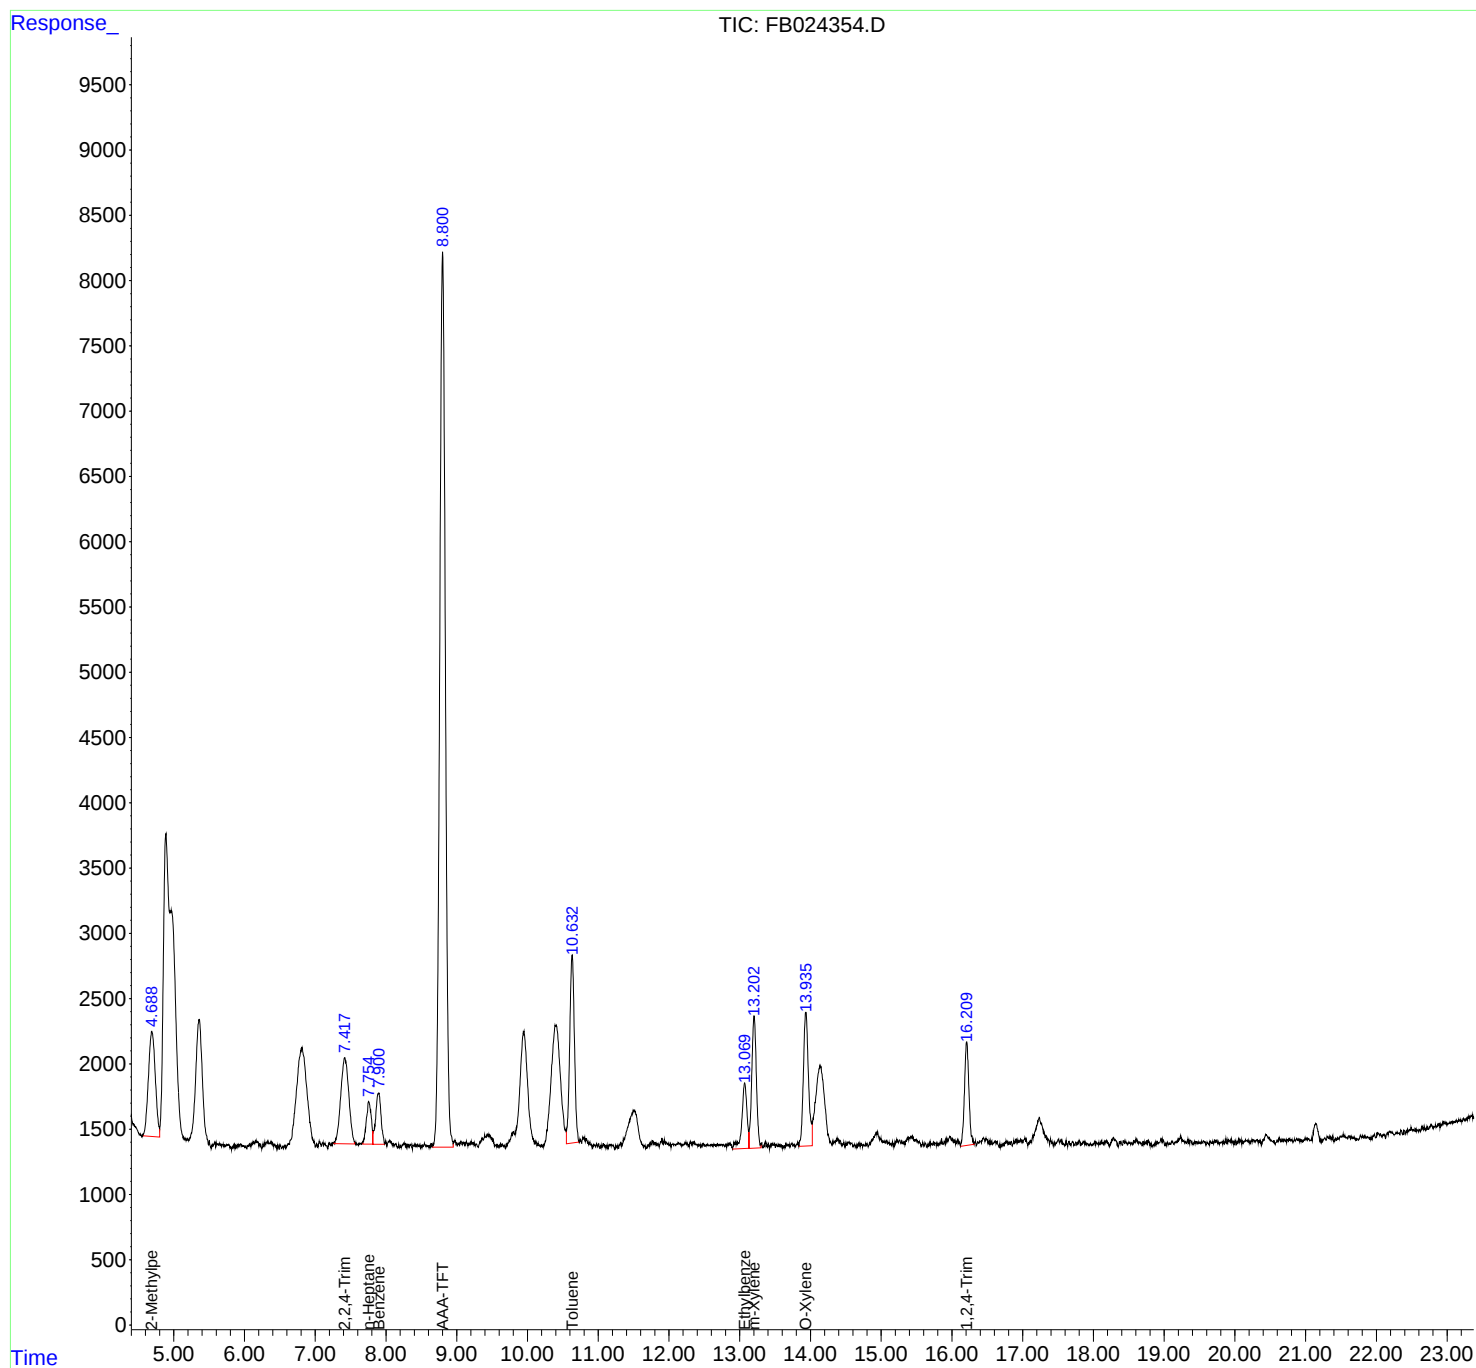


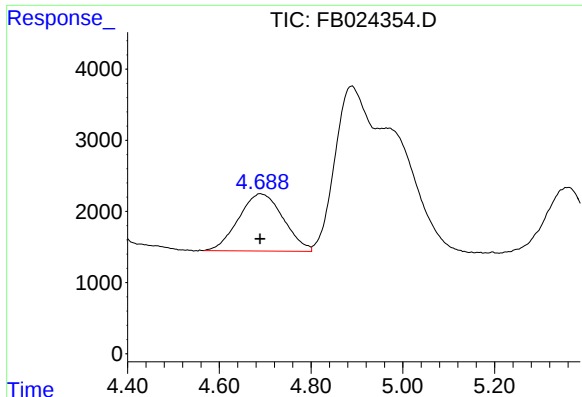

#1 2-Methylpentane


R.T.: 4.689 min
Delta R.T.: 0.000 min
Response: 54350
Conc: 1.84 ng/ml

Instrument :
FID_B
ClientSampleId :
LOD-MDL-WATER-01-QT2-2020

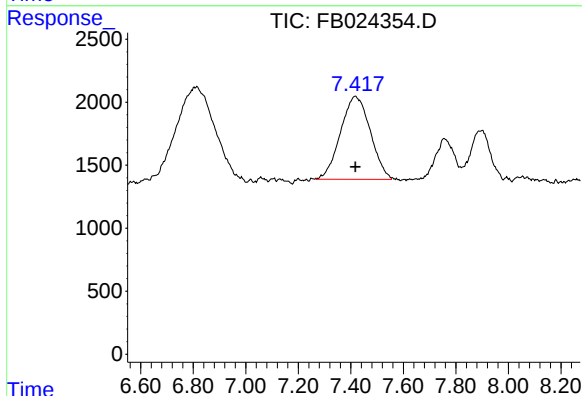


#2 2,2,4-Trimethylpentane

R.T.: 7.419 min
Delta R.T.: 0.002 min
Response: 51848
Conc: 1.70 ng/ml

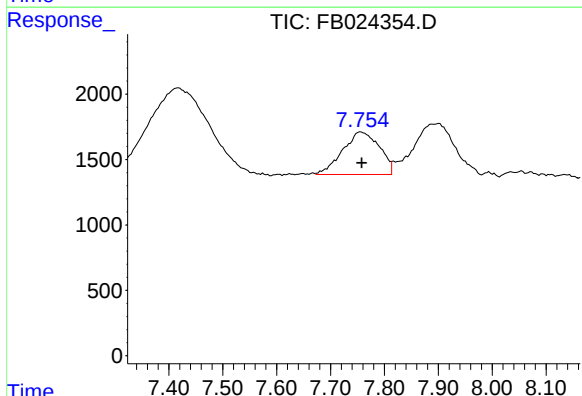


#3 n-Heptane

R.T.: 7.756 min
Delta R.T.: -0.002 min
Response: 15371
Conc: 0.51 ng/ml

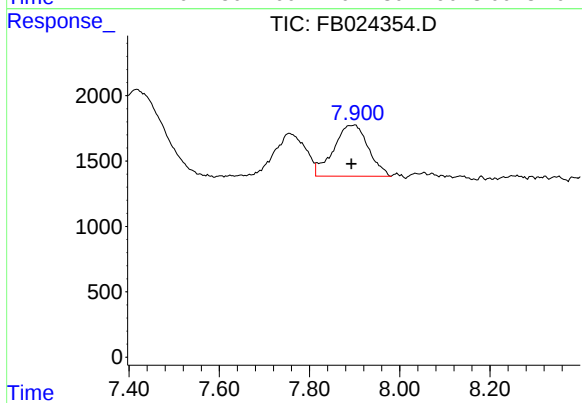

#4 Benzene


R.T.: 7.902 min
Delta R.T.: 0.009 min
Response: 20871
Conc: 0.55 ng/ml

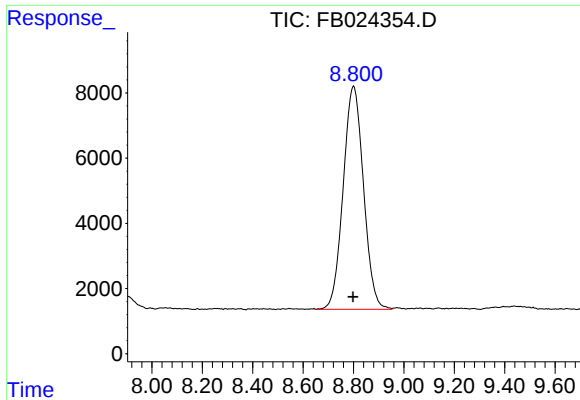

#5 AAA-TFT


R.T.: 8.801 min
Delta R.T.: 0.002 min
Response: 383262
Conc: 17.36 ng/ml

Instrument :
FID_B
ClientSampleId :
LOD-MDL-WATER-01-QT2-2020

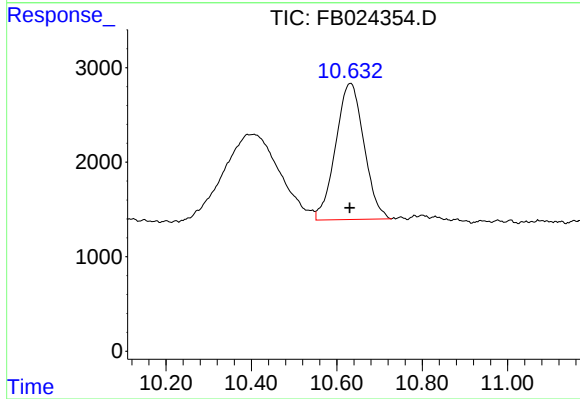


#6 Toluene

R.T.: 10.633 min
Delta R.T.: 0.003 min
Response: 66342
Conc: 1.83 ng/ml

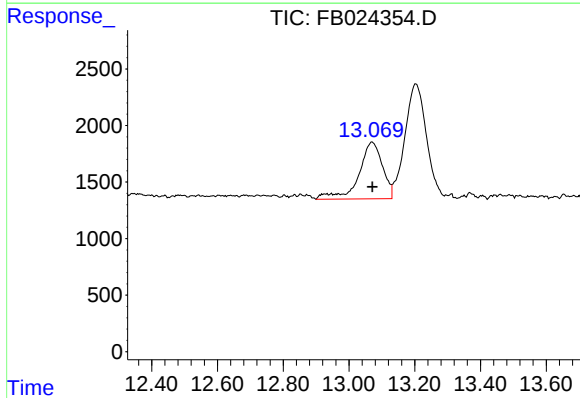


#7 Ethylbenzene

R.T.: 13.071 min
Delta R.T.: 0.000 min
Response: 24944
Conc: 0.74 ng/ml

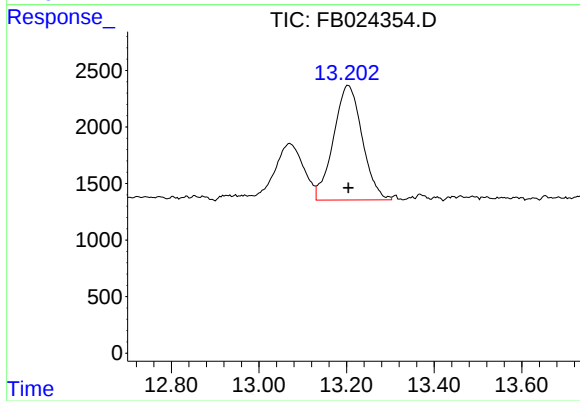

#8 m-Xylene


R.T.: 13.204 min
Delta R.T.: 0.000 min
Response: 46085
Conc: 1.40 ng/ml

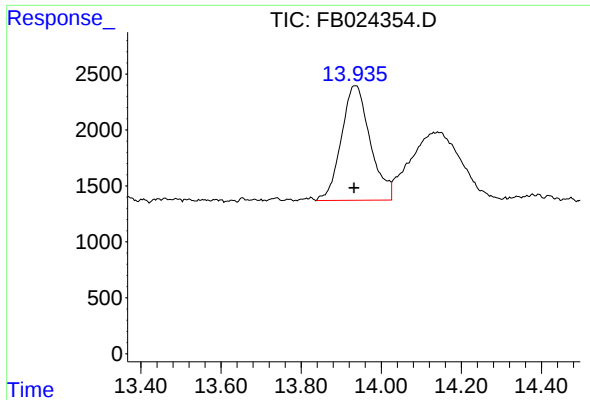

#9 O-Xylene

R.T.: 13.936 min
Delta R.T.: 0.004 min
Response: 51290
Conc: 1.59 ng/ml

Instrument :
FID_B
ClientSampleId :
LOD-MDL-WATER-01-QT2-2020

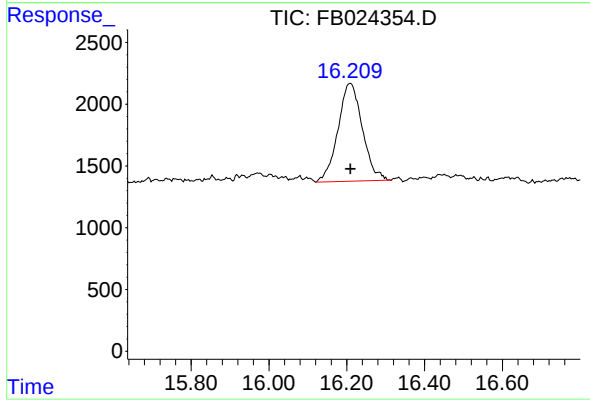

#10 1,2,4-Trimethylbenzene

R.T.: 16.210 min
Delta R.T.: 0.000 min
Response: 34455
Conc: 1.28 ng/ml