

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB051320\
 Data File : FB024355.D
 Signal(s) : FID2B.CH
 Acq On : 13 May 2020 17:54
 Operator : DD/AJ
 Sample : L2182-07
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 LOD-MDL-WATER-01-QT2-2020

Integration File: Calibration.e
 Quant Time: May 14 04:29:52 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051120.M
 Quant Title :
 QLast Update : Mon May 11 11:14:42 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.801	428701	19.414 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.694	203406	6.893 ng/ml
2) t 2,2,4-Trimethylpentane	7.420	213635	6.993 ng/ml
3) t n-Heptane	7.759	68209	2.251 ng/ml
4) t Benzene	7.893	79765	2.110 ng/ml
6) t Toluene	10.632	242367	6.688 ng/ml
7) t Ethylbenzene	13.072	75082	2.215 ng/ml
8) t m-Xylene	13.204	153173	4.642 ng/ml
9) t O-Xylene	13.932	157671	4.886 ng/ml
10) t 1,2,4-Trimethylbenzene	16.210	121965	4.522 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB051320\
Data File : FB024355.D
Signal(s) : FID2B.CH
Acq On : 13 May 2020 17:54
Operator : DD/AJ
Sample : L2182-07
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
LOD-MDL-WATER-01-QT2-2020

Integration File: Calibration.e
Quant Time: May 14 04:29:52 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051120.M
Quant Title :
QLast Update : Mon May 11 11:14:42 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

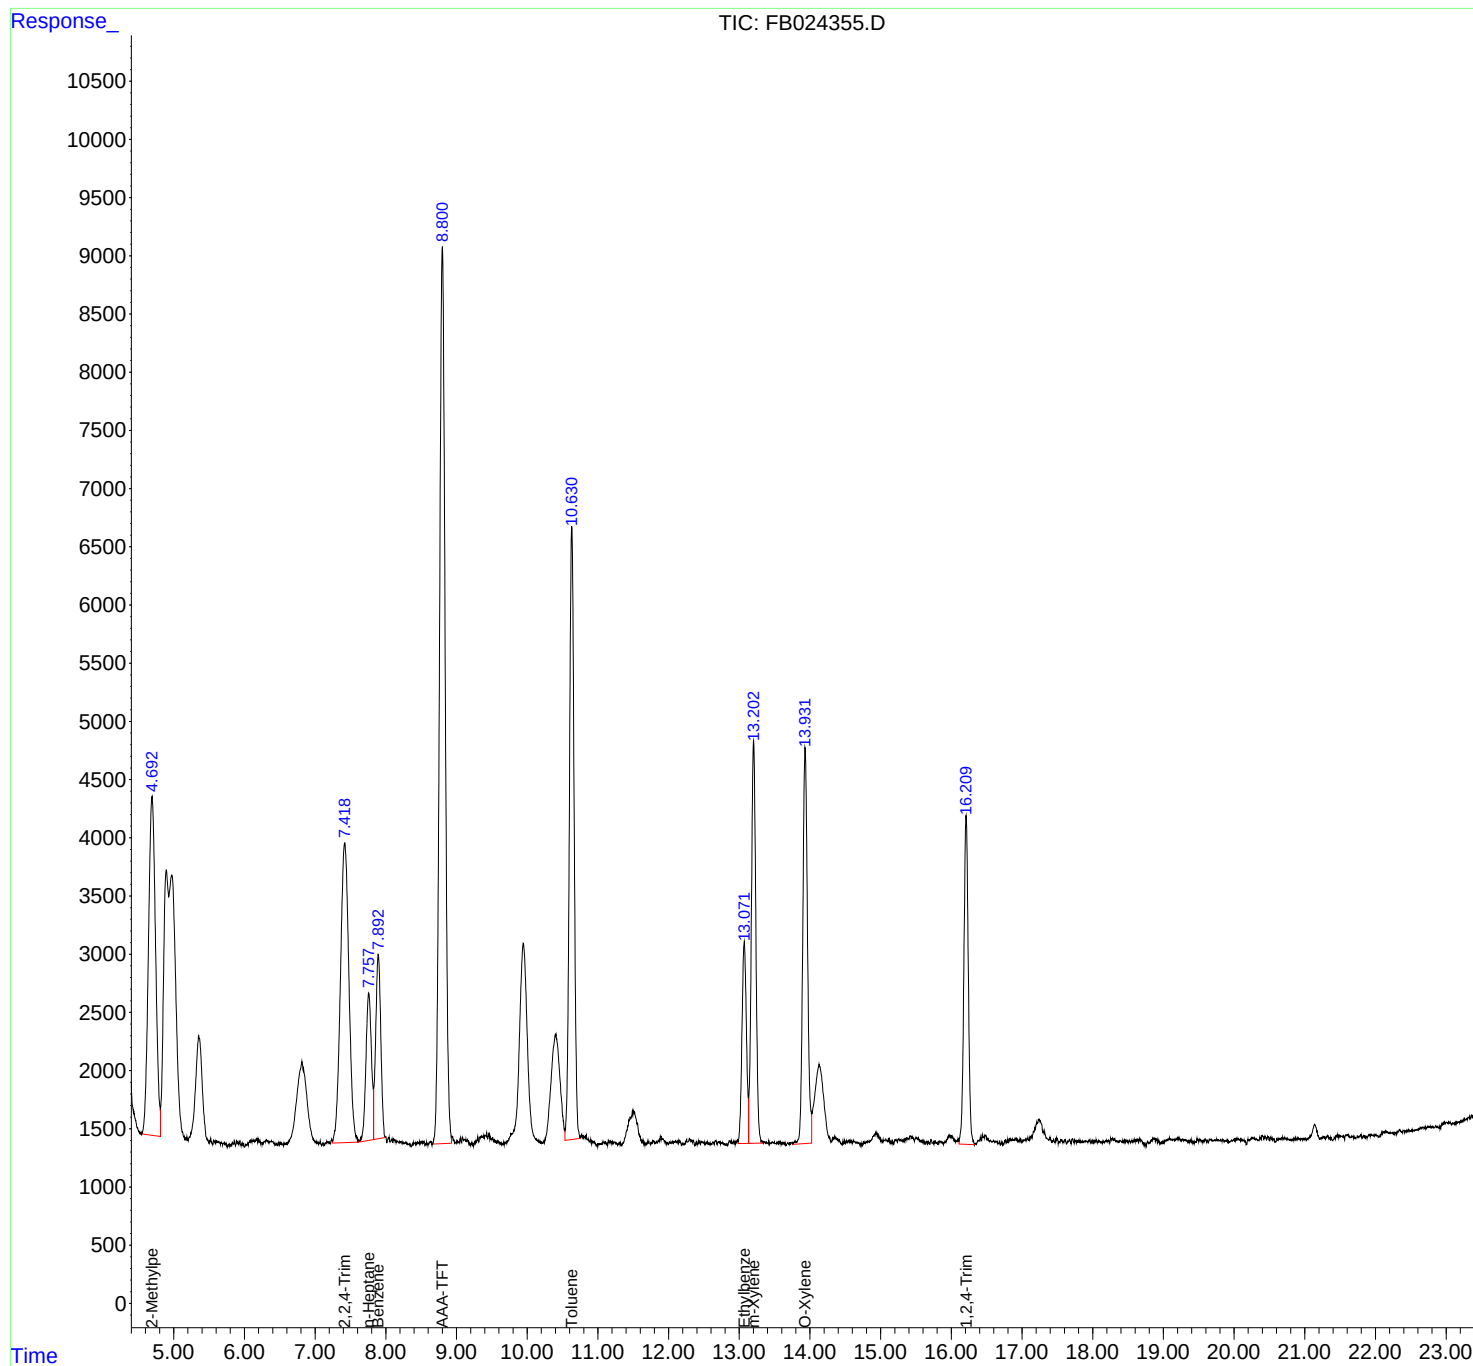


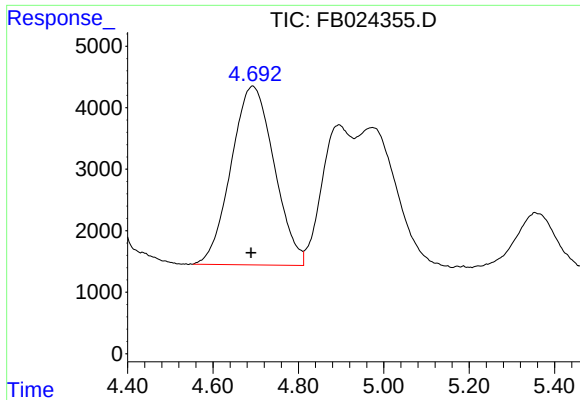

#1 2-Methylpentane


R.T.: 4.694 min
Delta R.T.: 0.005 min
Response: 203406
Conc: 6.89 ng/ml

Instrument :
FID_B
ClientSampleId :
LOD-MDL-WATER-01-QT2-2020

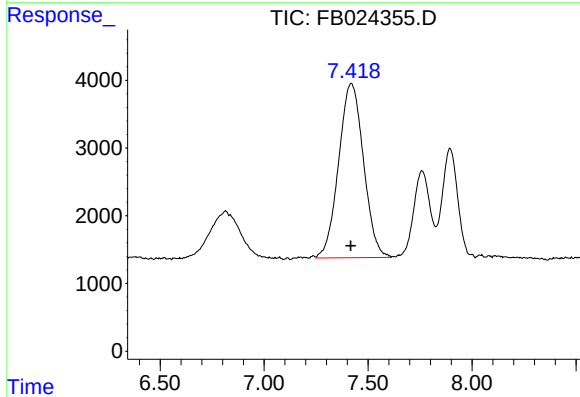


#2 2,2,4-Trimethylpentane

R.T.: 7.420 min
Delta R.T.: 0.003 min
Response: 213635
Conc: 6.99 ng/ml

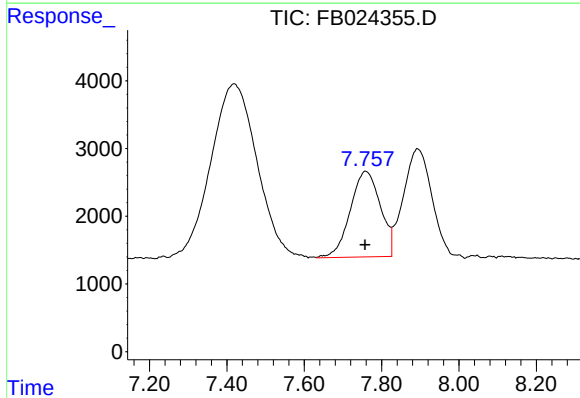


#3 n-Heptane

R.T.: 7.759 min
Delta R.T.: 0.000 min
Response: 68209
Conc: 2.25 ng/ml

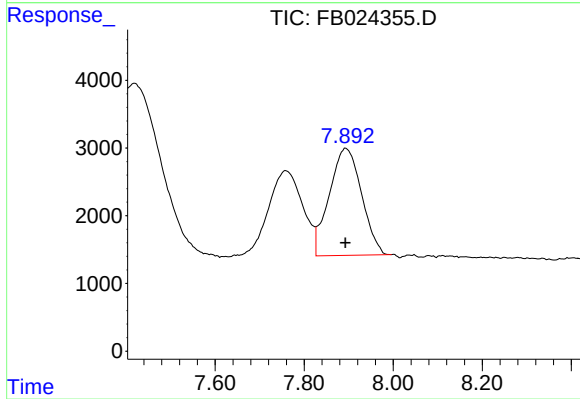

#4 Benzene


R.T.: 7.893 min
Delta R.T.: 0.000 min
Response: 79765
Conc: 2.11 ng/ml

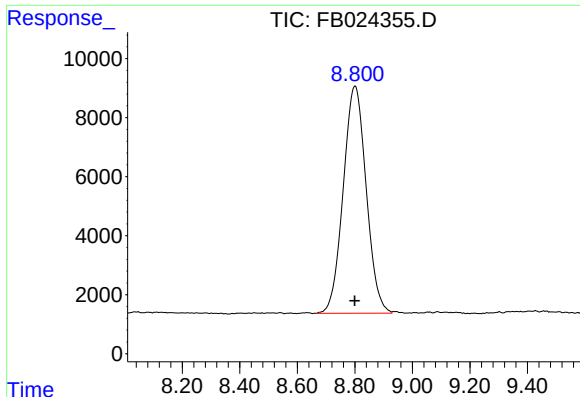

#5 AAA-TFT


R.T.: 8.801 min
Delta R.T.: 0.002 min
Response: 428701
Conc: 19.41 ng/ml

Instrument :
FID_B
ClientSampleId :
LOD-MDL-WATER-01-QT2-2020

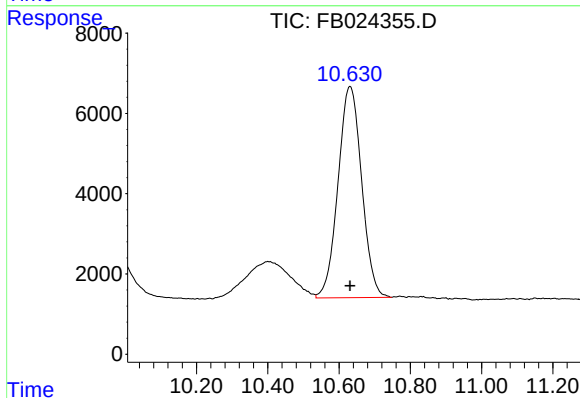


#6 Toluene

R.T.: 10.632 min
Delta R.T.: 0.000 min
Response: 242367
Conc: 6.69 ng/ml

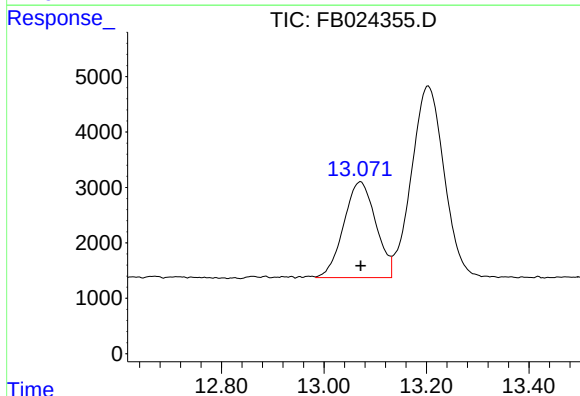


#7 Ethylbenzene

R.T.: 13.072 min
Delta R.T.: 0.000 min
Response: 75082
Conc: 2.21 ng/ml

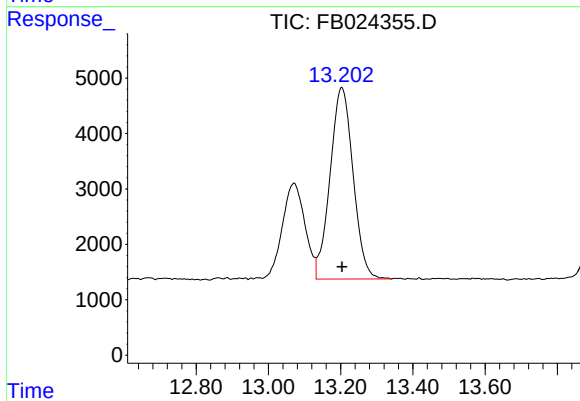

#8 m-Xylene


R.T.: 13.204 min
Delta R.T.: 0.000 min
Response: 153173
Conc: 4.64 ng/ml

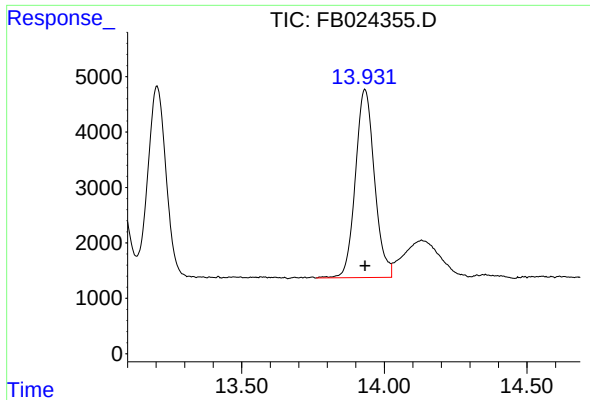

#9 O-Xylene

R.T.: 13.932 min
Delta R.T.: 0.000 min
Response: 157671
Conc: 4.89 ng/ml

Instrument :
FID_B
ClientSampleId :
LOD-MDL-WATER-01-QT2-2020

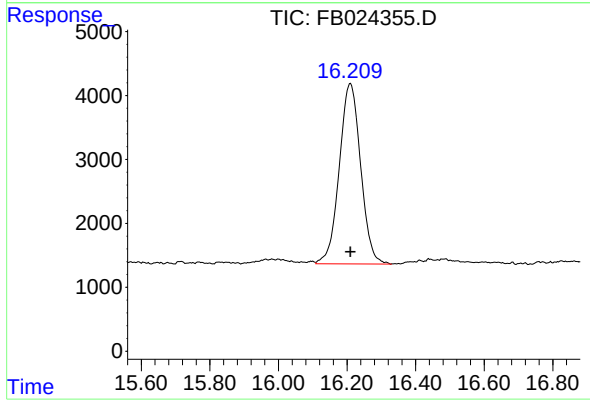

#10 1,2,4-Trimethylbenzene

R.T.: 16.210 min
Delta R.T.: 0.000 min
Response: 121965
Conc: 4.52 ng/ml