

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB051320\
 Data File : FB024356.D
 Signal(s) : FID2B.CH
 Acq On : 13 May 2020 18:25
 Operator : DD/AJ
 Sample : L2182-08
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 LOQ-WATER-02-QT2-2020

Integration File: Calibration.e
 Quant Time: May 14 04:30:00 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051120.M
 Quant Title :
 QLast Update : Mon May 11 11:14:42 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.795	432465	19.585 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.679	246462	8.352 ng/ml
2) t 2,2,4-Trimethylpentane	7.412	257283	8.422 ng/ml
3) t n-Heptane	7.755	81864	2.702 ng/ml
4) t Benzene	7.889	98191	2.597 ng/ml
6) t Toluene	10.628	290266	8.010 ng/ml
7) t Ethylbenzene	13.069	91564	2.701 ng/ml
8) t m-Xylene	13.201	181865	5.511 ng/ml
9) t O-Xylene	13.930	183448	5.685 ng/ml
10) t 1,2,4-Trimethylbenzene	16.208	145021	5.377 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB051320\
Data File : FB024356.D
Signal(s) : FID2B.CH
Acq On : 13 May 2020 18:25
Operator : DD/AJ
Sample : L2182-08
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
LOQ-WATER-02-QT2-2020

Integration File: Calibration.e
Quant Time: May 14 04:30:00 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051120.M
Quant Title :
QLast Update : Mon May 11 11:14:42 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

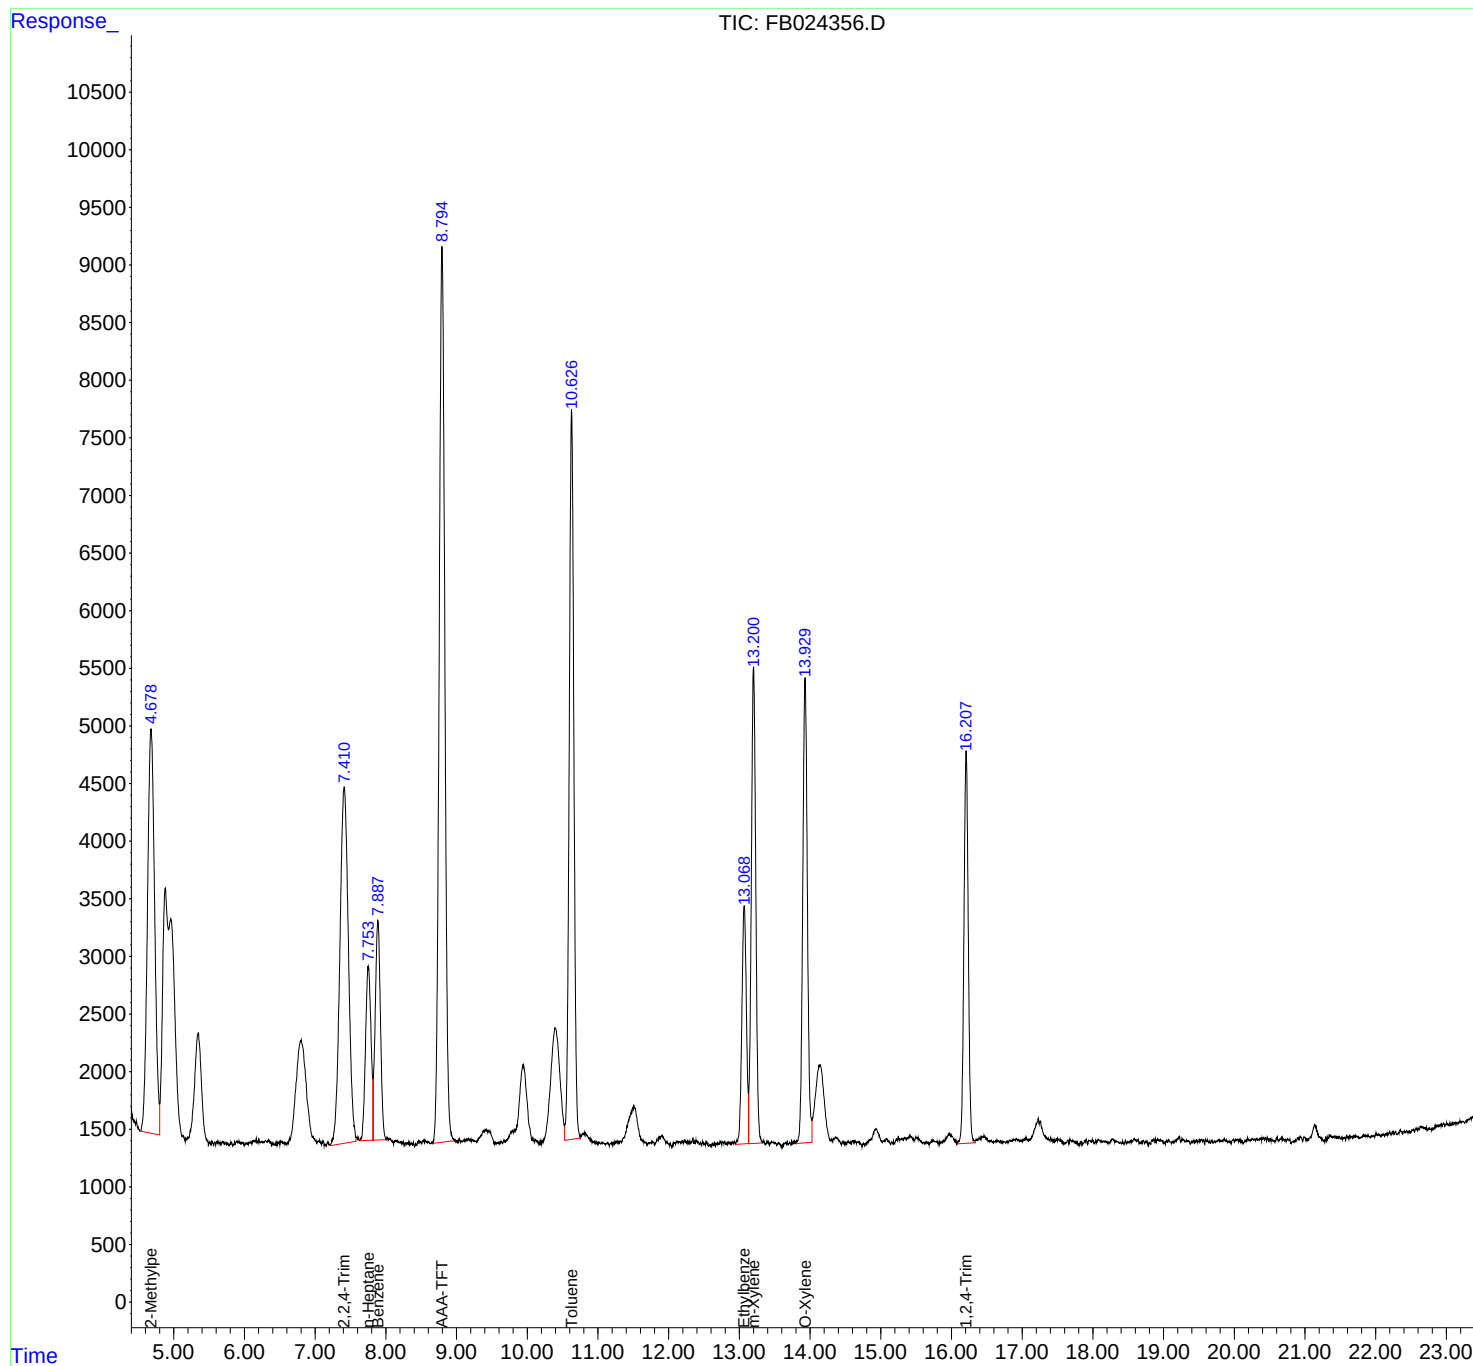


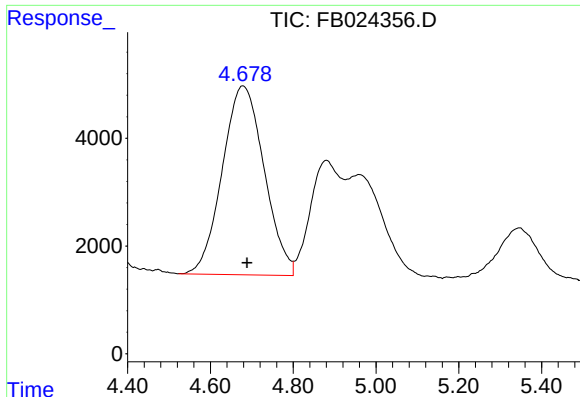

#1 2-Methylpentane


R.T.: 4.679 min
Delta R.T.: -0.010 min
Response: 246462
Conc: 8.35 ng/ml

Instrument :
FID_B
ClientSampleId :
LOQ-WATER-02-QT2-2020

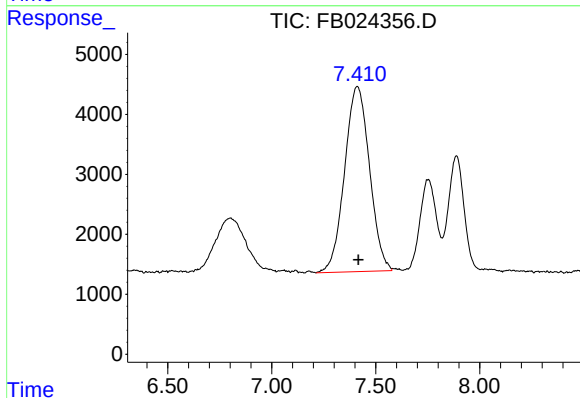


#2 2,2,4-Trimethylpentane

R.T.: 7.412 min
Delta R.T.: -0.005 min
Response: 257283
Conc: 8.42 ng/ml

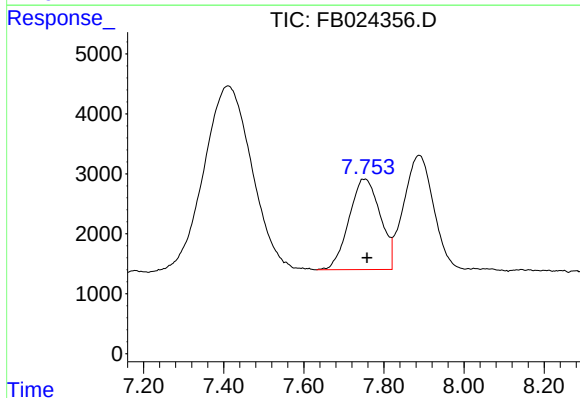


#3 n-Heptane

R.T.: 7.755 min
Delta R.T.: -0.003 min
Response: 81864
Conc: 2.70 ng/ml

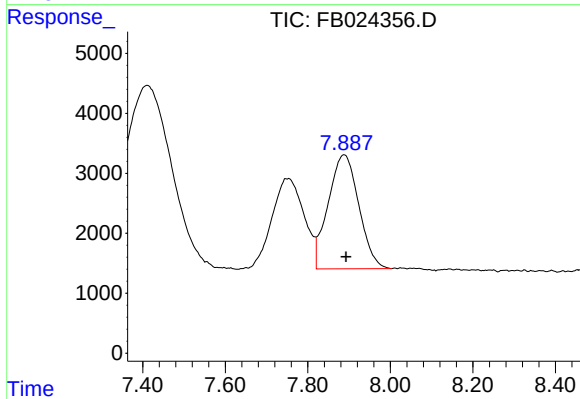

#4 Benzene


R.T.: 7.889 min
Delta R.T.: -0.004 min
Response: 98191
Conc: 2.60 ng/ml

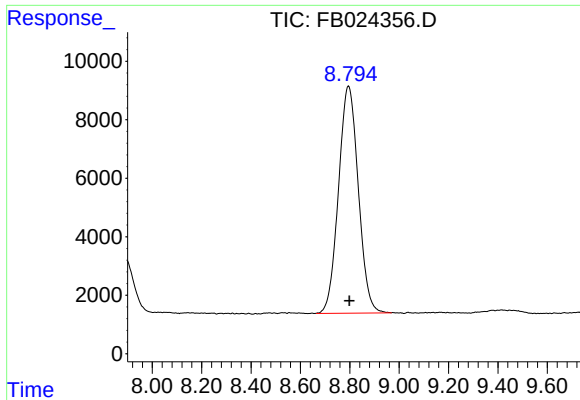

#5 AAA-TFT


R.T.: 8.795 min
Delta R.T.: -0.004 min
Response: 432465
Conc: 19.58 ng/ml

Instrument :
FID_B
ClientSampleId :
LOQ-WATER-02-QT2-2020

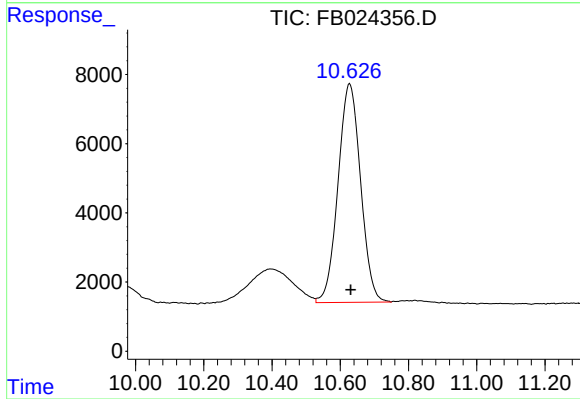


#6 Toluene

R.T.: 10.628 min
Delta R.T.: -0.003 min
Response: 290266
Conc: 8.01 ng/ml

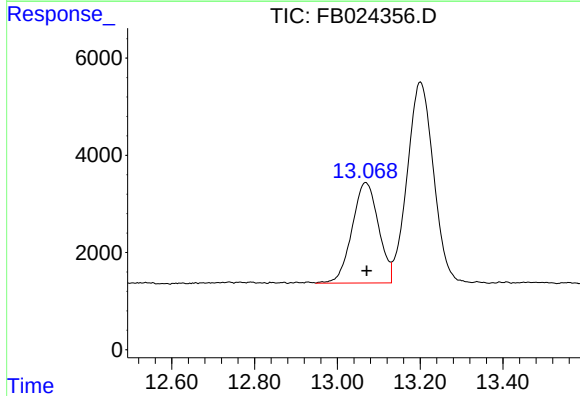


#7 Ethylbenzene

R.T.: 13.069 min
Delta R.T.: -0.002 min
Response: 91564
Conc: 2.70 ng/ml

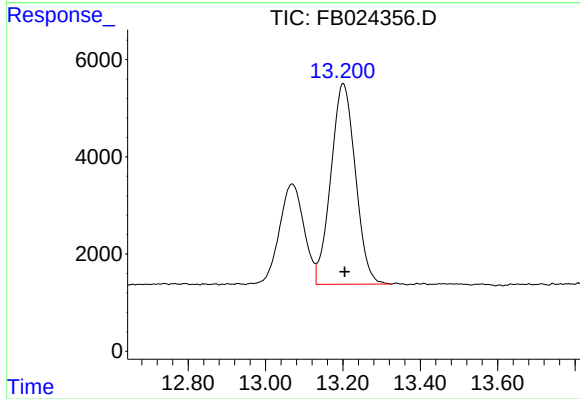

#8 m-Xylene


R.T.: 13.201 min
Delta R.T.: -0.003 min
Response: 181865
Conc: 5.51 ng/ml

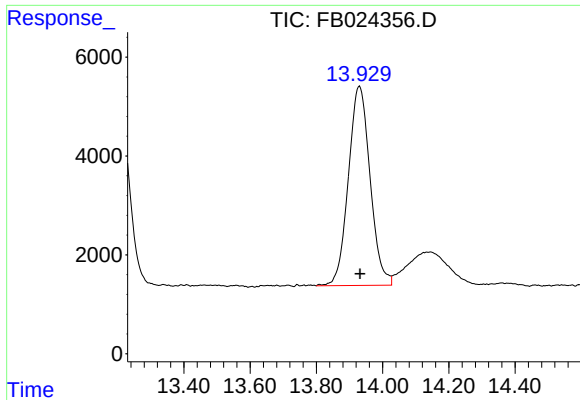

#9 O-Xylene

R.T.: 13.930 min
Delta R.T.: -0.002 min
Response: 183448
Conc: 5.68 ng/ml

Instrument :
FID_B
ClientSampleId :
LOQ-WATER-02-QT2-2020

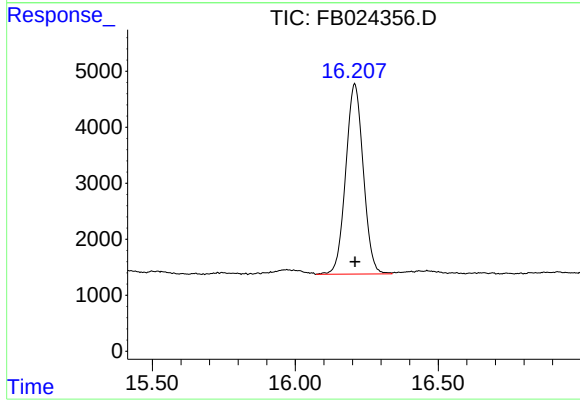

#10 1,2,4-Trimethylbenzene

R.T.: 16.208 min
Delta R.T.: -0.001 min
Response: 145021
Conc: 5.38 ng/ml