

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB051322\
 Data File : FB027187.D
 Signal(s) : FID2B.CH
 Acq On : 13 May 2022 11:20
 Operator : AJ/MA
 Sample : BSF0513S1
 Misc : 5.03G/5.00 ML DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0513S1

Integration File: Calibration.e
 Quant Time: May 13 22:56:26 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051022.M
 Quant Title :
 QLast Update : Tue May 10 13:42:12 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.788	241032	22.961 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.707	514505	32.331 ng/ml
2) t 2,2,4-Trimethylpentane	7.420	540880	33.525 ng/ml
3) t n-Heptane	7.747	180362	11.037 ng/ml
4) t Benzene	7.883	210538	11.353 ng/ml
6) t Toluene	10.616	597115	33.632 ng/ml
7) t Ethylbenzene	13.053	184138	11.151 ng/ml
8) t m-Xylene	13.185	367266	22.320 ng/ml
9) t O-Xylene	13.912	362358	22.091 ng/ml
10) t 1,2,4-Trimethylbenzene	16.187	368304	22.061 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB051322\
Data File : FB027187.D
Signal(s) : FID2B.CH
Acq On : 13 May 2022 11:20
Operator : AJ/MA
Sample : BSF0513S1
Misc : 5.03G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0513S1

Integration File: Calibration.e
Quant Time: May 13 22:56:26 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051022.M
Quant Title :
QLast Update : Tue May 10 13:42:12 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

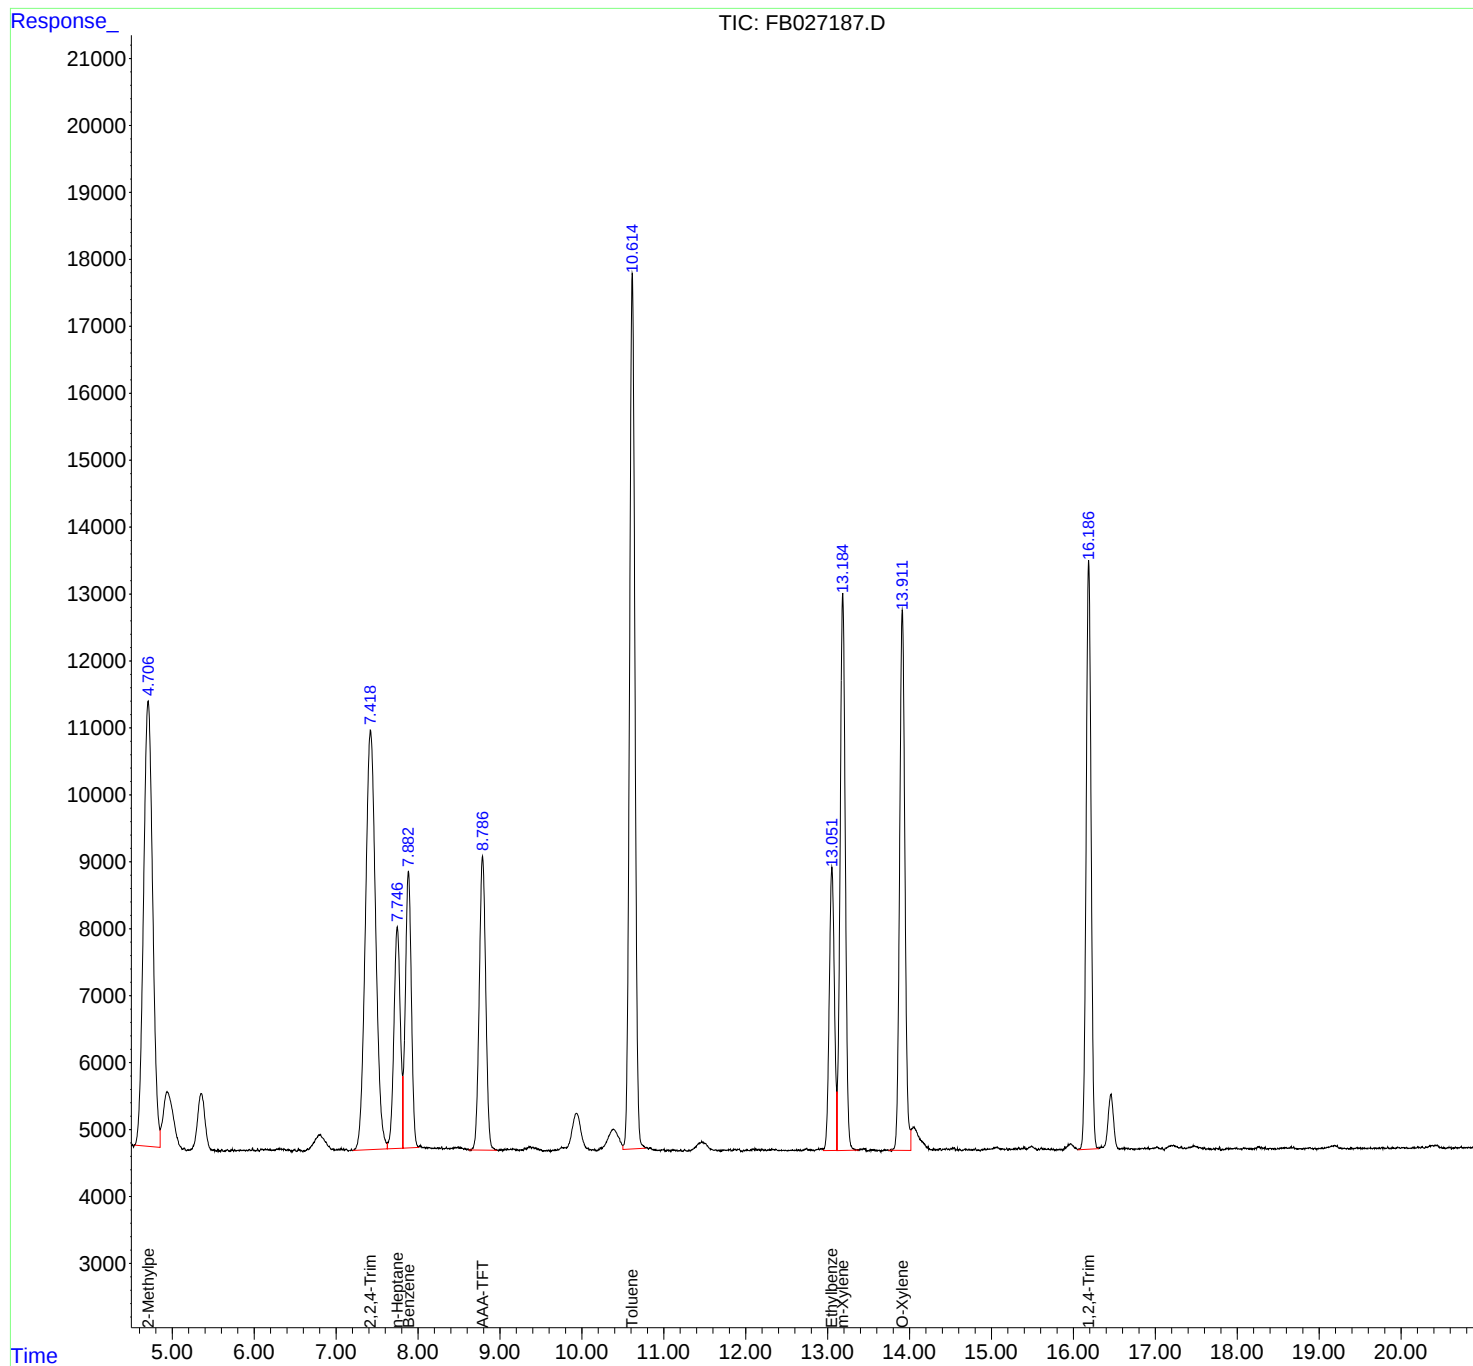


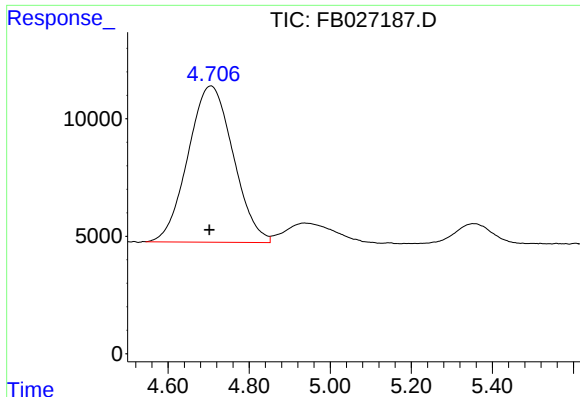

#1 2-Methylpentane


R.T.: 4.707 min
Delta R.T.: 0.005 min
Response: 514505
Conc: 32.33 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0513S1

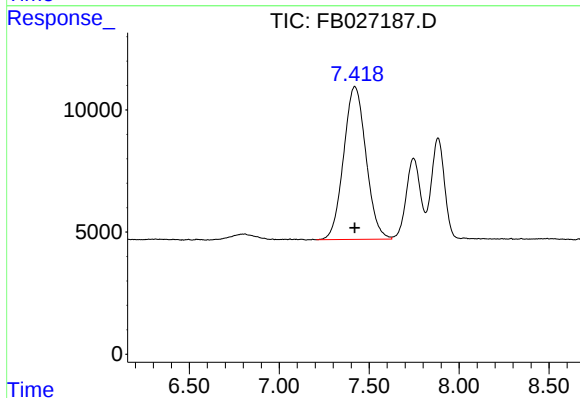


#2 2,2,4-Trimethylpentane

R.T.: 7.420 min
Delta R.T.: 0.000 min
Response: 540880
Conc: 33.52 ng/ml

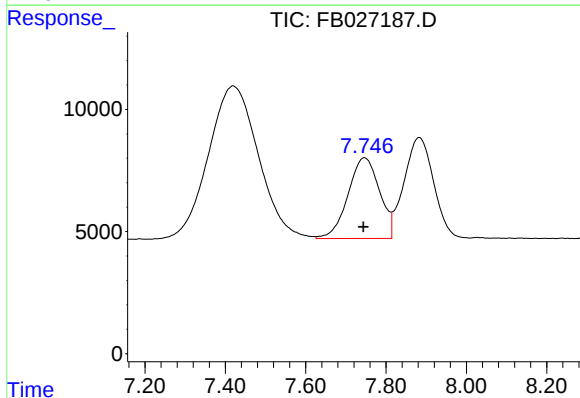


#3 n-Heptane

R.T.: 7.747 min
Delta R.T.: 0.003 min
Response: 180362
Conc: 11.04 ng/ml

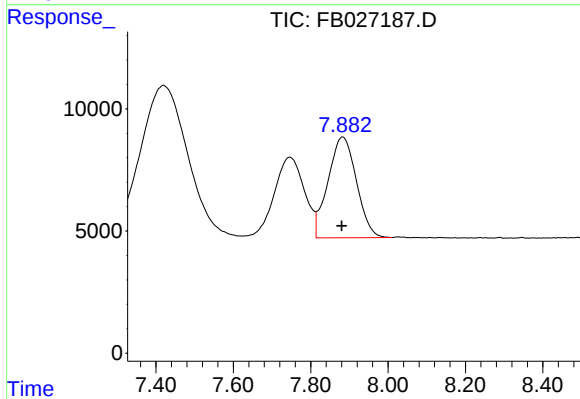

#4 Benzene


R.T.: 7.883 min
Delta R.T.: 0.003 min
Response: 210538
Conc: 11.35 ng/ml

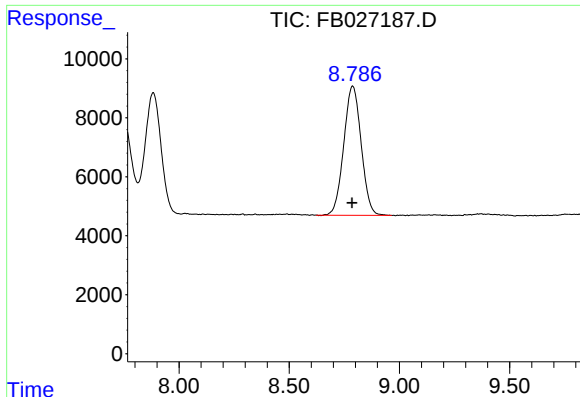

#5 AAA-TFT


R.T.: 8.788 min
Delta R.T.: 0.003 min
Response: 241032
Conc: 22.96 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0513S1

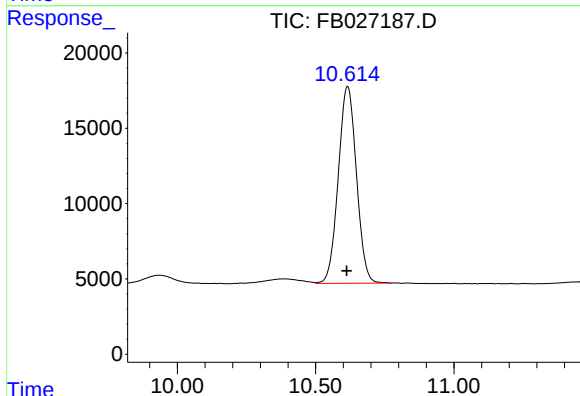


#6 Toluene

R.T.: 10.616 min
Delta R.T.: 0.003 min
Response: 597115
Conc: 33.63 ng/ml

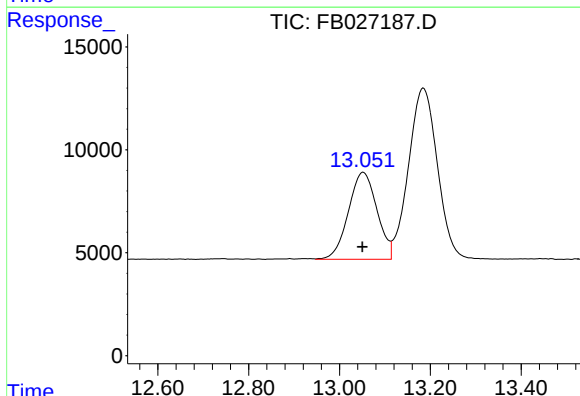


#7 Ethylbenzene

R.T.: 13.053 min
Delta R.T.: 0.002 min
Response: 184138
Conc: 11.15 ng/ml

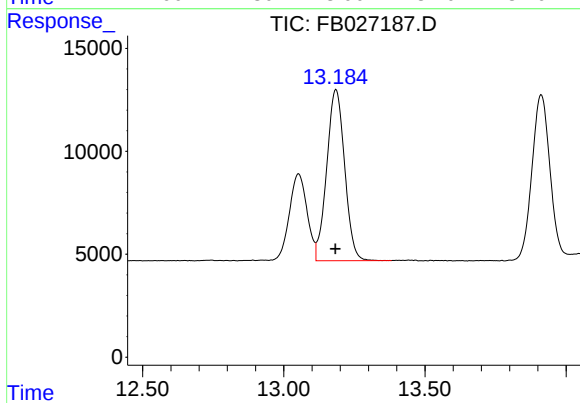

#8 m-Xylene


R.T.: 13.185 min
Delta R.T.: 0.002 min
Response: 367266
Conc: 22.32 ng/ml

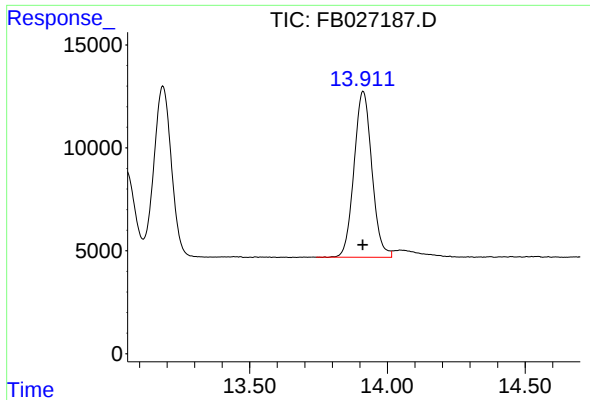

#9 O-Xylene

R.T.: 13.912 min
Delta R.T.: 0.002 min
Response: 362358
Conc: 22.09 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0513S1

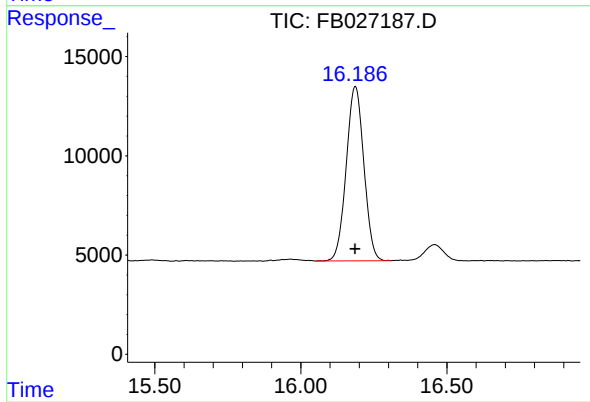

#10 1,2,4-Trimethylbenzene

R.T.: 16.187 min
Delta R.T.: 0.001 min
Response: 368304
Conc: 22.06 ng/ml