

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB051325\
Data File : FB031705.D
Signal(s) : FID2B.CH
Acq On : 13 May 2025 9:24
Operator : YP/AJ
Sample : VBF0513S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: May 14 07:19:53 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB042325.M
Quant Title :
QLast Update : Wed Apr 23 13:48:24 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.793	501449	21.866 ng/ml
Target Compounds			
6) t Toluene	10.616	13218	0.332 ng/ml
8) t m-Xylene	13.191	13952	0.357 ng/ml
9) t O-Xylene	13.917	12797	0.347 ng/ml
10) t 1,2,4-Trimethylbenzene	16.192	22039	0.817 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB051325\
Data File : FB031705.D
Signal(s) : FID2B.CH
Acq On : 13 May 2025 9:24
Operator : YP/AJ
Sample : VBF0513S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: May 14 07:19:53 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB042325.M
Quant Title :
QLast Update : Wed Apr 23 13:48:24 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

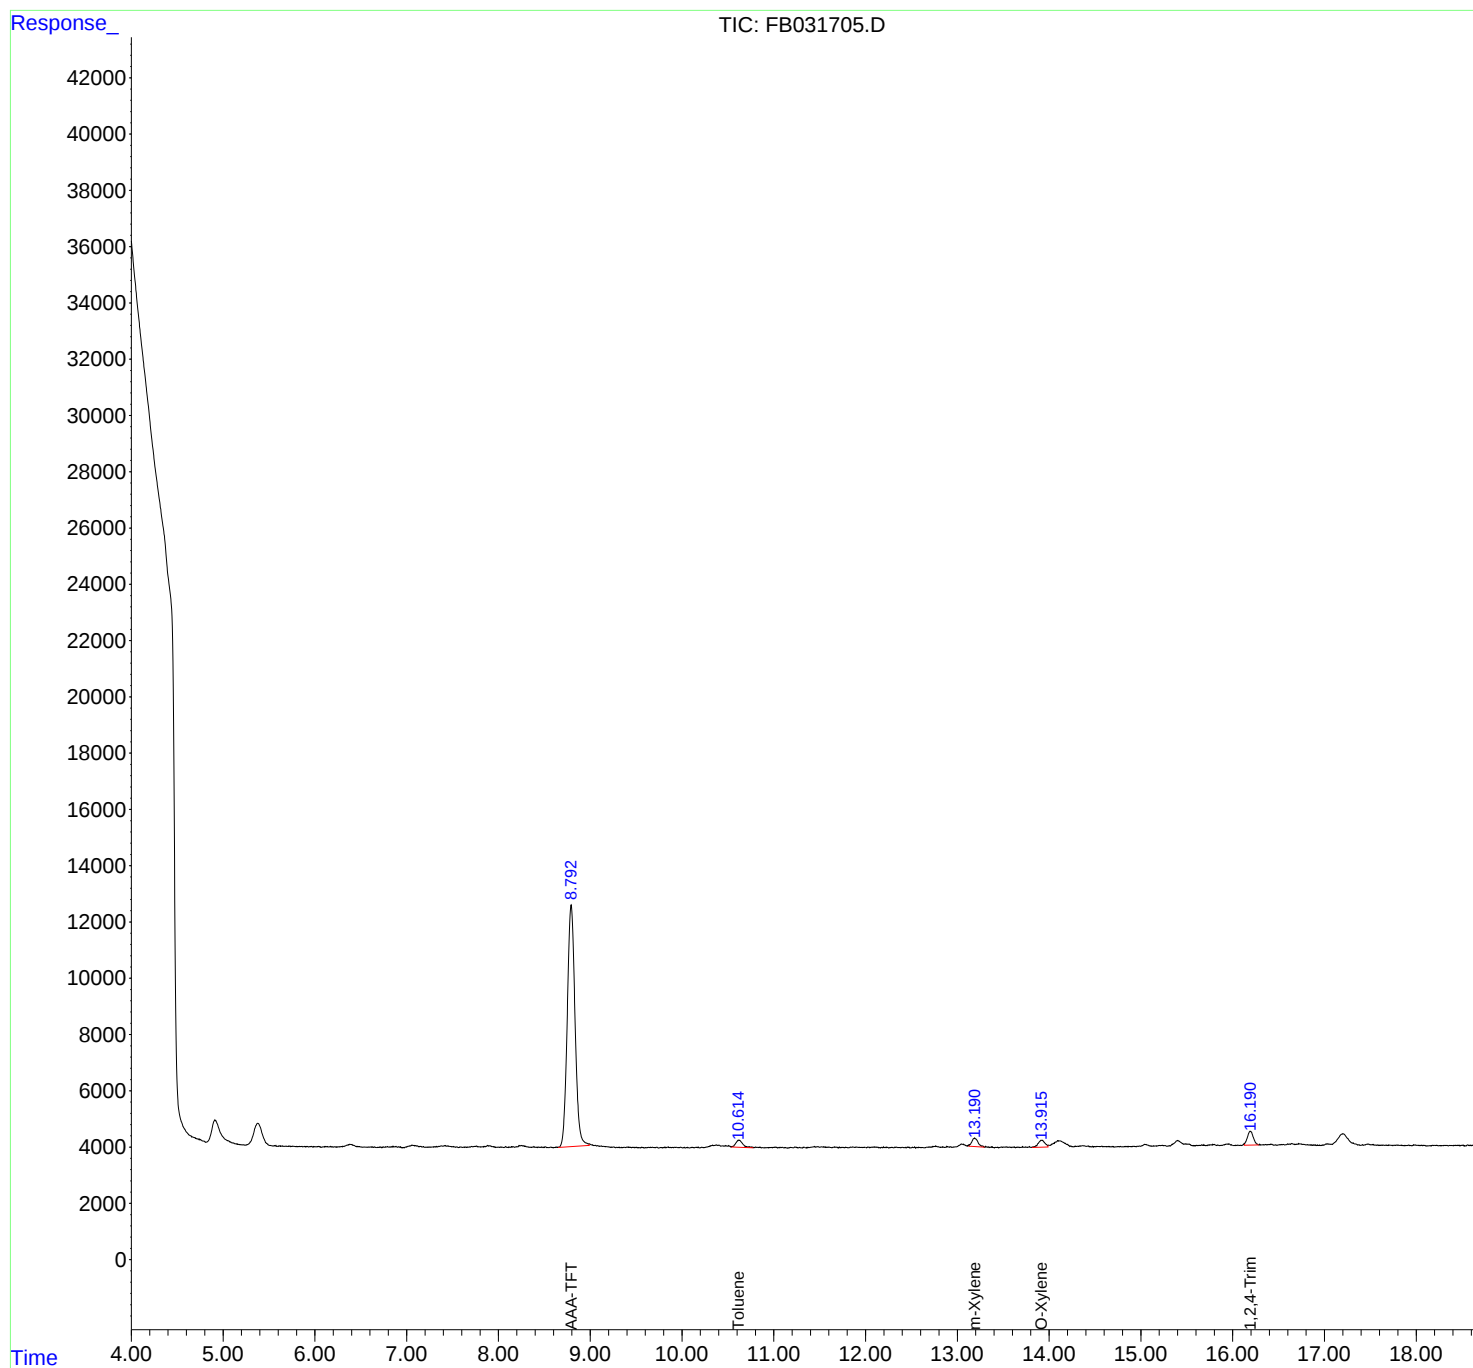


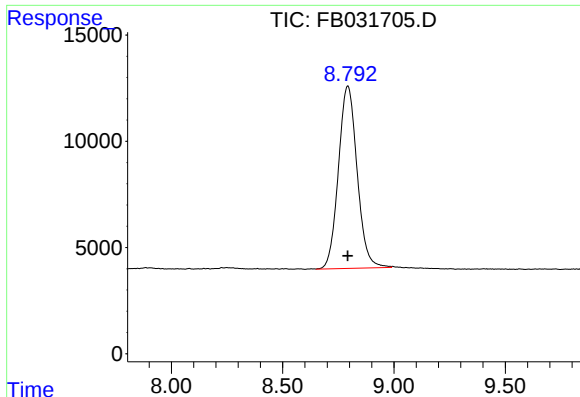

#5 AAA-TFT


R.T.: 8.793 min
Delta R.T.: 0.001 min
Response: 501449
Conc: 21.87 ng/ml

Instrument :
FID_B
ClientSampleId :

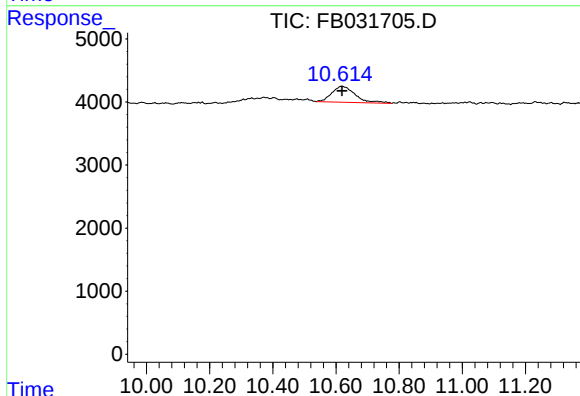


#6 Toluene

R.T.: 10.616 min
Delta R.T.: -0.004 min
Response: 13218
Conc: 0.33 ng/ml

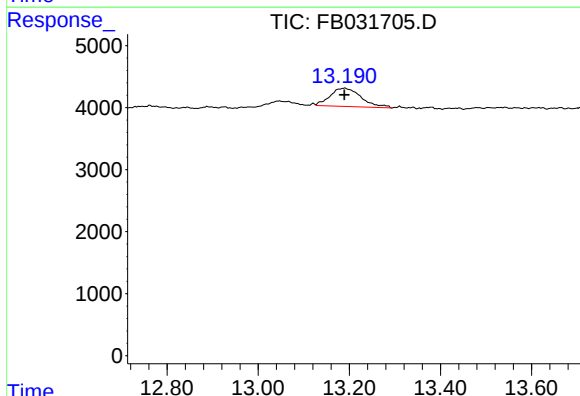


#8 m-Xylene

R.T.: 13.191 min
Delta R.T.: 0.002 min
Response: 13952
Conc: 0.36 ng/ml

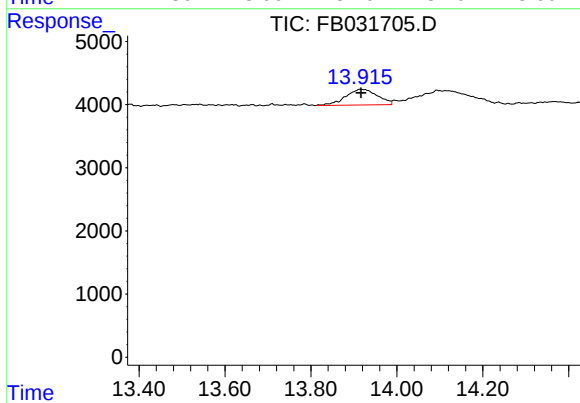

#9 O-Xylene

R.T.: 13.917 min
Delta R.T.: 0.000 min
Response: 12797
Conc: 0.35 ng/ml

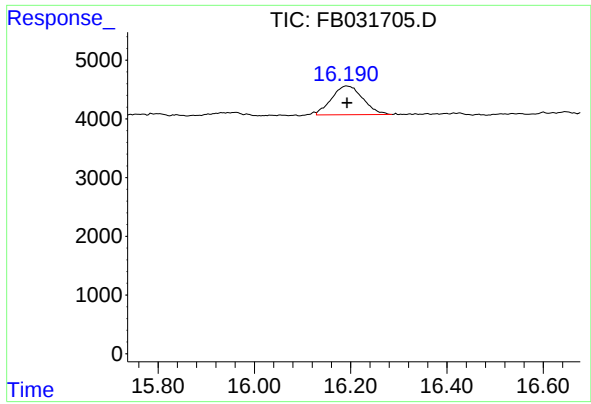

#10 1,2,4-Trimethylbenzene

R.T.: 16.192 min
Delta R.T.: -0.001 min
Response: 22039
Conc: 0.82 ng/ml

Instrument :

FID_B

ClientSampleId :