

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB051325\  
Data File : FB031705.D  
Signal(s) : FID2B.CH  
Acq On : 13 May 2025 9:24  
Operator : YP/AJ  
Sample : VBF0513S1  
Misc : 5.00G/5.00 ML DI WATER  
ALS Vial : 2 Sample Multiplier: 1

Instrument :  
FID\_B  
ClientSampleId :  
VBF0513S1

Integration File: Calibration.e  
Quant Time: May 14 07:19:53 2025  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB042325.M  
Quant Title :  
QLast Update : Wed Apr 23 13:48:24 2025  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 5 g/ml  
Signal Phase : RTX-502.2  
Signal Info : 60mx0.53mmx3.00um

| Compound                     | R.T.   | Response | Conc Units   |
|------------------------------|--------|----------|--------------|
| -----                        |        |          |              |
| System Monitoring Compounds  |        |          |              |
| 5) s AAA-TFT                 | 8.793  | 501449   | 21.866 ng/ml |
| Target Compounds             |        |          |              |
| 6) t Toluene                 | 10.616 | 13218    | 0.332 ng/ml  |
| 8) t m-Xylene                | 13.191 | 13952    | 0.357 ng/ml  |
| 9) t O-Xylene                | 13.917 | 12797    | 0.347 ng/ml  |
| 10) t 1,2,4-Trimethylbenzene | 16.192 | 22039    | 0.817 ng/ml  |
| -----                        |        |          |              |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB051325\  
Data File : FB031705.D  
Signal(s) : FID2B.CH  
Acq On : 13 May 2025 9:24  
Operator : YP/AJ  
Sample : VBF0513S1  
Misc : 5.00G/5.00 ML DI WATER  
ALS Vial : 2 Sample Multiplier: 1

Instrument :  
FID\_B  
ClientSampleId :  
VBF0513S1

Integration File: Calibration.e  
Quant Time: May 14 07:19:53 2025  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB042325.M  
Quant Title :  
QLast Update : Wed Apr 23 13:48:24 2025  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 5 g/ml  
Signal Phase : RTX-502.2  
Signal Info : 60mx0.53mmx3.00um

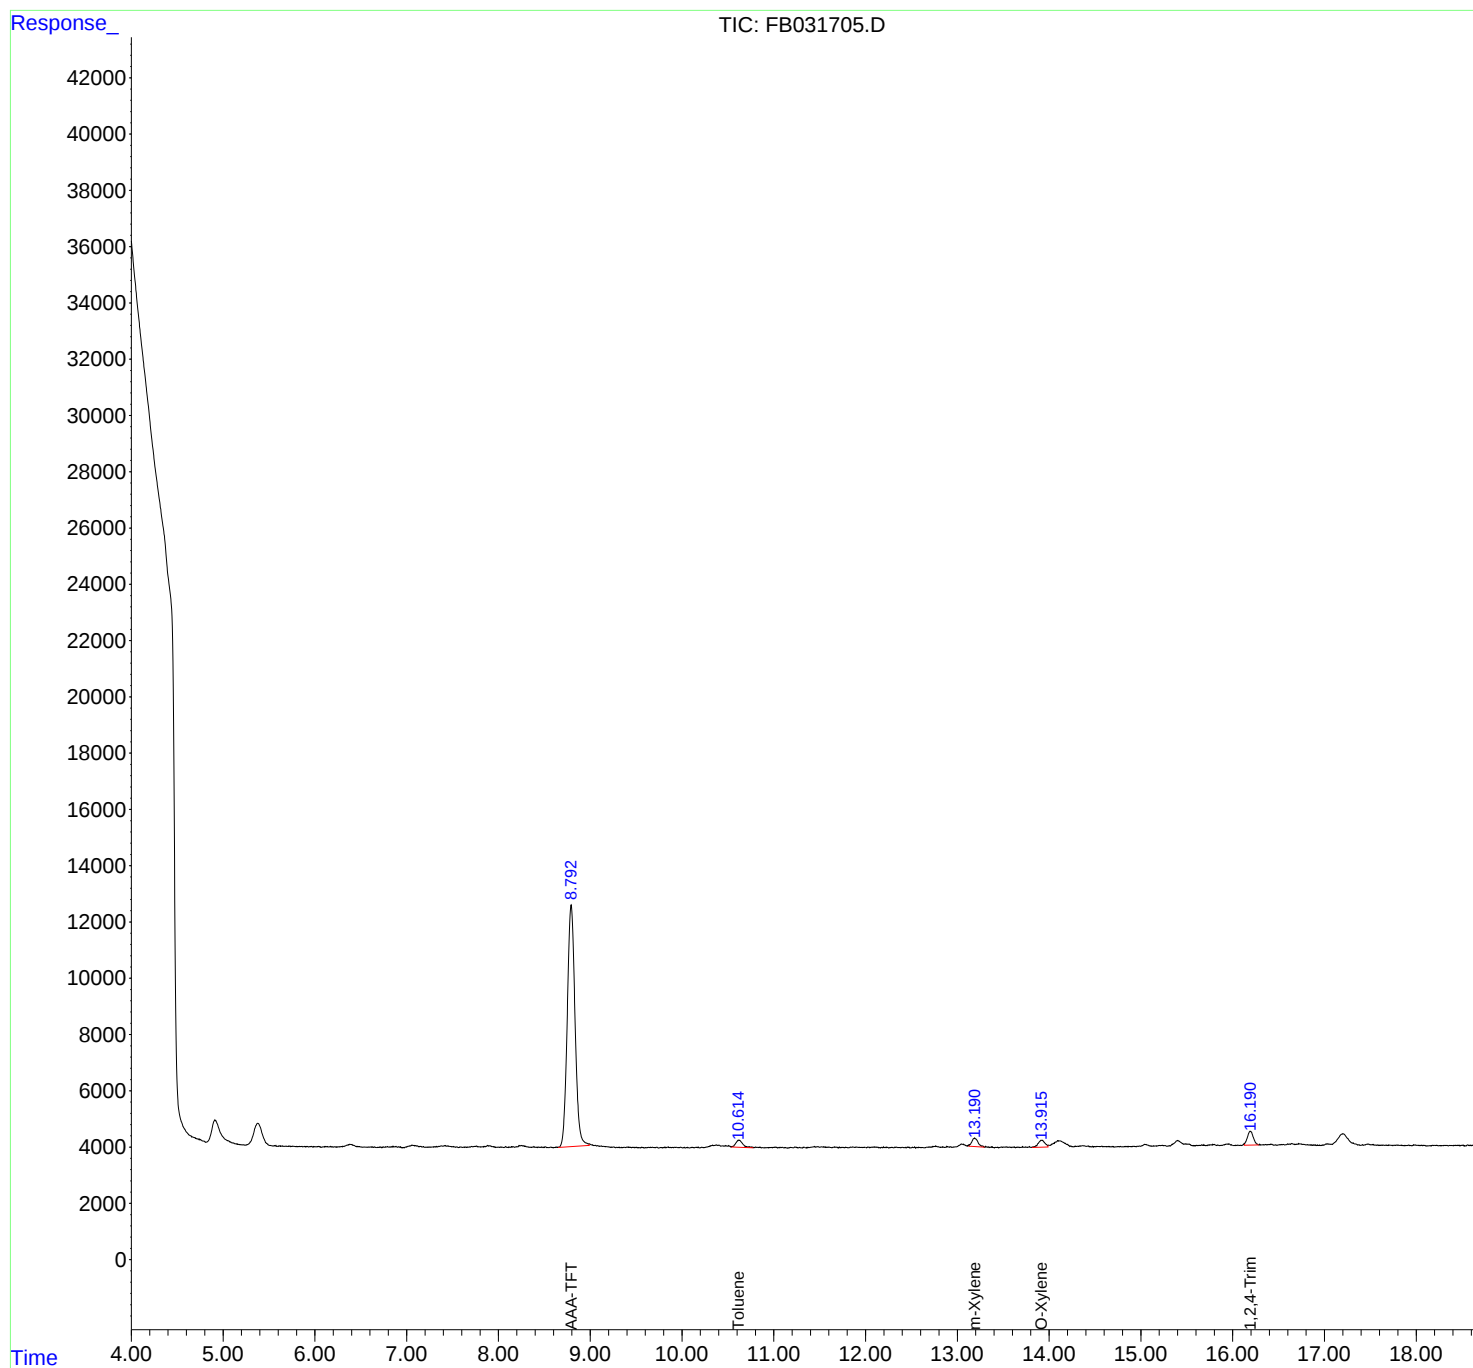


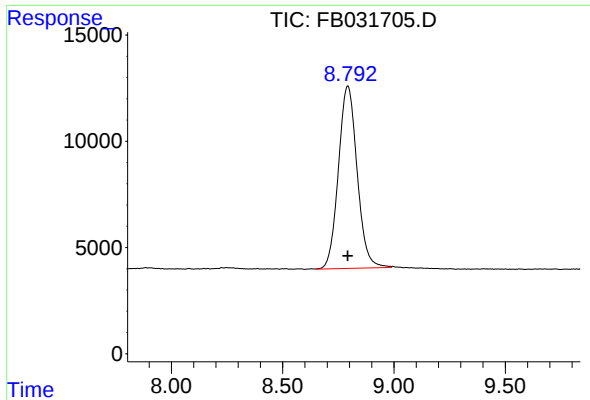

#5 AAA-TFT


R.T.: 8.793 min  
Delta R.T.: 0.001 min  
Response: 501449  
Conc: 21.87 ng/ml

Instrument :  
FID\_B  
ClientSampleId :  
VBF0513S1

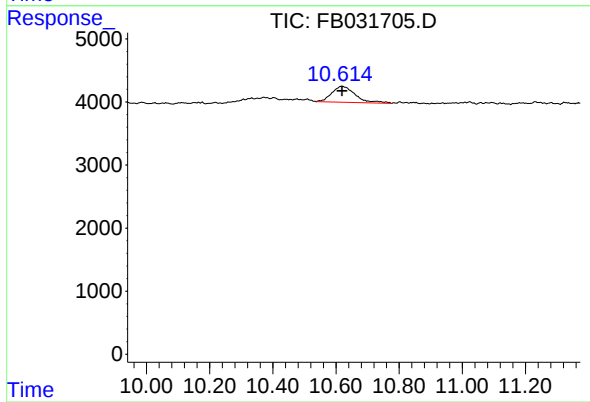


#6 Toluene

R.T.: 10.616 min  
Delta R.T.: -0.004 min  
Response: 13218  
Conc: 0.33 ng/ml

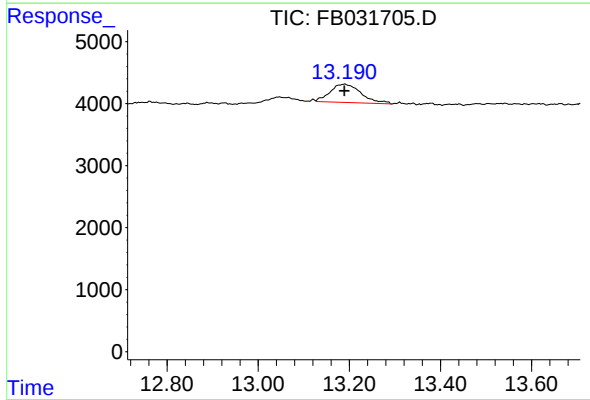


#8 m-Xylene

R.T.: 13.191 min  
Delta R.T.: 0.002 min  
Response: 13952  
Conc: 0.36 ng/ml

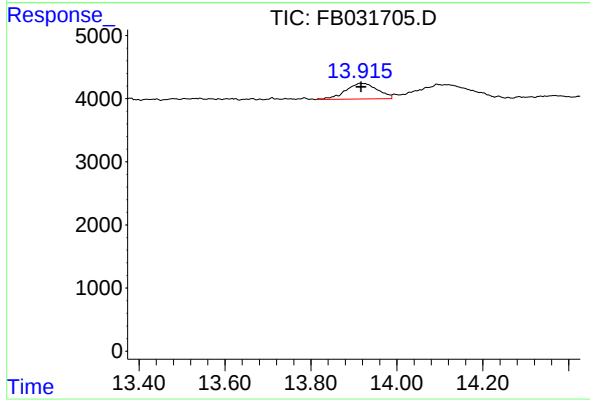

#9 O-Xylene

R.T.: 13.917 min  
Delta R.T.: 0.000 min  
Response: 12797  
Conc: 0.35 ng/ml

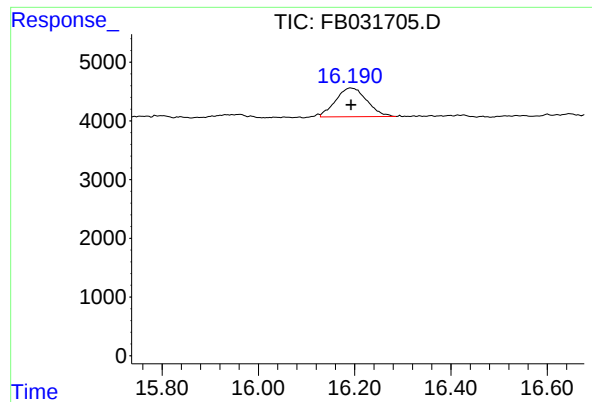

#10 1,2,4-Trimethylbenzene

R.T.: 16.192 min  
Delta R.T.: -0.001 min  
Response: 22039  
Conc: 0.82 ng/ml

Instrument :

FID\_B

ClientSampleId :

VBF0513S1