

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB051325\
Data File : FB031708.D
Signal(s) : FID2B.CH
Acq On : 13 May 2025 10:45
Operator : YP/AJ
Sample : Q1982-02
Misc : 5.16G/5.00 ML DI WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
TP-2B

Integration File: Calibration.e
Quant Time: May 14 07:20:23 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB042325.M
Quant Title :
QLast Update : Wed Apr 23 13:48:24 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

6) t	Toluene	10.624	6759	0.170 ng/ml
7) t	Ethylbenzene	13.060	4840	0.135 ng/ml
8) t	m-Xylene	13.189	14609	0.374 ng/ml
9) t	O-Xylene	13.925	7555	0.205 ng/ml
10) t	1,2,4-Trimethylbenzene	16.194	20035	0.743 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB051325\
Data File : FB031708.D
Signal(s) : FID2B.CH
Acq On : 13 May 2025 10:45
Operator : YP/AJ
Sample : Q1982-02
Misc : 5.16G/5.00 ML DI WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
TP-2B

Integration File: Calibration.e
Quant Time: May 14 07:20:23 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB042325.M
Quant Title :
QLast Update : Wed Apr 23 13:48:24 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

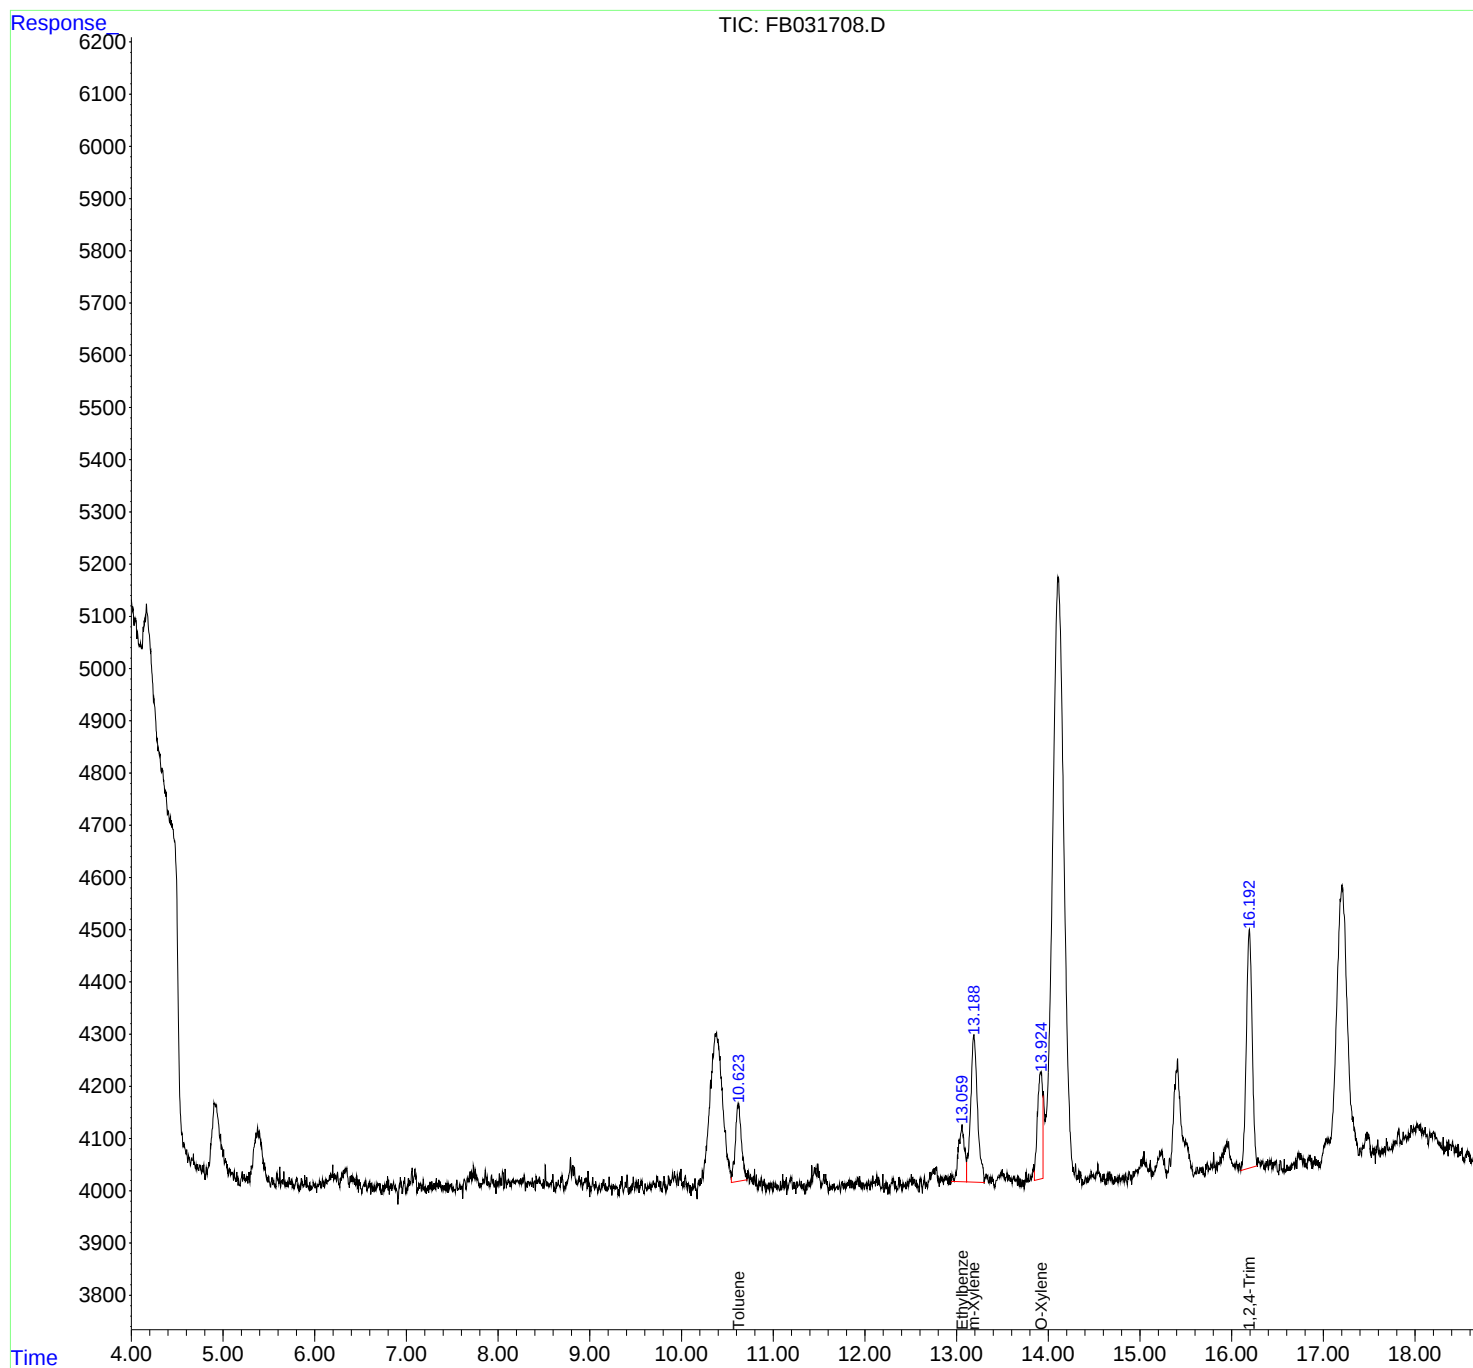


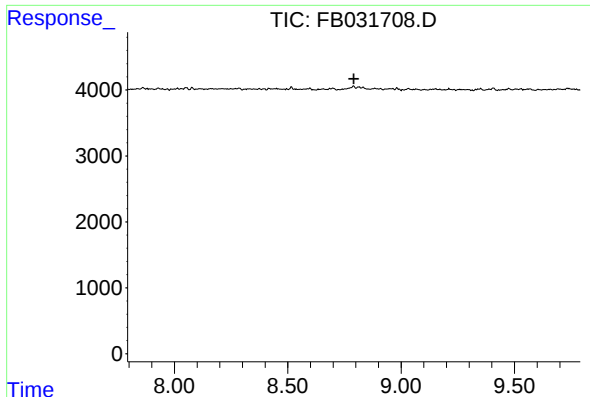

#5 AAA-TFT


R.T.: 0.000 min
Exp R.T.: 8.792 min
Response: 0
Conc: N.D.

Instrument :
FID_B
ClientSampleId :
TP-2B

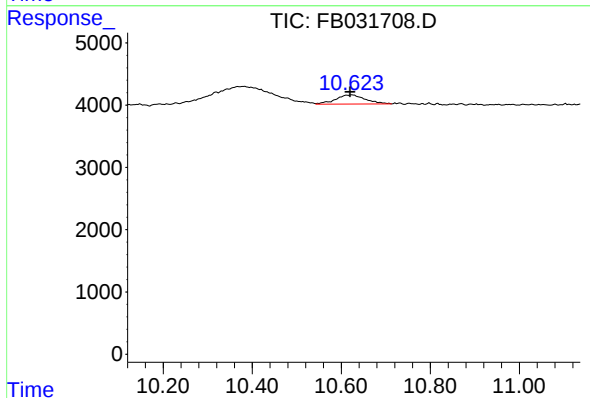


#6 Toluene

R.T.: 10.624 min
Delta R.T.: 0.005 min
Response: 6759
Conc: 0.17 ng/ml

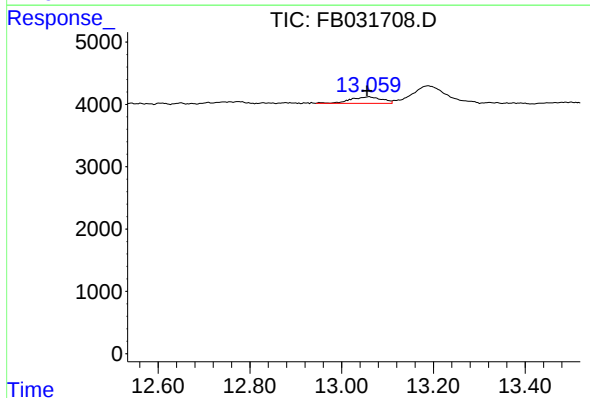


#7 Ethylbenzene

R.T.: 13.060 min
Delta R.T.: 0.005 min
Response: 4840
Conc: 0.14 ng/ml

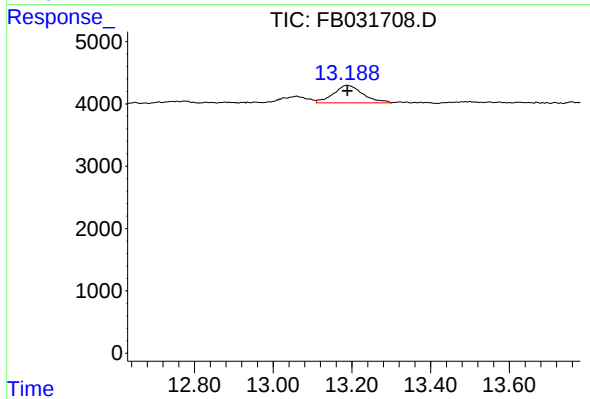

#8 m-Xylene


R.T.: 13.189 min
Delta R.T.: 0.000 min
Response: 14609
Conc: 0.37 ng/ml

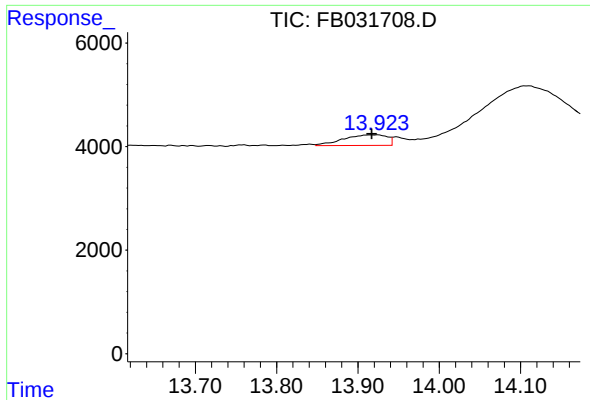

#9 O-Xylene

R.T.: 13.925 min
Delta R.T.: 0.008 min
Response: 7555
Conc: 0.21 ng/ml

Instrument :
FID_B
ClientSampleId :
TP-2B

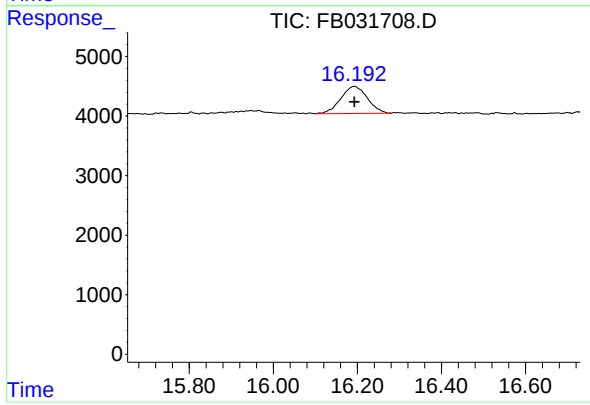

#10 1,2,4-Trimethylbenzene

R.T.: 16.194 min
Delta R.T.: 0.000 min
Response: 20035
Conc: 0.74 ng/ml