

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB051325\  
Data File : FB031710.D  
Signal(s) : FID2B.CH  
Acq On : 13 May 2025 11:54  
Operator : YP/AJ  
Sample : Q1982-04  
Misc : 5.61G/5.00 ML DI WATER  
ALS Vial : 7 Sample Multiplier: 1

Instrument :  
FID\_B  
ClientSampleId :  
TP-4

Integration File: Calibration.e  
Quant Time: May 14 07:20:40 2025  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB042325.M  
Quant Title :  
QLast Update : Wed Apr 23 13:48:24 2025  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 5 g/ml  
Signal Phase : RTX-502.2  
Signal Info : 60mx0.53mmx3.00um

| Compound                     | R.T.   | Response | Conc Units   |
|------------------------------|--------|----------|--------------|
| -----                        |        |          |              |
| System Monitoring Compounds  |        |          |              |
| 5) s AAA-TFT                 | 8.794  | 362132   | 15.791 ng/ml |
| Target Compounds             |        |          |              |
| 8) t m-Xylene                | 13.187 | 8770     | 0.224 ng/ml  |
| 9) t O-Xylene                | 13.917 | 5127     | 0.139 ng/ml  |
| 10) t 1,2,4-Trimethylbenzene | 16.199 | 10756    | 0.399 ng/ml  |
| -----                        |        |          |              |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB051325\  
Data File : FB031710.D  
Signal(s) : FID2B.CH  
Acq On : 13 May 2025 11:54  
Operator : YP/AJ  
Sample : Q1982-04  
Misc : 5.61G/5.00 ML DI WATER  
ALS Vial : 7 Sample Multiplier: 1

Instrument :  
FID\_B  
ClientSampleId :  
TP-4

Integration File: Calibration.e  
Quant Time: May 14 07:20:40 2025  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB042325.M  
Quant Title :  
QLast Update : Wed Apr 23 13:48:24 2025  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 5 g/ml  
Signal Phase : RTX-502.2  
Signal Info : 60mx0.53mmx3.00um

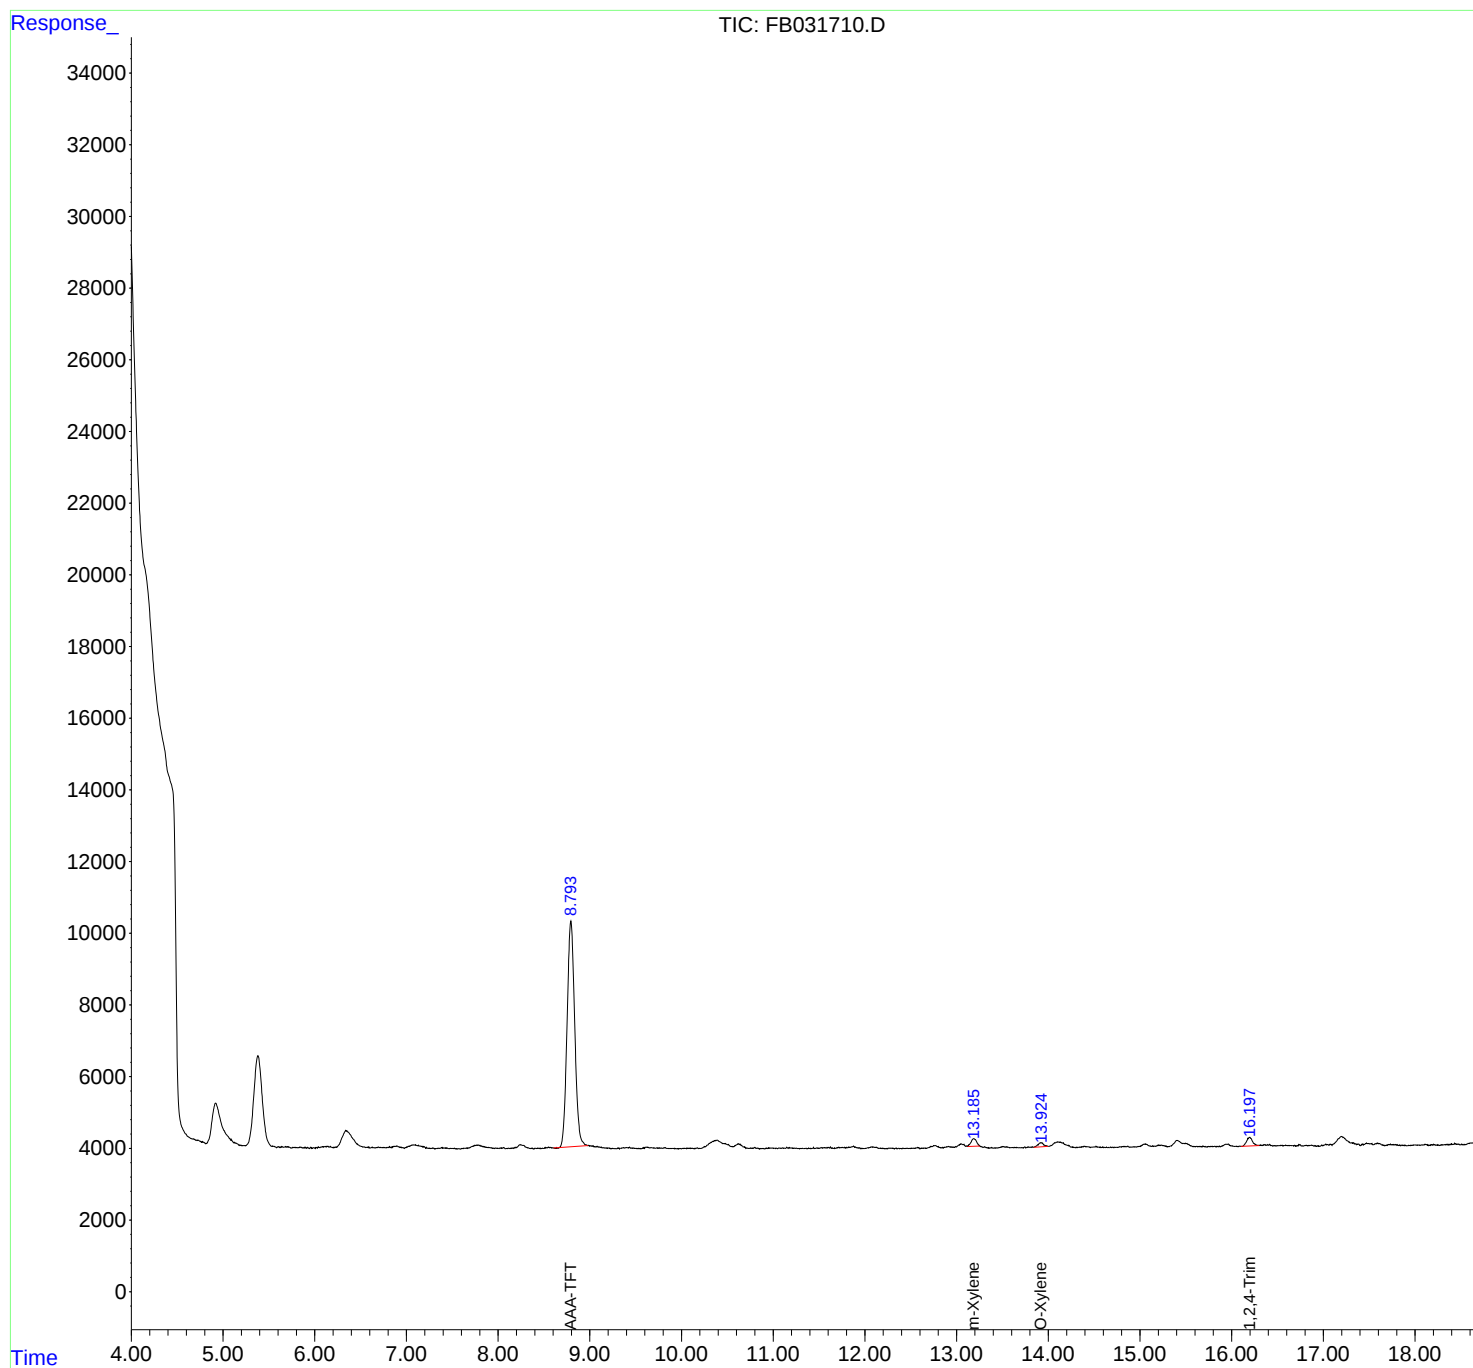


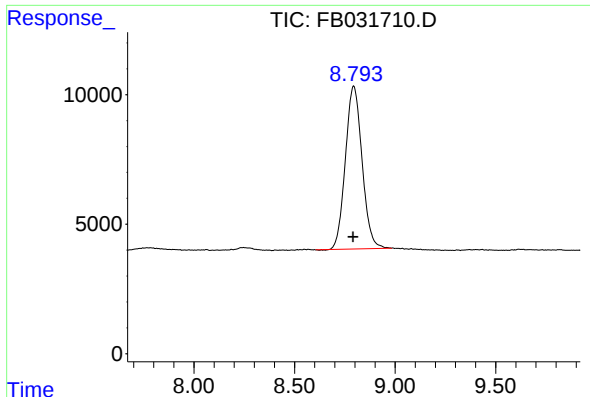

#5 AAA-TFT


R.T.: 8.794 min  
Delta R.T.: 0.002 min  
Response: 362132  
Conc: 15.79 ng/ml

Instrument :  
FID\_B  
ClientSampleId :  
TP-4

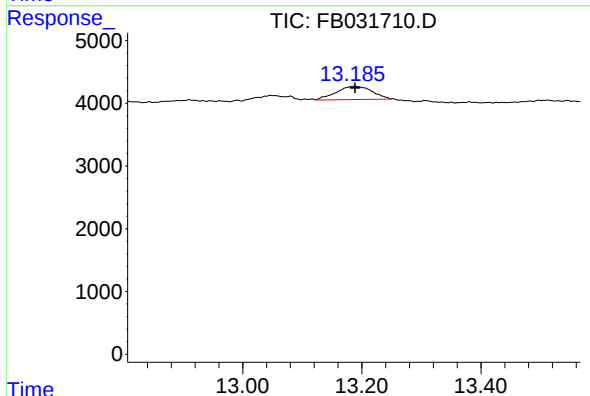


#8 m-Xylene

R.T.: 13.187 min  
Delta R.T.: -0.002 min  
Response: 8770  
Conc: 0.22 ng/ml

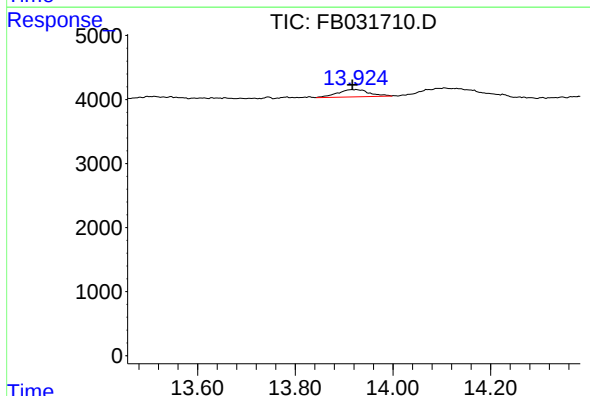

#9 o-Xylene

R.T.: 13.917 min  
Delta R.T.: 0.000 min  
Response: 5127  
Conc: 0.14 ng/ml

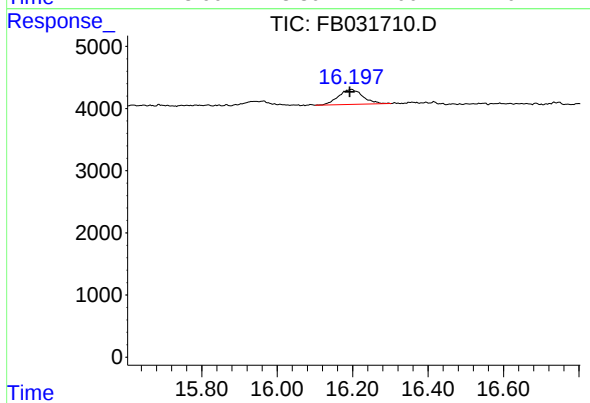

#10 1,2,4-Trimethylbenzene

R.T.: 16.199 min  
Delta R.T.: 0.006 min  
Response: 10756  
Conc: 0.40 ng/ml