

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB051325\
Data File : FB031711.D
Signal(s) : FID2B.CH
Acq On : 13 May 2025 12:21
Operator : YP/AJ
Sample : Q1982-05
Misc : 5.61G/5.00 ML DI WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
TP-5

Integration File: Calibration.e
Quant Time: May 14 07:20:48 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB042325.M
Quant Title :
QLast Update : Wed Apr 23 13:48:24 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.794	384039	16.746 ng/ml
Target Compounds			
6) t Toluene	10.616	6750	0.169 ng/ml
8) t m-Xylene	13.198	9113	0.233 ng/ml
9) t O-Xylene	13.927	4887	0.133 ng/ml
10) t 1,2,4-Trimethylbenzene	16.196	9053	0.336 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB051325\
Data File : FB031711.D
Signal(s) : FID2B.CH
Acq On : 13 May 2025 12:21
Operator : YP/AJ
Sample : Q1982-05
Misc : 5.61G/5.00 ML DI WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
TP-5

Integration File: Calibration.e
Quant Time: May 14 07:20:48 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB042325.M
Quant Title :
QLast Update : Wed Apr 23 13:48:24 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

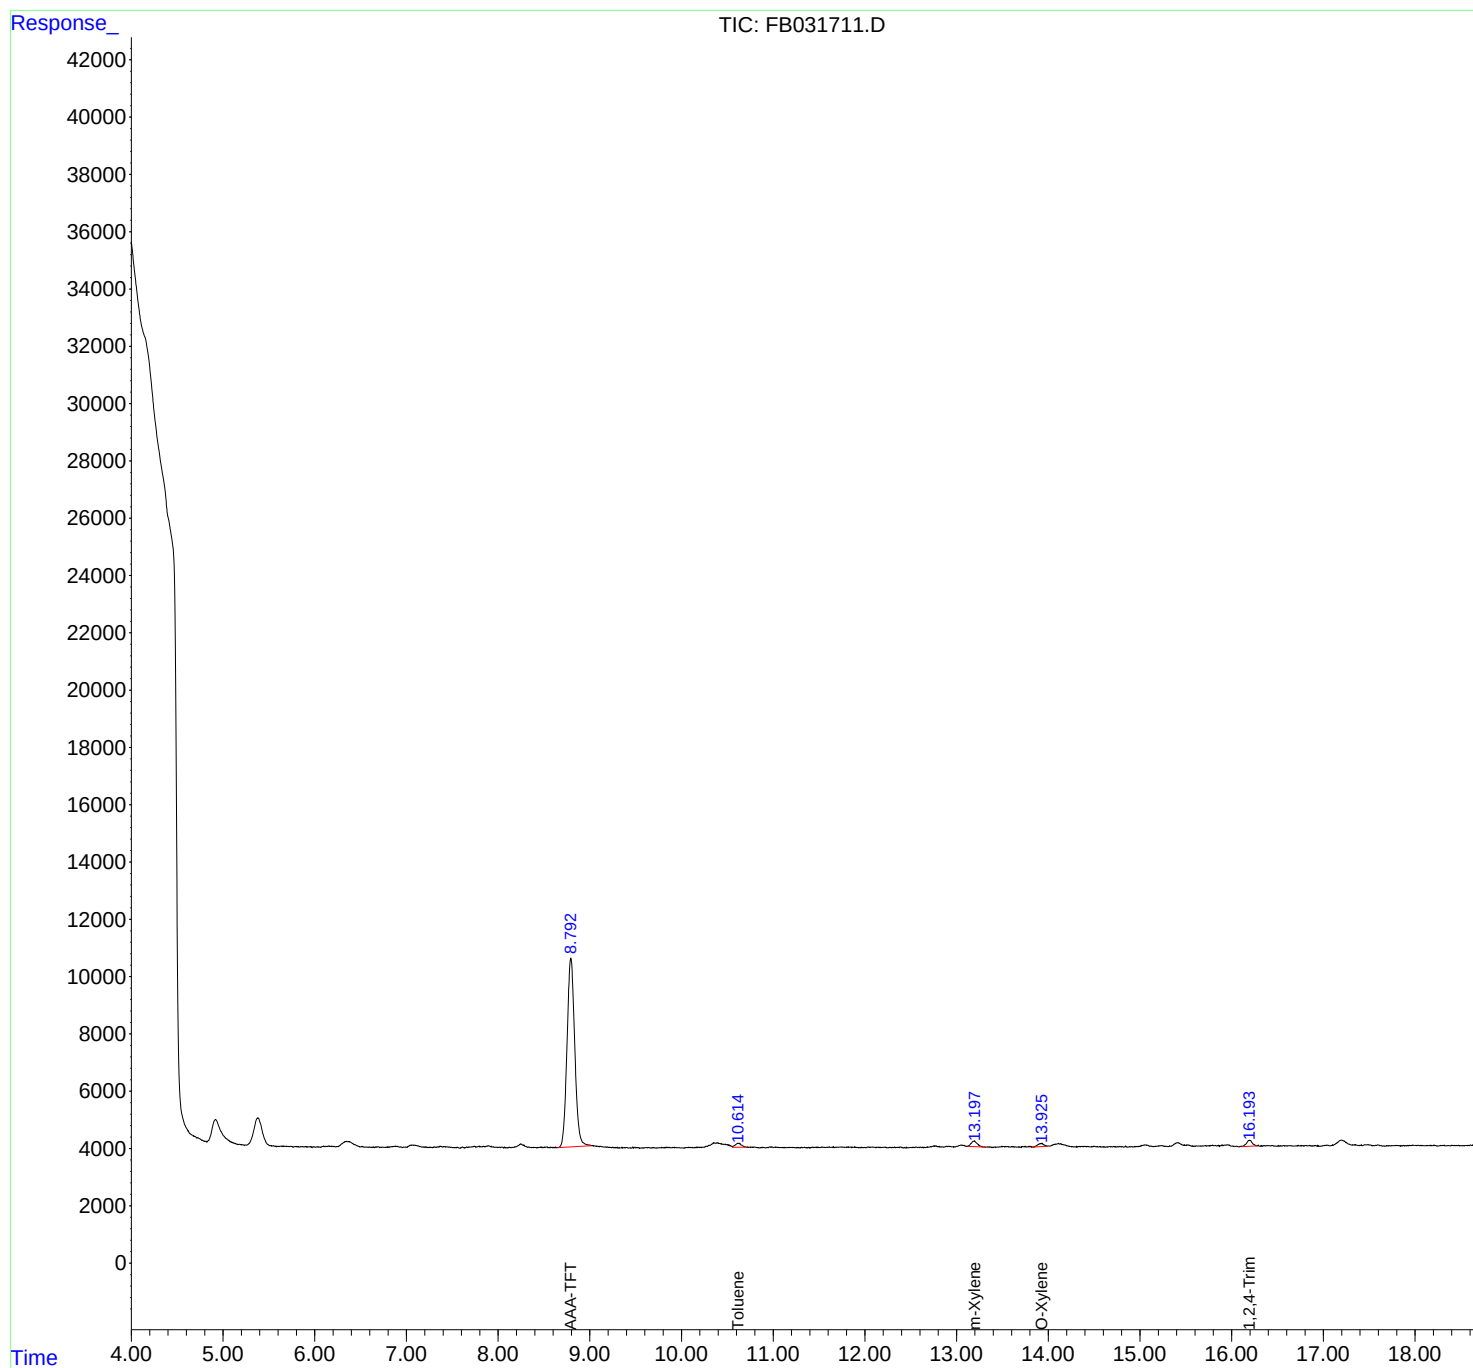


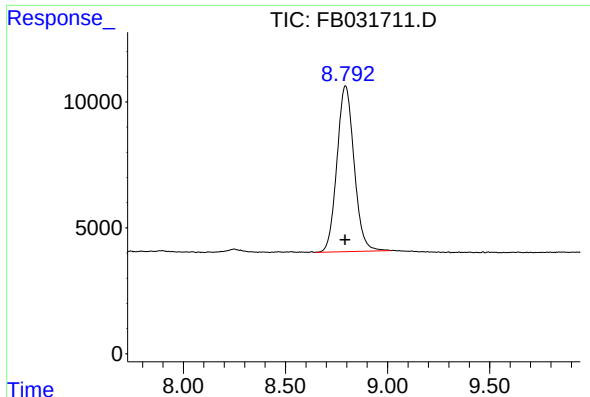

#5 AAA-TFT


R.T.: 8.794 min
Delta R.T.: 0.002 min
Response: 384039
Conc: 16.75 ng/ml

Instrument :
FID_B
ClientSampleId :
TP-5

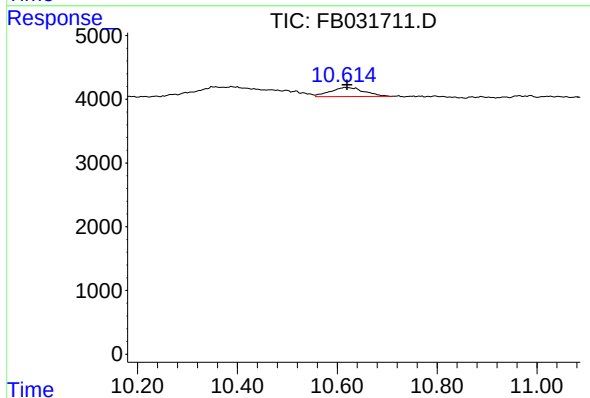


#6 Toluene

R.T.: 10.616 min
Delta R.T.: -0.004 min
Response: 6750
Conc: 0.17 ng/ml

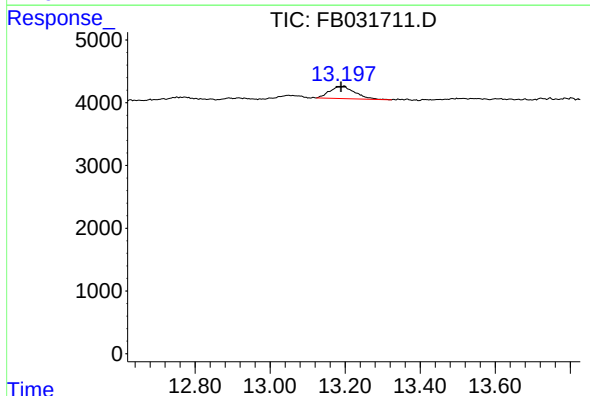


#8 m-Xylene

R.T.: 13.198 min
Delta R.T.: 0.009 min
Response: 9113
Conc: 0.23 ng/ml

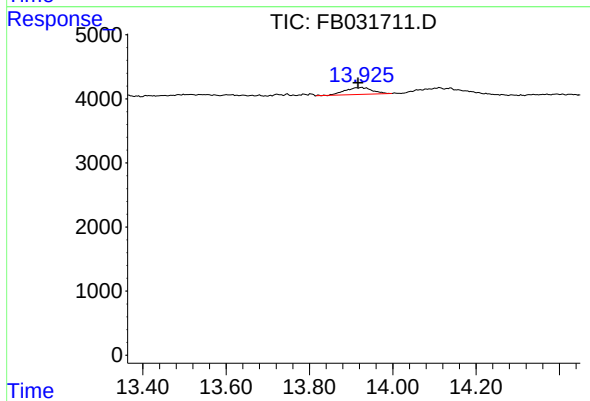

#9 O-Xylene

R.T.: 13.927 min
Delta R.T.: 0.010 min
Response: 4887
Conc: 0.13 ng/ml

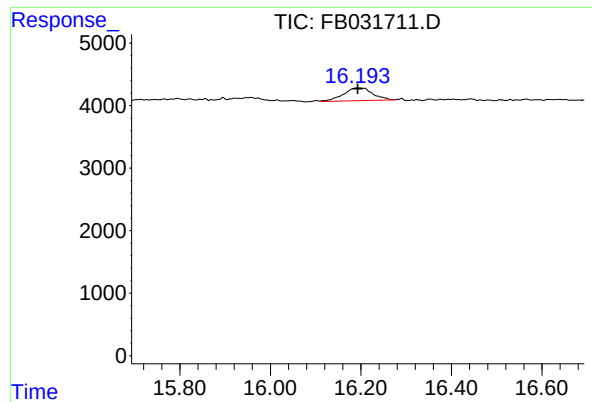

#10 1,2,4-Trimethylbenzene

R.T.: 16.196 min
Delta R.T.: 0.003 min
Response: 9053
Conc: 0.34 ng/ml

Instrument :

FID_B

ClientSampleId :

TP-5