

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB051325\
 Data File : FB031720.D
 Signal(s) : FID2B.CH
 Acq On : 13 May 2025 17:44
 Operator : YP/AJ
 Sample : Q2010-04
 Misc : 7.00G/5.00 ML DI WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: May 14 07:22:12 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB042325.M
 Quant Title :
 QLast Update : Wed Apr 23 13:48:24 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.796	387346	16.890 ng/ml
Target Compounds			
2) t 2,2,4-Trimethylpentane	7.387	9317	0.273 ng/ml
4) t Benzene	7.896	262289	6.414 ng/ml
6) t Toluene	10.621	10857	0.273 ng/ml
7) t Ethylbenzene	13.065	4936	0.138 ng/ml
8) t m-Xylene	13.185	24514	0.627 ng/ml
9) t O-Xylene	13.919	18772	0.510 ng/ml
10) t 1,2,4-Trimethylbenzene	16.204	7729	0.287 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB051325\
Data File : FB031720.D
Signal(s) : FID2B.CH
Acq On : 13 May 2025 17:44
Operator : YP/AJ
Sample : Q2010-04
Misc : 7.00G/5.00 ML DI WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: May 14 07:22:12 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB042325.M
Quant Title :
QLast Update : Wed Apr 23 13:48:24 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

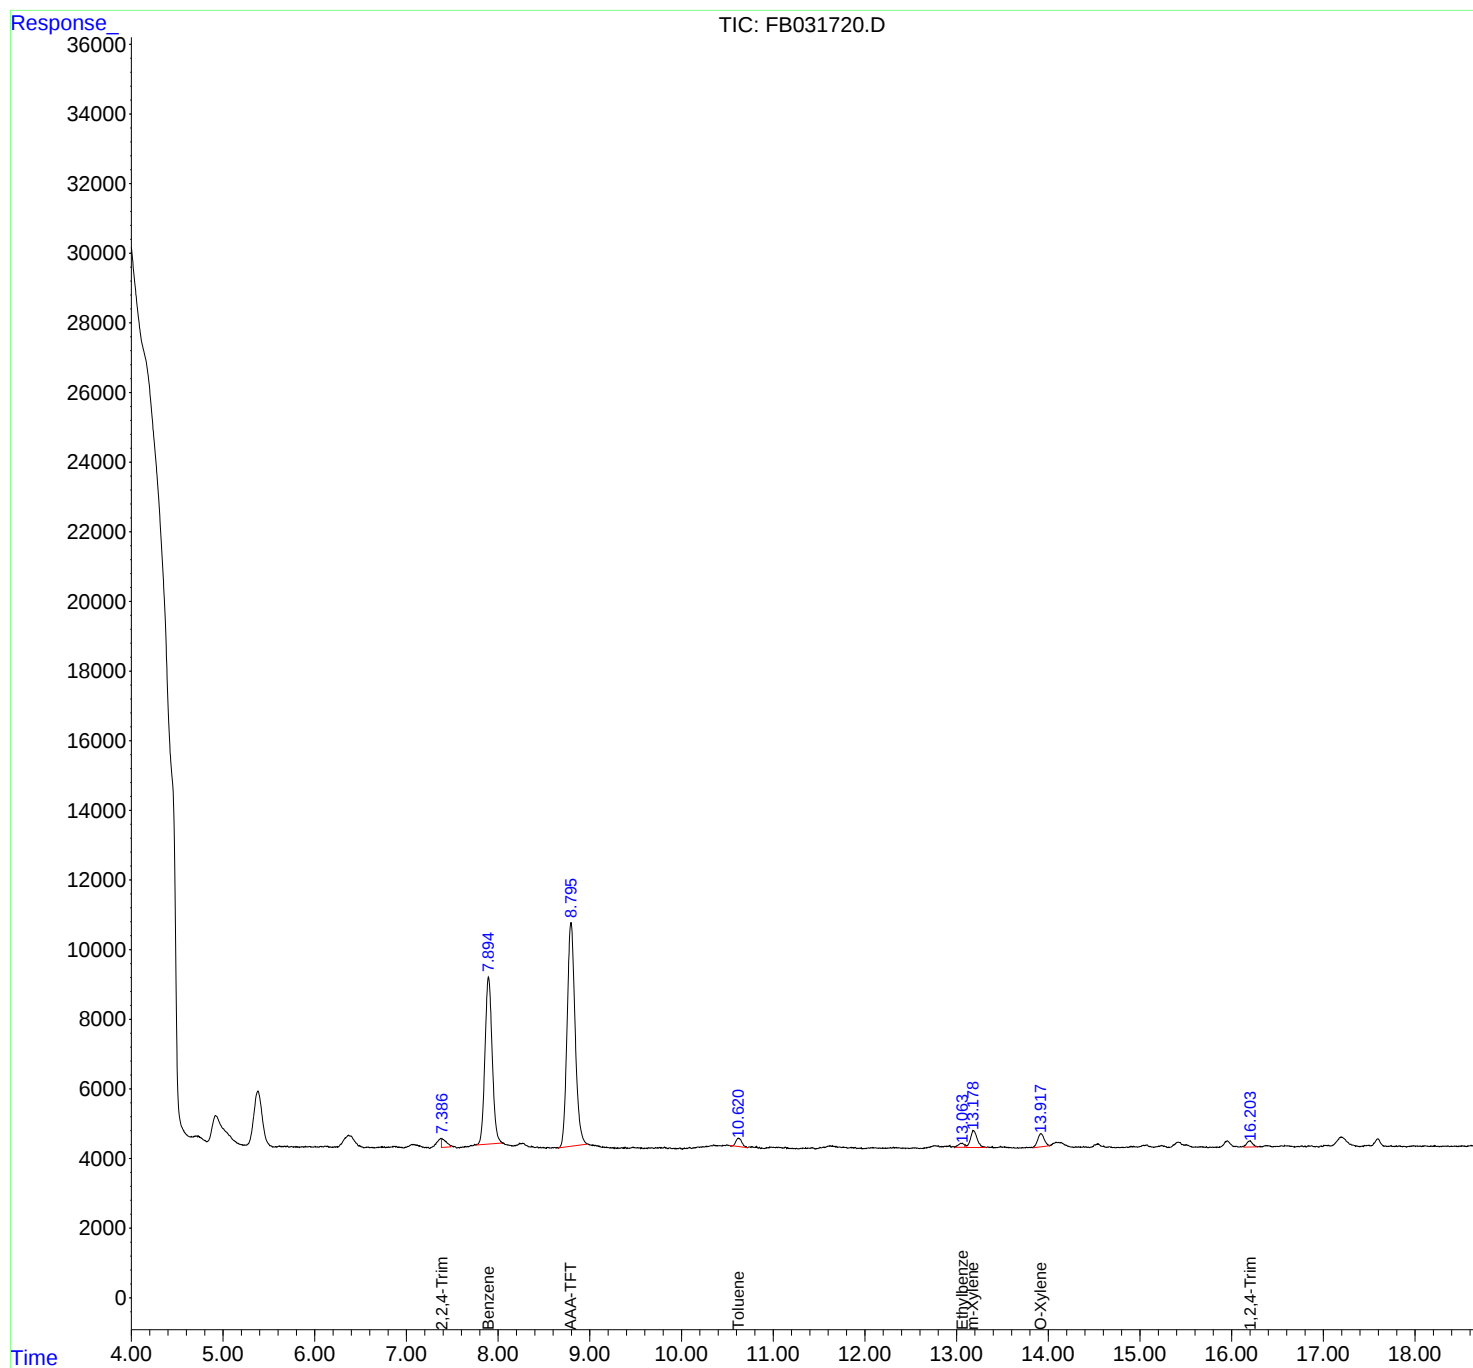


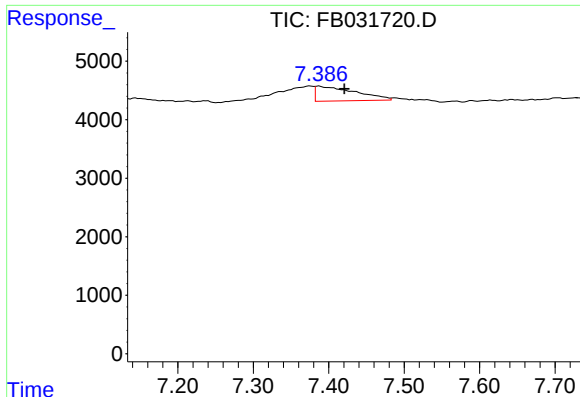

#2 2,2,4-Trimethylpentane


R.T.: 7.387 min
Delta R.T.: -0.033 min
Response: 9317
Conc: 0.27 ng/ml

Instrument :
FID_B
ClientSampleId :

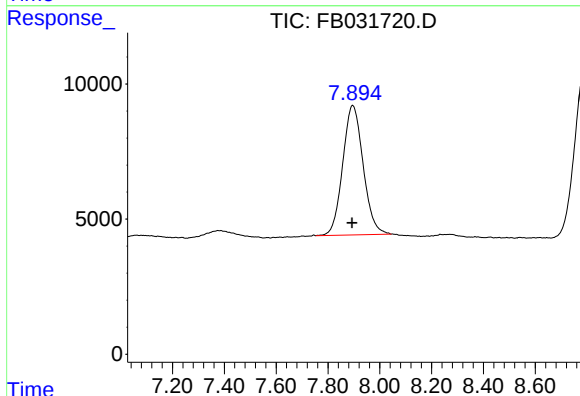


#4 Benzene

R.T.: 7.896 min
Delta R.T.: 0.002 min
Response: 262289
Conc: 6.41 ng/ml

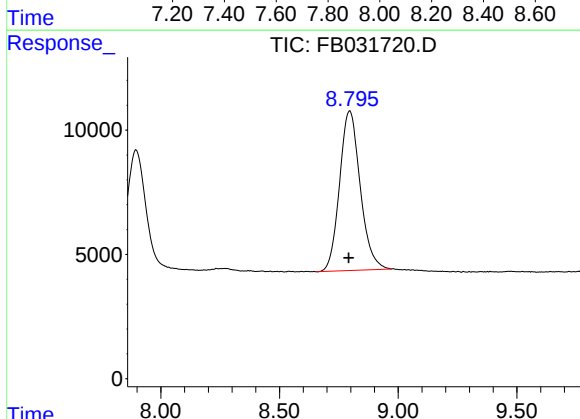


#5 AAA-TFT

R.T.: 8.796 min
Delta R.T.: 0.004 min
Response: 387346
Conc: 16.89 ng/ml

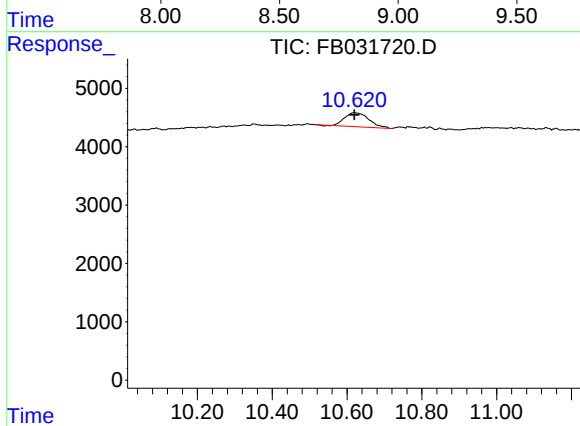

#6 Toluene


R.T.: 10.621 min
Delta R.T.: 0.002 min
Response: 10857
Conc: 0.27 ng/ml

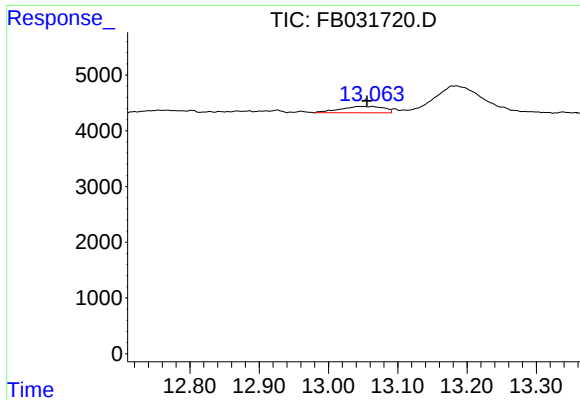

#7 Ethylbenzene


R.T.: 13.065 min
Delta R.T.: 0.009 min
Response: 4936
Conc: 0.14 ng/ml

Instrument :
FID_B
ClientSampleId :

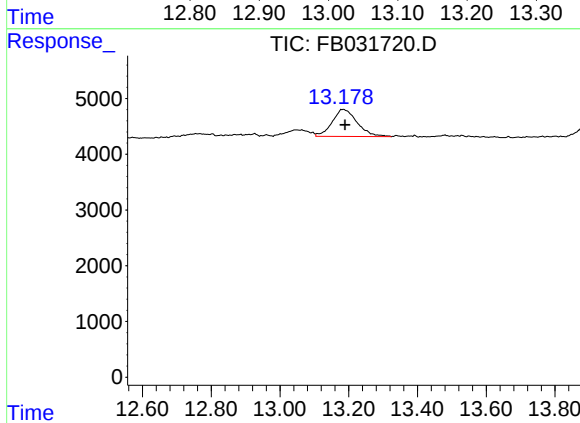


#8 m-Xylene

R.T.: 13.185 min
Delta R.T.: -0.004 min
Response: 24514
Conc: 0.63 ng/ml

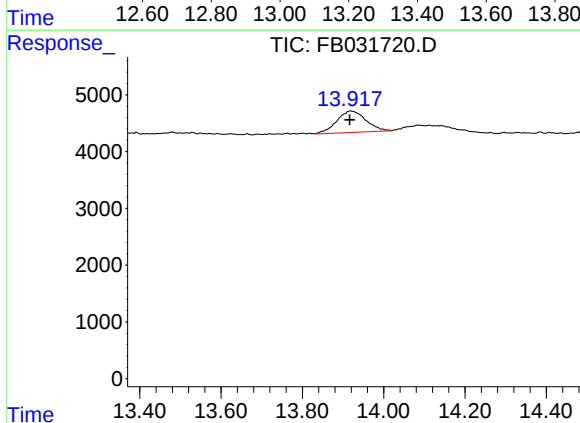

#9 o-Xylene

R.T.: 13.919 min
Delta R.T.: 0.002 min
Response: 18772
Conc: 0.51 ng/ml

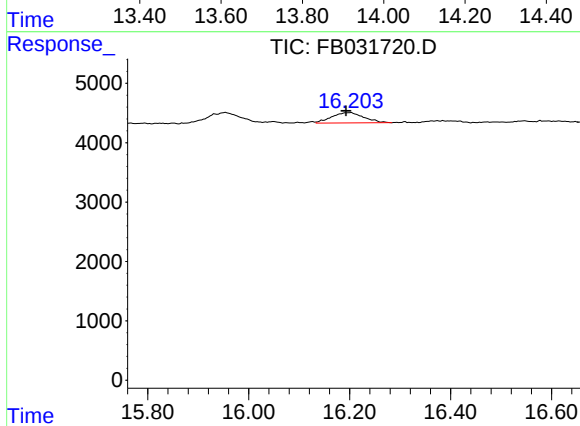

#10 1,2,4-Trimethylbenzene

R.T.: 16.204 min
Delta R.T.: 0.011 min
Response: 7729
Conc: 0.29 ng/ml