

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB051425\
Data File : FB031736.D
Signal(s) : FID2B.CH
Acq On : 14 May 2025 10:36
Operator : YP/AJ
Sample : VBF0514S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
VBF0514S1

Integration File: Calibration.e
Quant Time: May 15 04:27:43 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB042325.M
Quant Title :
QLast Update : Wed Apr 23 13:48:24 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.795	490712	21.398 ng/ml
Target Compounds			
8) t m-Xylene	13.180	6749	0.173 ng/ml
9) t O-Xylene	13.929	5425	0.147 ng/ml
10) t 1,2,4-Trimethylbenzene	16.190	4591	0.170 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB051425\
Data File : FB031736.D
Signal(s) : FID2B.CH
Acq On : 14 May 2025 10:36
Operator : YP/AJ
Sample : VBF0514S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
VBF0514S1

Integration File: Calibration.e
Quant Time: May 15 04:27:43 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB042325.M
Quant Title :
QLast Update : Wed Apr 23 13:48:24 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

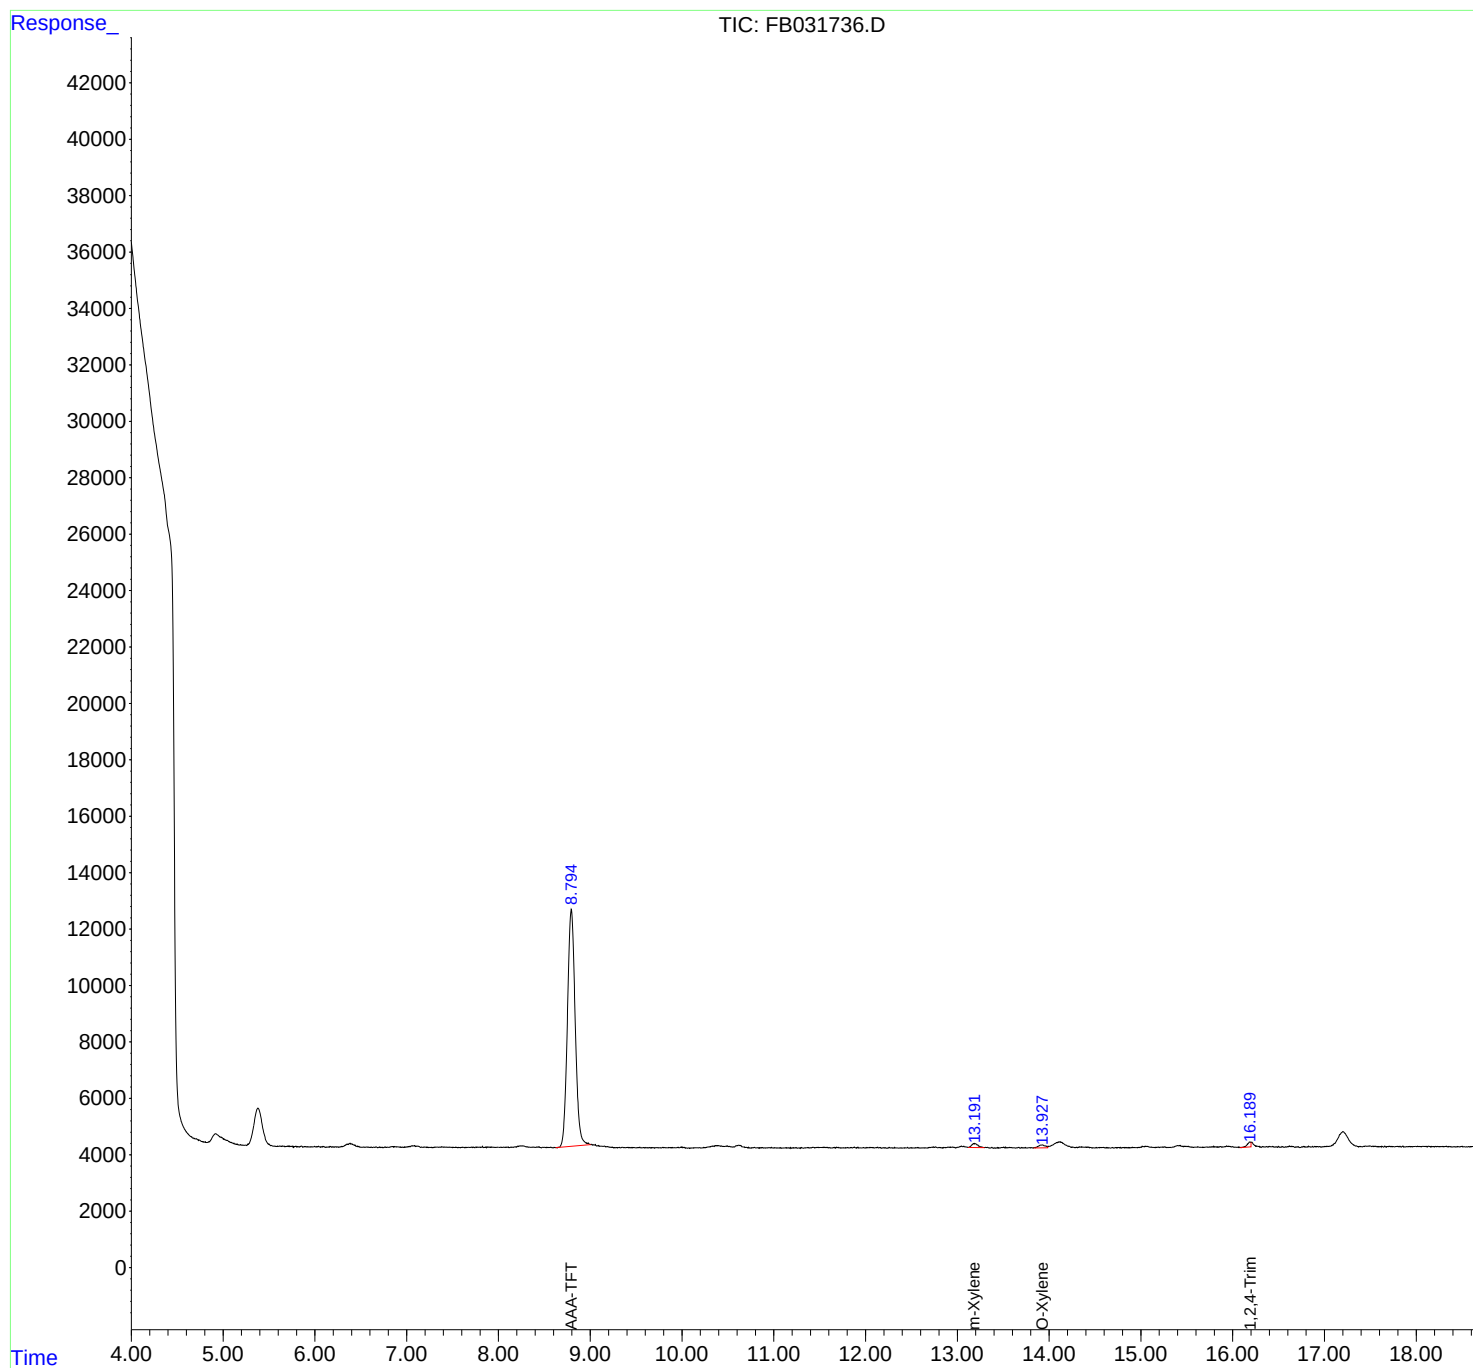


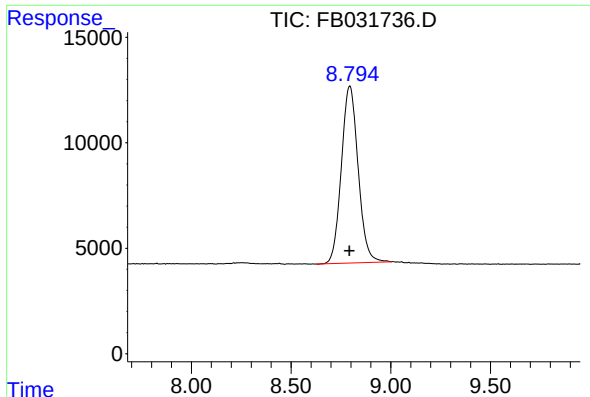

#5 AAA-TFT


R.T.: 8.795 min
Delta R.T.: 0.003 min
Response: 490712
Conc: 21.40 ng/ml

Instrument :
FID_B
ClientSampleId :
VBF0514S1

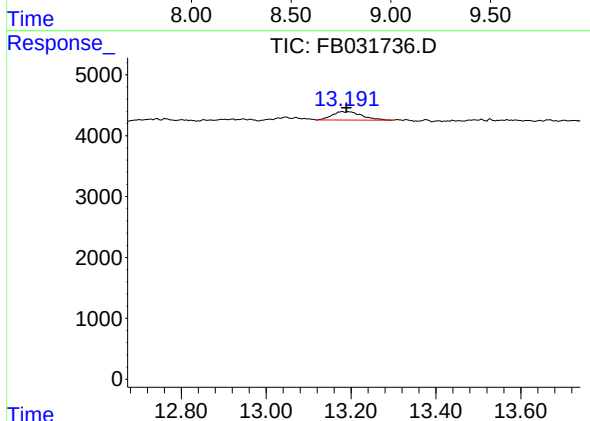


#8 m-Xylene

R.T.: 13.180 min
Delta R.T.: -0.009 min
Response: 6749
Conc: 0.17 ng/ml

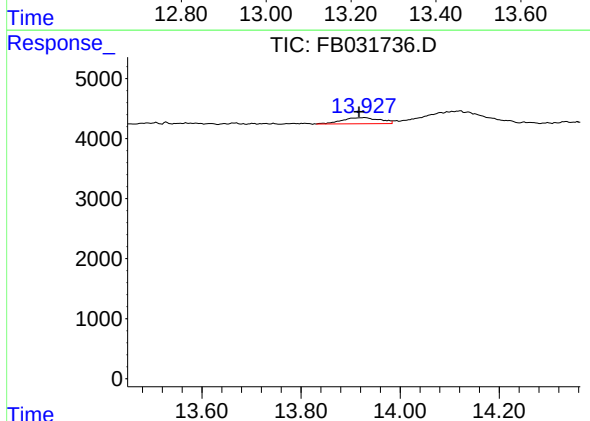

#9 o-Xylene

R.T.: 13.929 min
Delta R.T.: 0.012 min
Response: 5425
Conc: 0.15 ng/ml

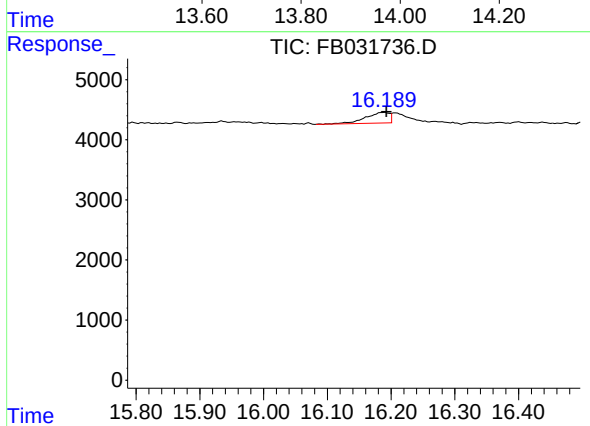

#10 1,2,4-Trimethylbenzene

R.T.: 16.190 min
Delta R.T.: -0.003 min
Response: 4591
Conc: 0.17 ng/ml