

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB051519\
 Data File : FB021035.D
 Signal(s) : FID2B.CH
 Acq On : 15 May 2019 10:44
 Operator : MJ/SJ
 Sample : BSF0515S1
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: May 16 02:22:32 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB042919.M
 Quant Title :
 QLast Update : Mon Apr 29 15:53:58 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.996	410198	22.866 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.857	1274666	28.258 ng/ml
2) t 2,2,4-Trimethylpentane	7.612	1246167	29.896 ng/ml
3) t n-Heptane	7.952	388572	9.815 ng/ml
4) t Benzene	8.088	419830	10.035 ng/ml
6) t Toluene	10.840	816598	29.478 ng/ml
7) t Ethylbenzene	13.292	258509	9.217 ng/ml
8) t m-Xylene	13.424	558784	18.801 ng/ml
9) t O-Xylene	14.155	579919	18.709 ng/ml
10) t 1,2,4-Trimethylbenzene	16.441	603617	19.463 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB051519\
Data File : FB021035.D
Signal(s) : FID2B.CH
Acq On : 15 May 2019 10:44
Operator : MJ/SJ
Sample : BSF0515S1
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: May 16 02:22:32 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB042919.M
Quant Title :
QLast Update : Mon Apr 29 15:53:58 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

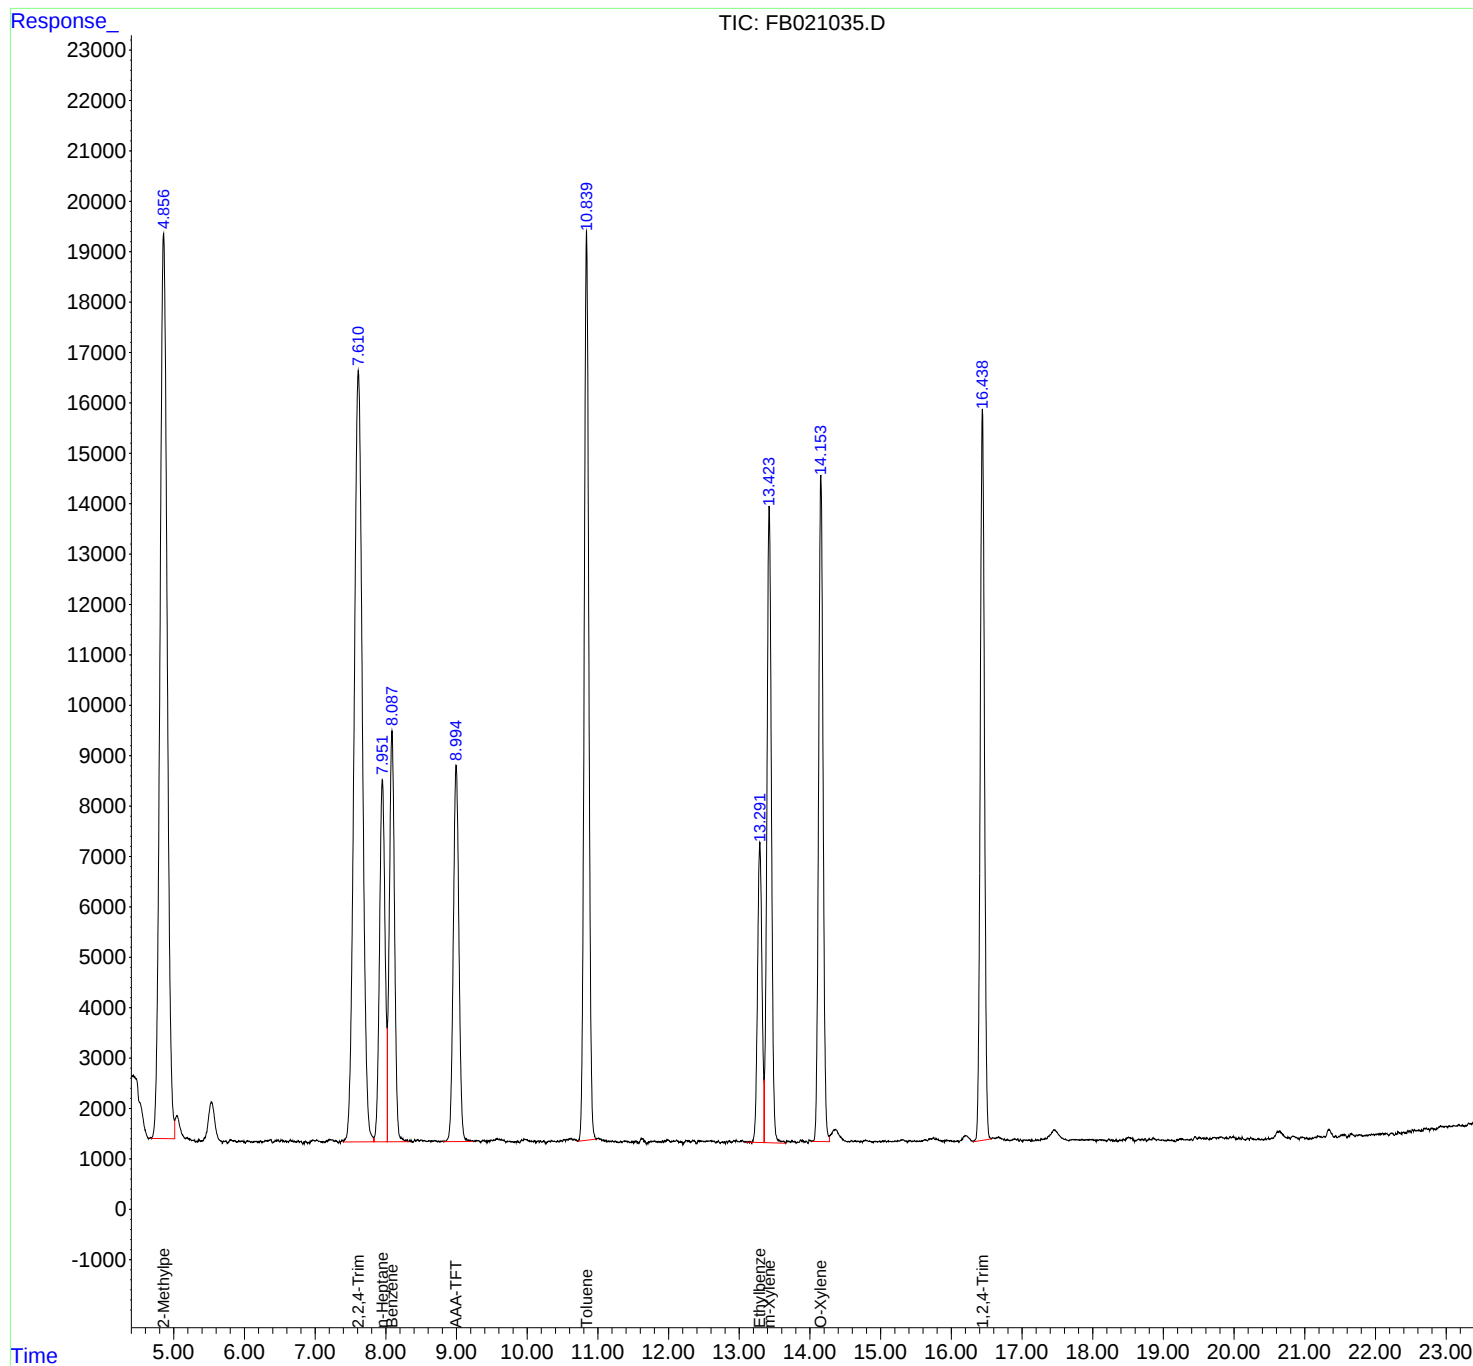

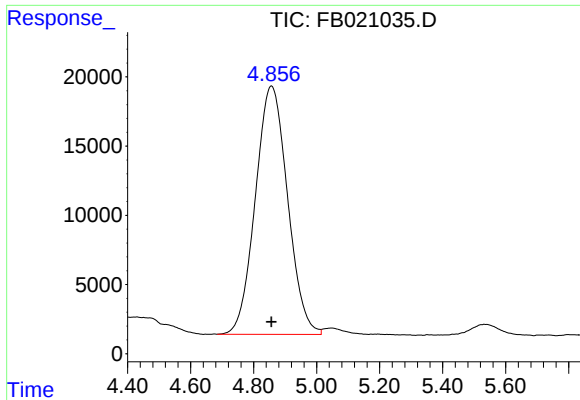


#1 2-Methylpentane

R.T.: 4.857 min
Delta R.T.: 0.000 min
Response: 1274666
Conc: 28.26 ng/ml

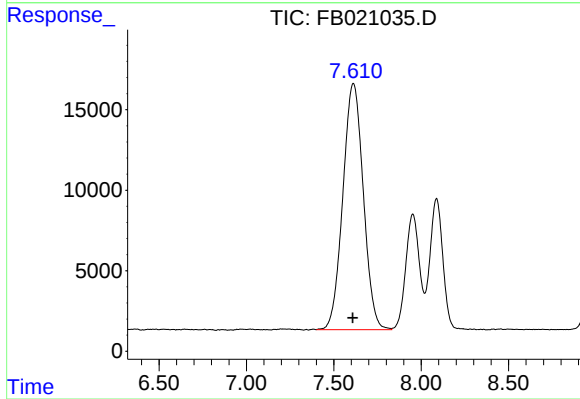


#2 2,2,4-Trimethylpentane

R.T.: 7.612 min
Delta R.T.: 0.003 min
Response: 1246167
Conc: 29.90 ng/ml

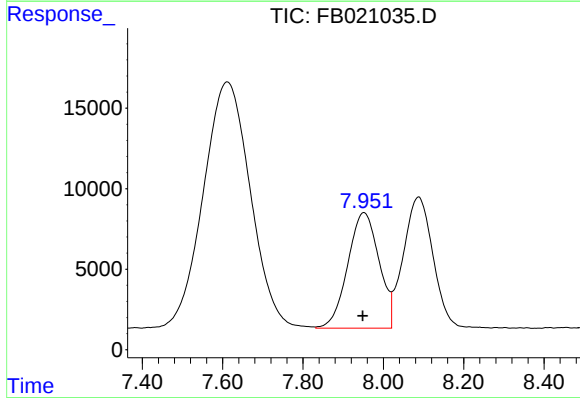


#3 n-Heptane

R.T.: 7.952 min
Delta R.T.: 0.004 min
Response: 388572
Conc: 9.82 ng/ml

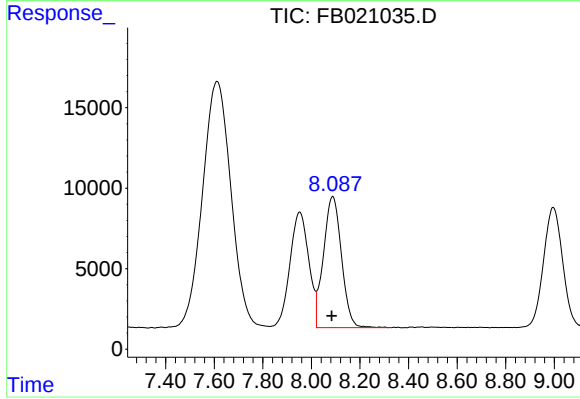


#4 Benzene

R.T.: 8.088 min
Delta R.T.: 0.004 min
Response: 419830
Conc: 10.04 ng/ml

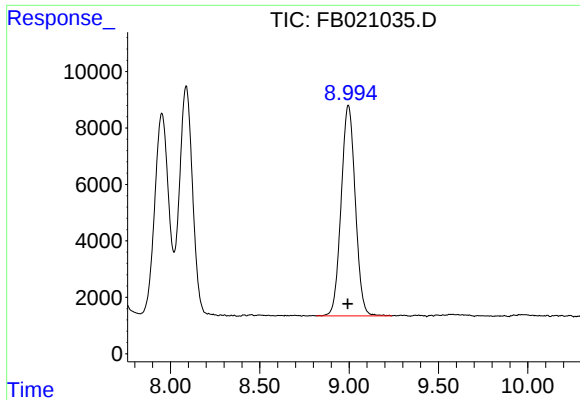


#5 AAA-TFT

R.T.: 8.996 min
Delta R.T.: 0.004 min
Response: 410198
Conc: 22.87 ng/ml

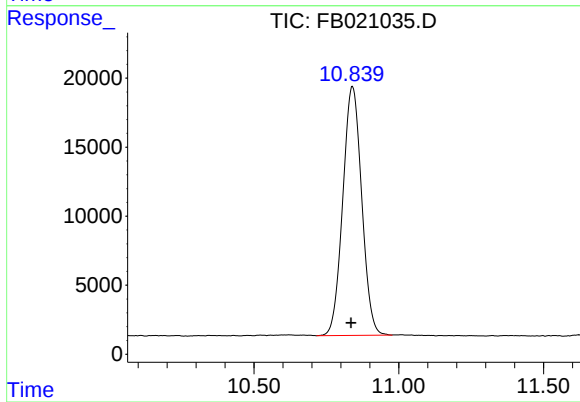


#6 Toluene

R.T.: 10.840 min
Delta R.T.: 0.005 min
Response: 816598
Conc: 29.48 ng/ml

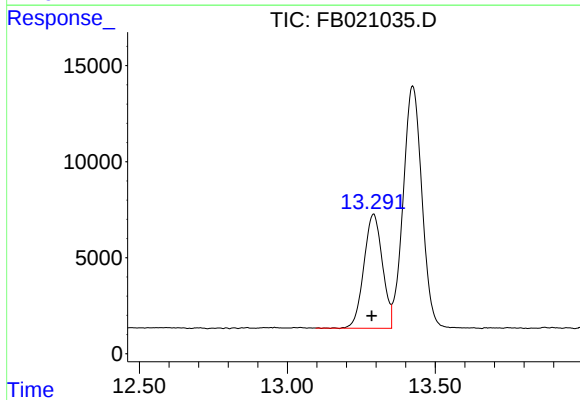


#7 Ethylbenzene

R.T.: 13.292 min
Delta R.T.: 0.006 min
Response: 258509
Conc: 9.22 ng/ml

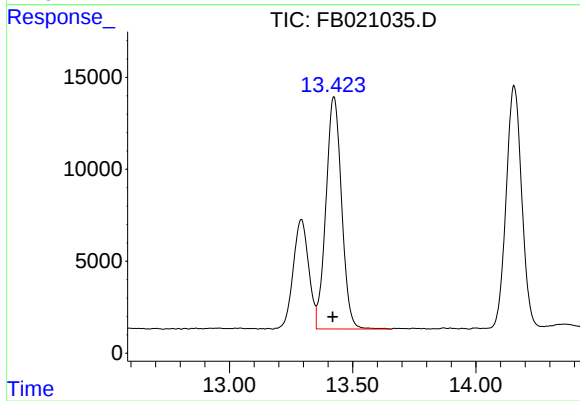

#8 m-Xylene

R.T.: 13.424 min
Delta R.T.: 0.005 min
Response: 558784
Conc: 18.80 ng/ml

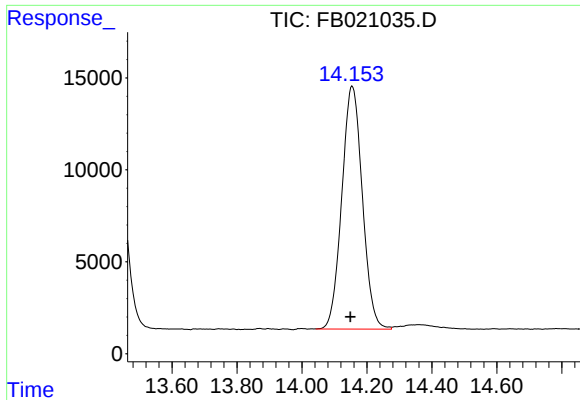


#9 O-Xylene

R.T.: 14.155 min

Delta R.T.: 0.006 min

Response: 579919

Conc: 18.71 ng/ml

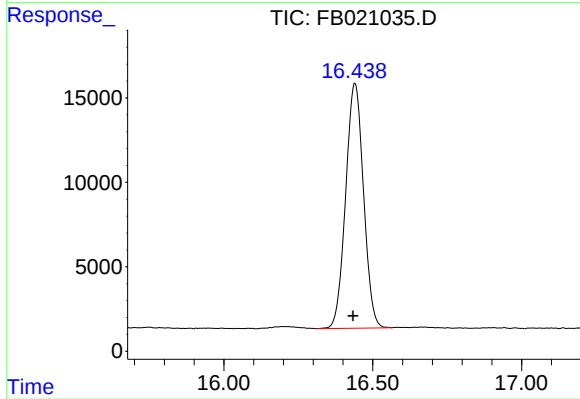

#10 1,2,4-Trimethylbenzene

R.T.: 16.441 min

Delta R.T.: 0.007 min

Response: 603617

Conc: 19.46 ng/ml