

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB051523\
 Data File : FB029794.D
 Signal(s) : FID2B.CH
 Acq On : 15 May 2023 10:27
 Operator : YP/AJ
 Sample : BSF0515S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0515S1

Integration File: Calibration.e
 Quant Time: May 16 01:13:45 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051123.M
 Quant Title :
 QLast Update : Thu May 11 11:33:20 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.783	222477	18.269 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.703	486665	28.404 ng/ml
2) t 2,2,4-Trimethylpentane	7.407	482643	28.278 ng/ml
3) t n-Heptane	7.742	170009	9.573 ng/ml
4) t Benzene	7.878	198042	9.454 ng/ml
6) t Toluene	10.611	572808	28.132 ng/ml
7) t Ethylbenzene	13.047	180763	9.432 ng/ml
8) t m-Xylene	13.179	360322	18.701 ng/ml
9) t O-Xylene	13.906	349118	18.768 ng/ml
10) t 1,2,4-Trimethylbenzene	16.181	348248	18.722 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB051523\
Data File : FB029794.D
Signal(s) : FID2B.CH
Acq On : 15 May 2023 10:27
Operator : YP/AJ
Sample : BSF0515S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0515S1

Integration File: Calibration.e
Quant Time: May 16 01:13:45 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB051123.M
Quant Title :
QLast Update : Thu May 11 11:33:20 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

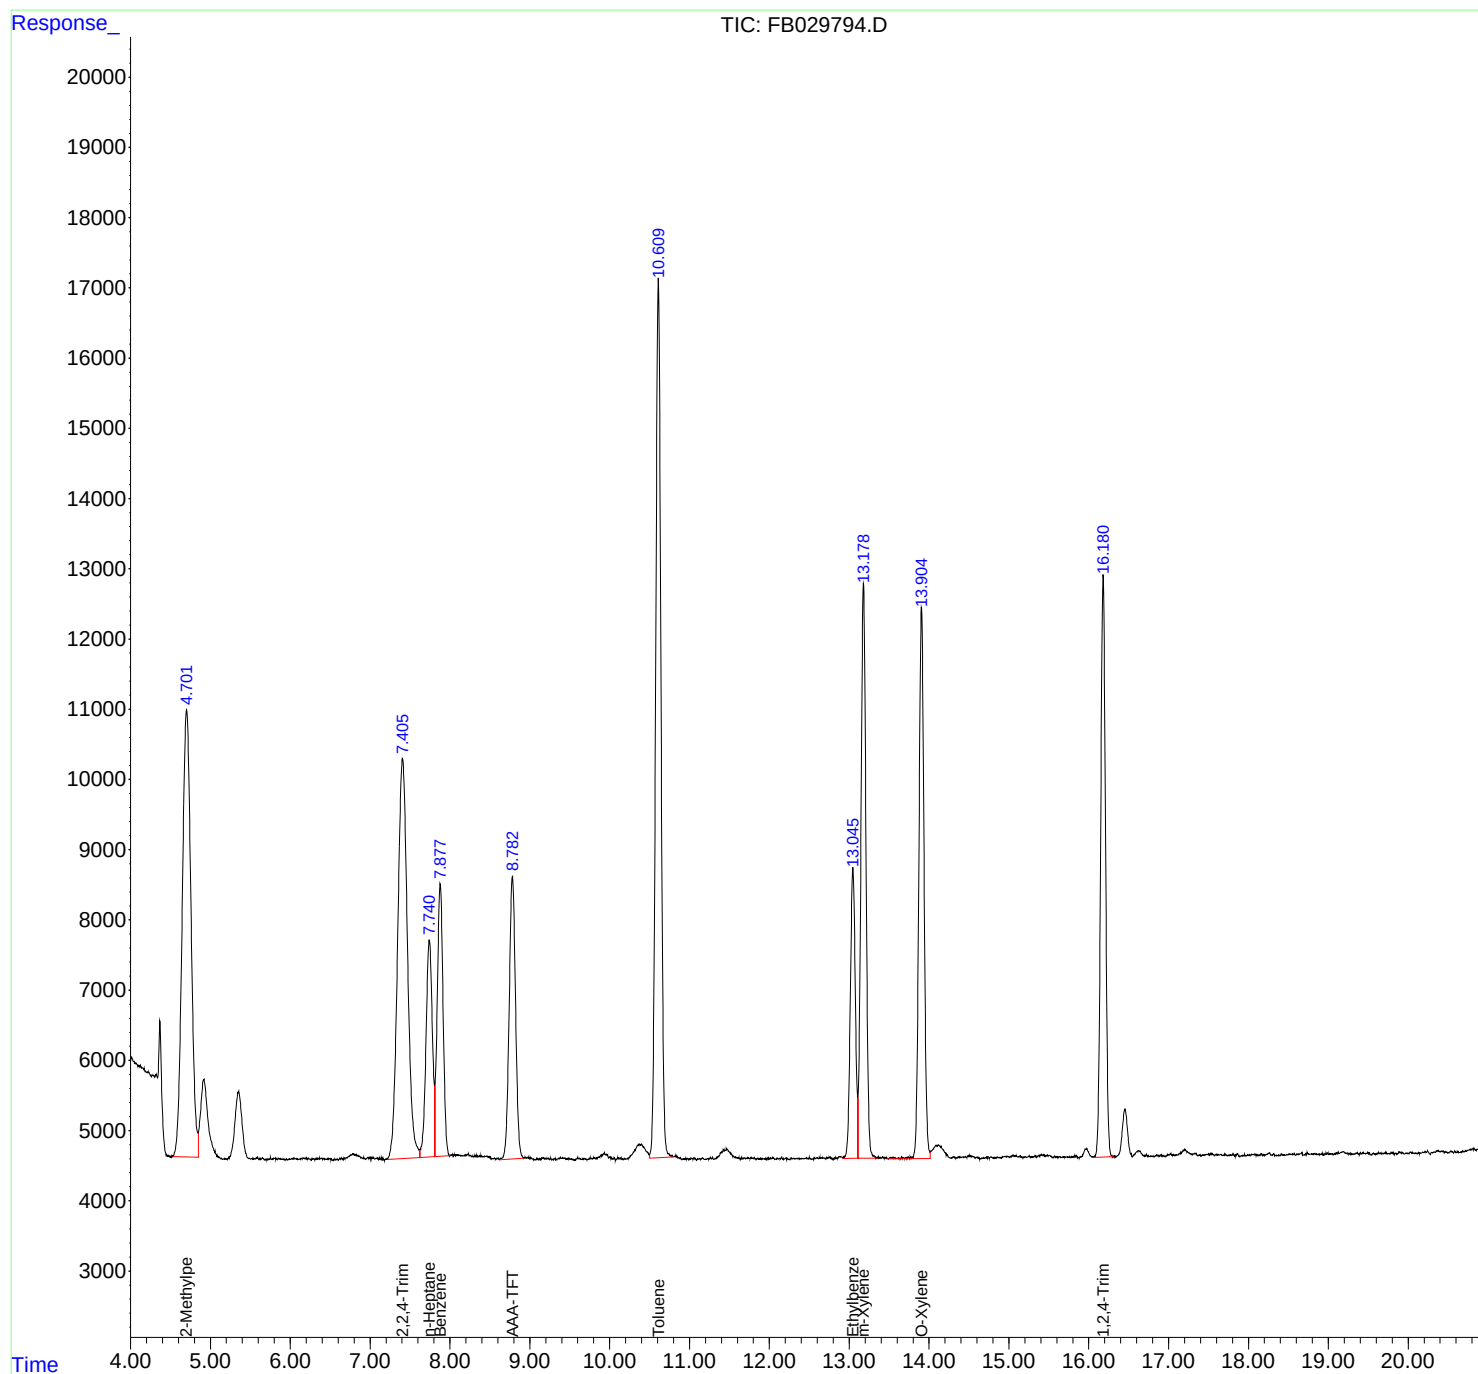


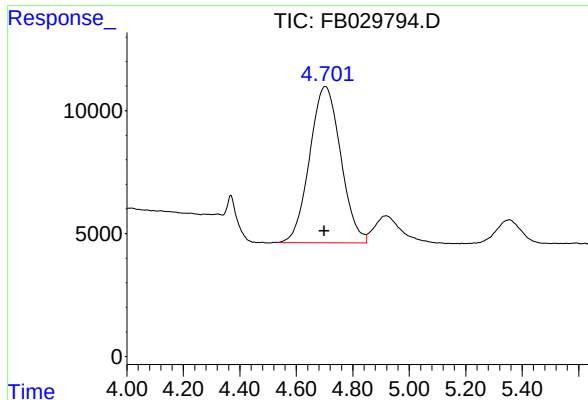

#1 2-Methylpentane


R.T.: 4.703 min
Delta R.T.: 0.004 min
Response: 486665
Conc: 28.40 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0515S1

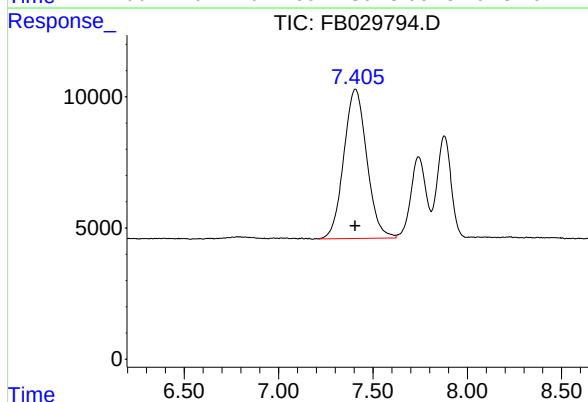


#2 2,2,4-Trimethylpentane

R.T.: 7.407 min
Delta R.T.: 0.000 min
Response: 482643
Conc: 28.28 ng/ml

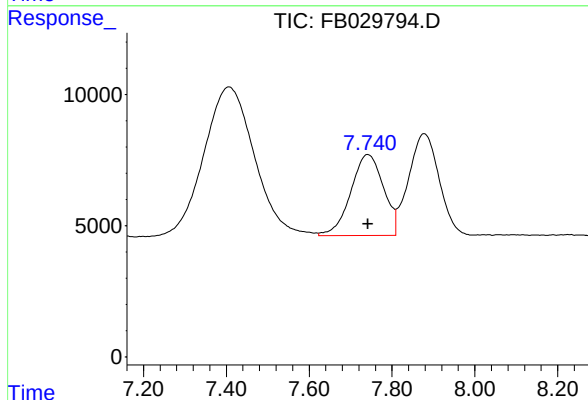


#3 n-Heptane

R.T.: 7.742 min
Delta R.T.: 0.000 min
Response: 170009
Conc: 9.57 ng/ml

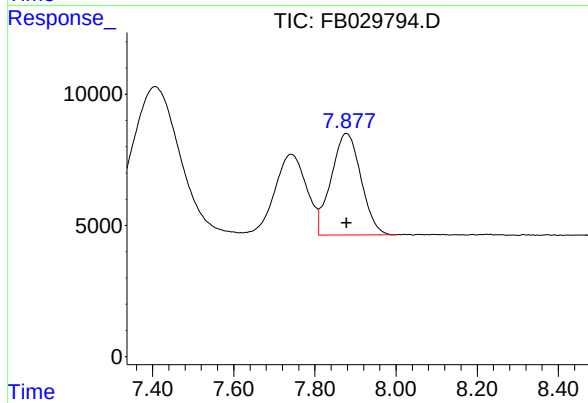

#4 Benzene


R.T.: 7.878 min
Delta R.T.: 0.000 min
Response: 198042
Conc: 9.45 ng/ml

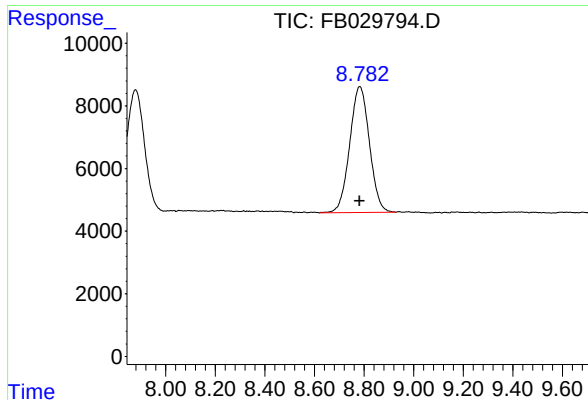

#5 AAA-TFT


R.T.: 8.783 min
Delta R.T.: 0.000 min
Response: 222477
Conc: 18.27 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0515S1

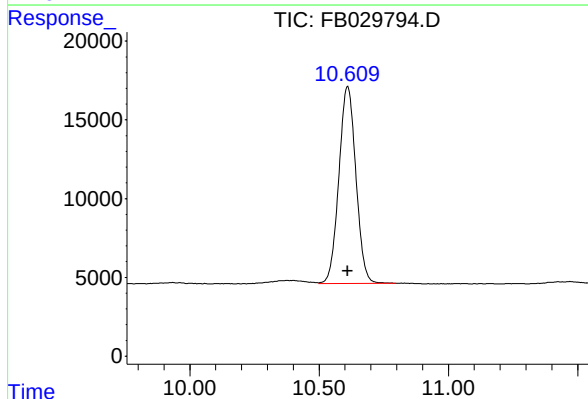


#6 Toluene

R.T.: 10.611 min
Delta R.T.: 0.000 min
Response: 572808
Conc: 28.13 ng/ml

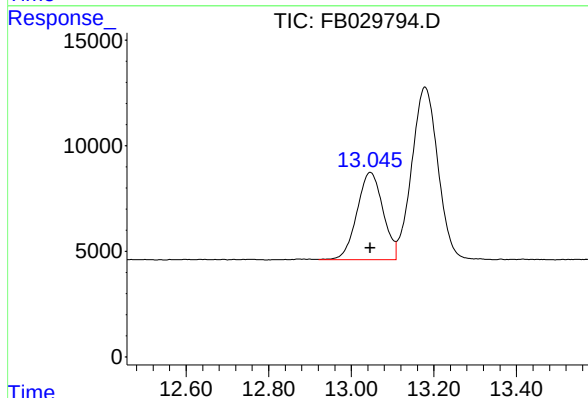


#7 Ethylbenzene

R.T.: 13.047 min
Delta R.T.: 0.000 min
Response: 180763
Conc: 9.43 ng/ml

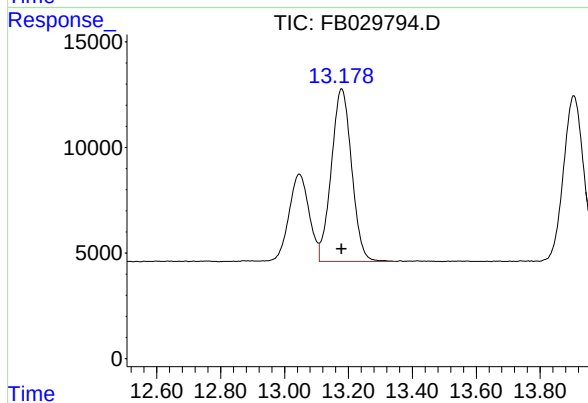

#8 m-Xylene


R.T.: 13.179 min
Delta R.T.: 0.000 min
Response: 360322
Conc: 18.70 ng/ml

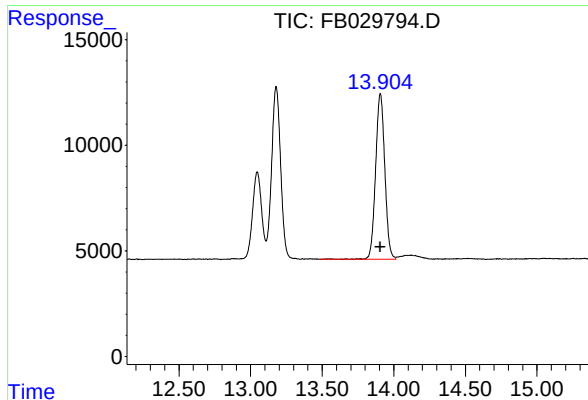

#9 O-Xylene

R.T.: 13.906 min
Delta R.T.: 0.000 min
Response: 349118
Conc: 18.77 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0515S1

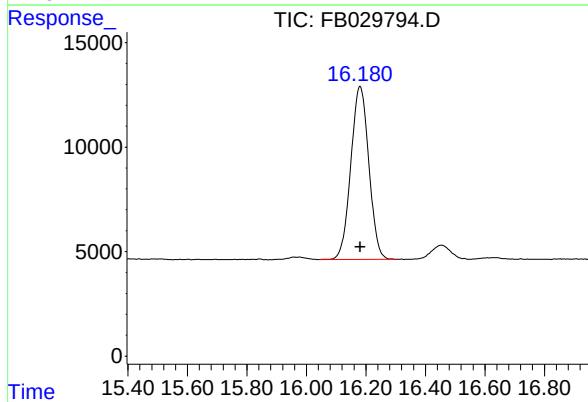

#10 1,2,4-Trimethylbenzene

R.T.: 16.181 min
Delta R.T.: 0.000 min
Response: 348248
Conc: 18.72 ng/ml