

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB051525\
Data File : FB031750.D
Signal(s) : FID2B.CH
Acq On : 15 May 2025 12:30
Operator : YP/AJ
Sample : VBF0515S2 50X
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: May 16 02:33:03 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB042325.M
Quant Title :
QLast Update : Wed Apr 23 13:48:24 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.799	525454	22.913 ng/ml
Target Compounds			
6) t Toluene	10.635	4632	0.116 ng/ml
8) t m-Xylene	13.184	1678	0.043 ng/ml
10) t 1,2,4-Trimethylbenzene	16.202	5888	0.218 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB051525\
Data File : FB031750.D
Signal(s) : FID2B.CH
Acq On : 15 May 2025 12:30
Operator : YP/AJ
Sample : VBF0515S2 50X
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: May 16 02:33:03 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB042325.M
Quant Title :
QLast Update : Wed Apr 23 13:48:24 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

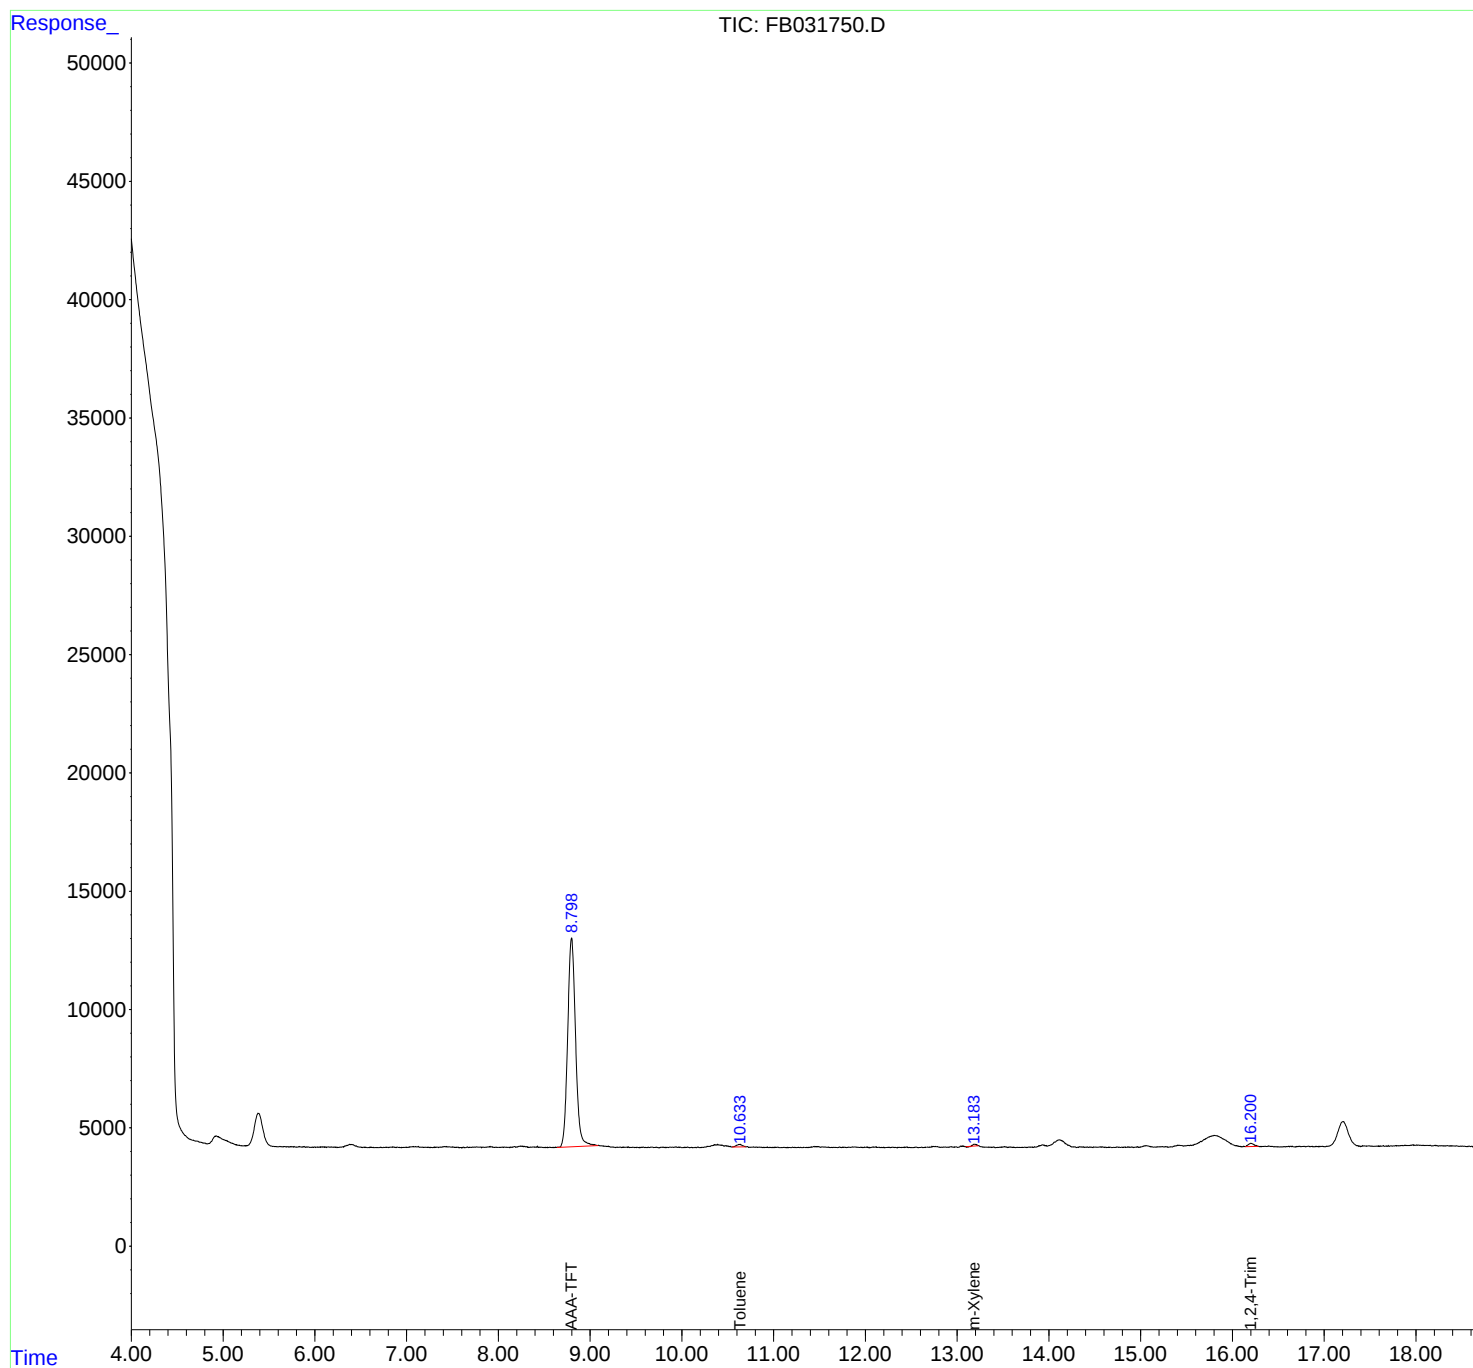


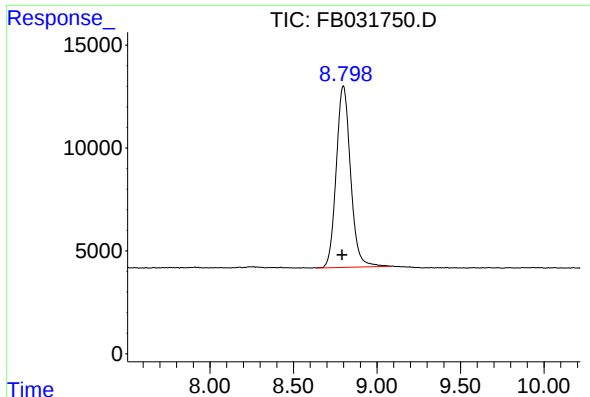

#5 AAA-TFT


R.T.: 8.799 min
Delta R.T.: 0.007 min
Response: 525454
Conc: 22.91 ng/ml

Instrument :
FID_B
ClientSampleId :

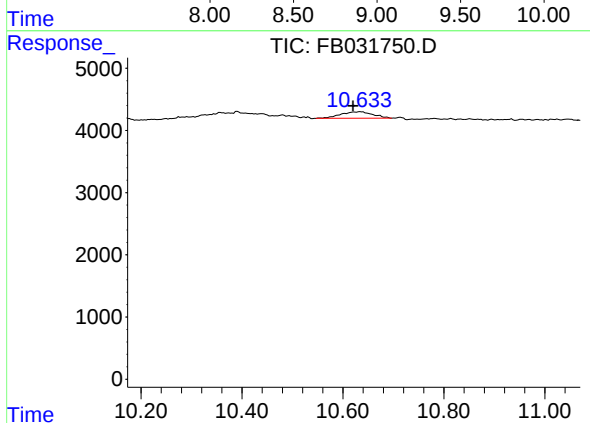


#6 Toluene

R.T.: 10.635 min
Delta R.T.: 0.015 min
Response: 4632
Conc: 0.12 ng/ml

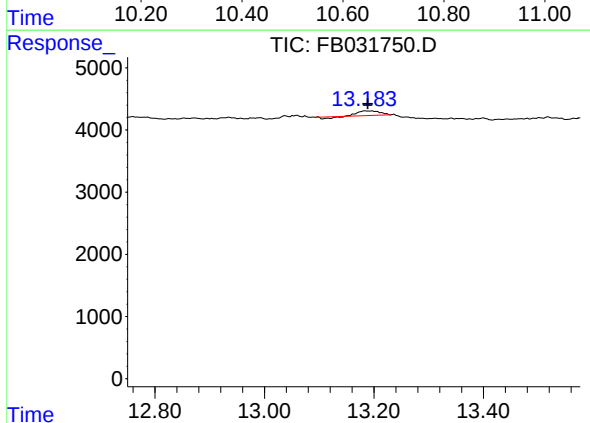

#8 m-Xylene

R.T.: 13.184 min
Delta R.T.: -0.005 min
Response: 1678
Conc: 0.04 ng/ml

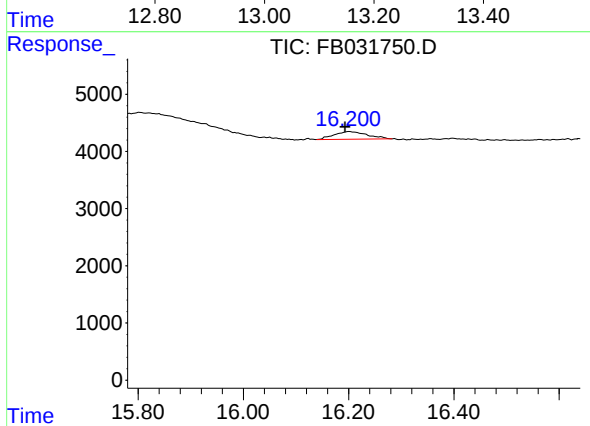

#10 1,2,4-Trimethylbenzene

R.T.: 16.202 min
Delta R.T.: 0.009 min
Response: 5888
Conc: 0.22 ng/ml