

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB051619\
 Data File : FB021061.D
 Signal(s) : FID2B.CH
 Acq On : 16 May 2019 13:14
 Operator : MJ/SJ
 Sample : K2644-01MS
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: May 16 23:15:01 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB042919.M
 Quant Title :
 QLast Update : Mon Apr 29 15:53:58 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.996	422193	23.534 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.856	1080492	23.953 ng/ml
2) t 2,2,4-Trimethylpentane	7.612	1003962	24.085 ng/ml
3) t n-Heptane	7.952	306548	7.743 ng/ml
4) t Benzene	8.088	403121	9.636 ng/ml
6) t Toluene	10.841	777634	28.072 ng/ml
7) t Ethylbenzene	13.291	225246	8.031 ng/ml
8) t m-Xylene	13.425	479786	16.143 ng/ml
9) t O-Xylene	14.156	508826	16.416 ng/ml
10) t 1,2,4-Trimethylbenzene	16.440	494791	15.954 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB051619\
Data File : FB021061.D
Signal(s) : FID2B.CH
Acq On : 16 May 2019 13:14
Operator : MJ/SJ
Sample : K2644-01MS
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: May 16 23:15:01 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB042919.M
Quant Title :
QLast Update : Mon Apr 29 15:53:58 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

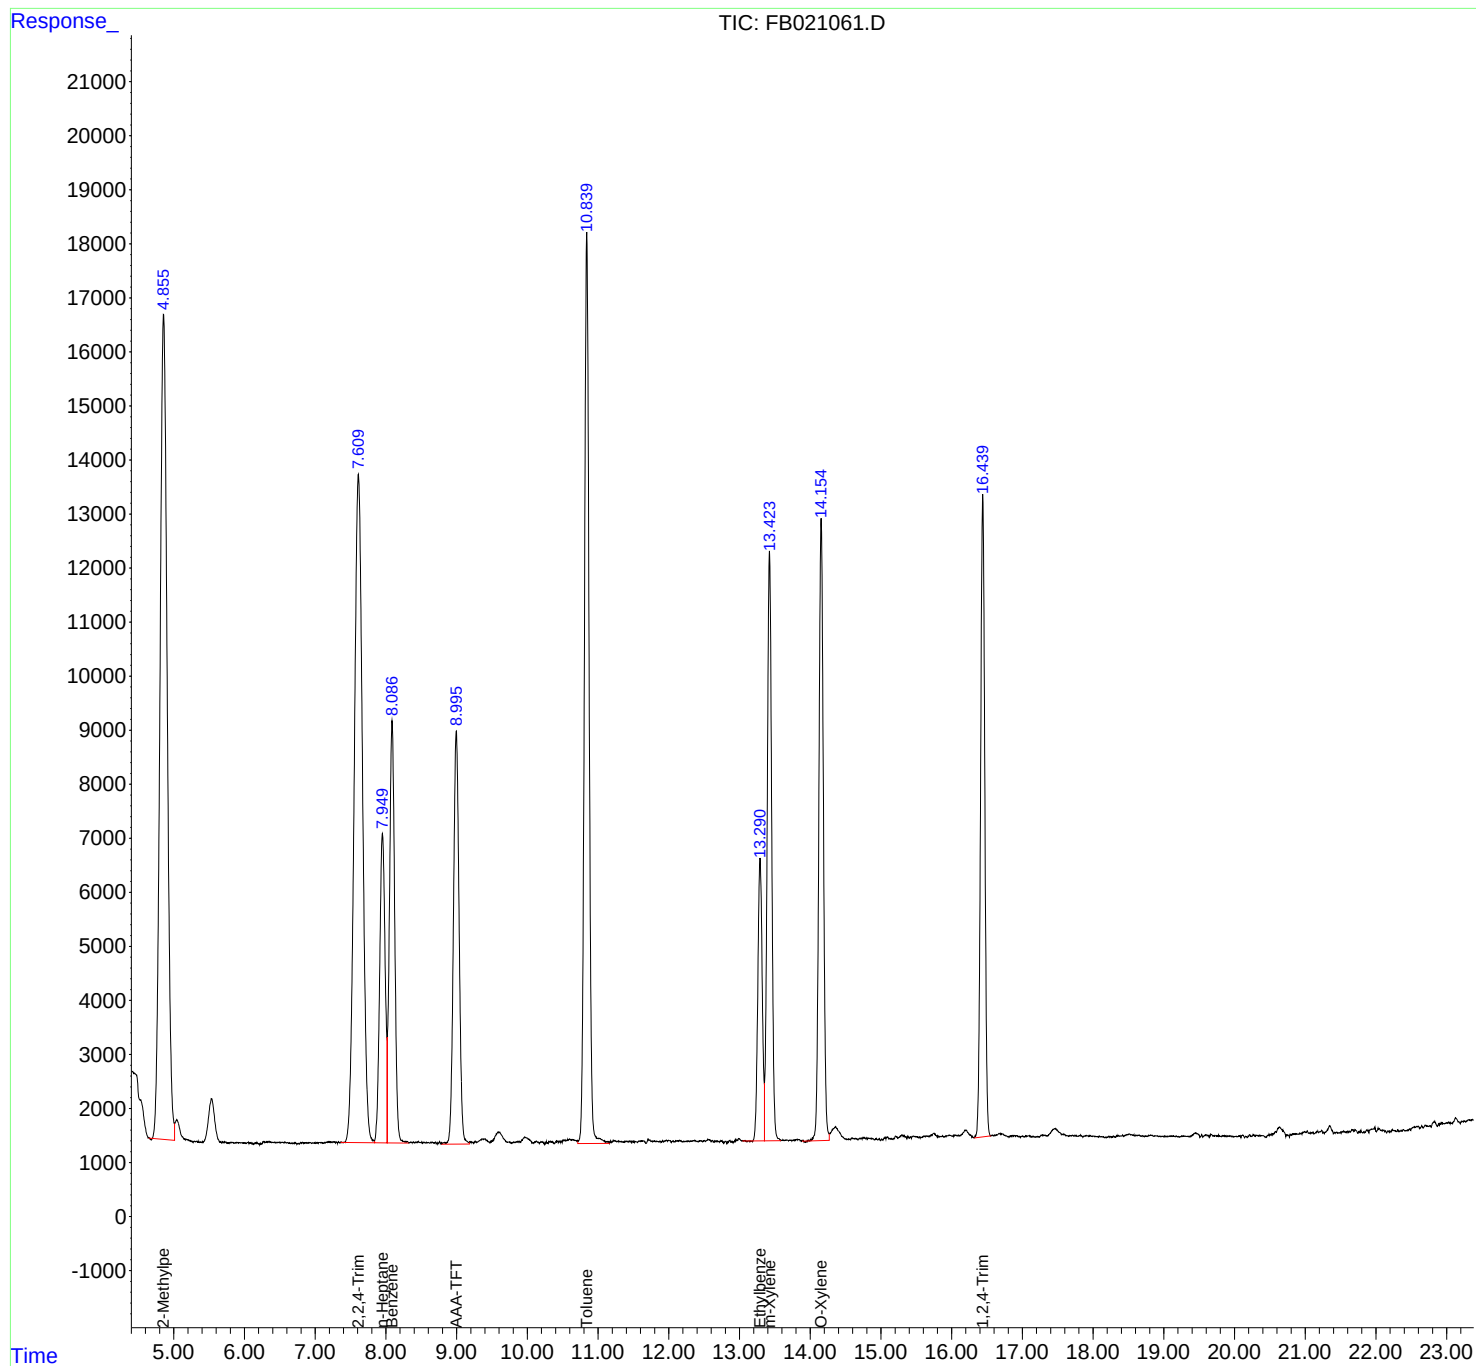


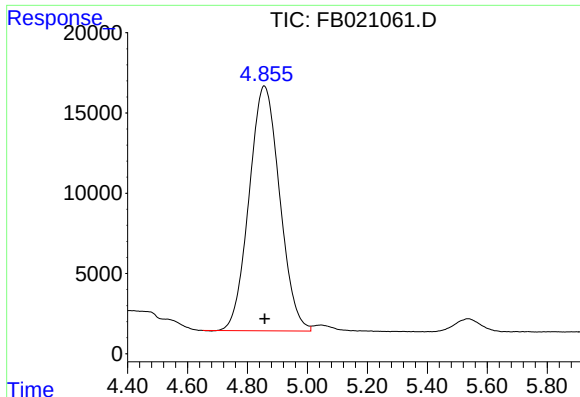

#1 2-Methylpentane


R.T.: 4.856 min
Delta R.T.: 0.000 min
Response: 1080492
Conc: 23.95 ng/ml

Instrument :
FID_B
ClientSampleId :

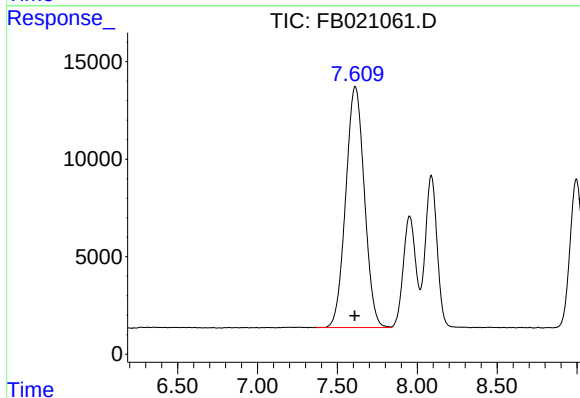


#2 2,2,4-Trimethylpentane

R.T.: 7.612 min
Delta R.T.: 0.003 min
Response: 1003962
Conc: 24.09 ng/ml

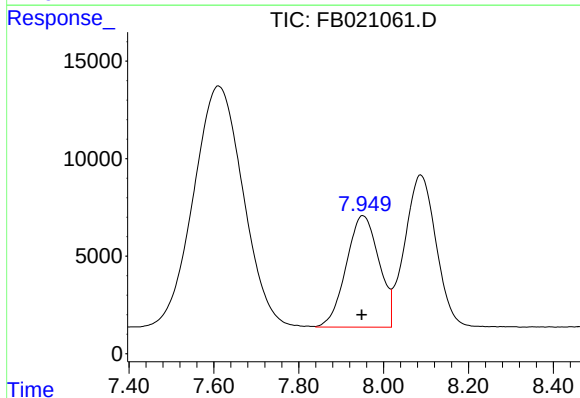


#3 n-Heptane

R.T.: 7.952 min
Delta R.T.: 0.003 min
Response: 306548
Conc: 7.74 ng/ml

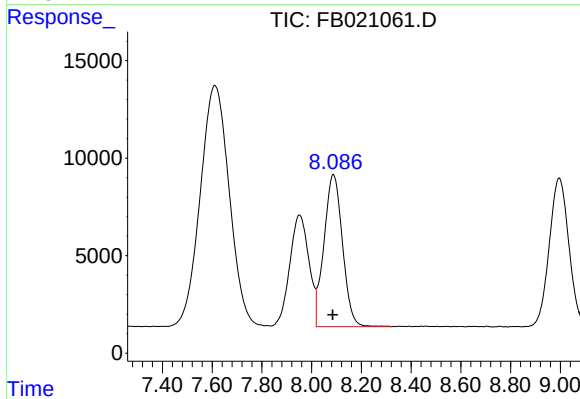

#4 Benzene


R.T.: 8.088 min
Delta R.T.: 0.004 min
Response: 403121
Conc: 9.64 ng/ml

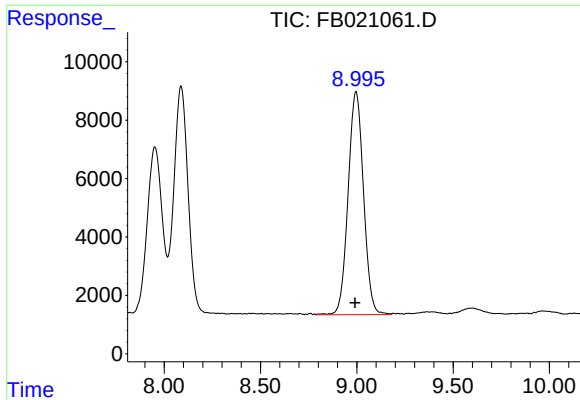

#5 AAA-TFT


R.T.: 8.996 min
Delta R.T.: 0.004 min
Response: 422193
Conc: 23.53 ng/ml

Instrument :
FID_B
ClientSampleId :

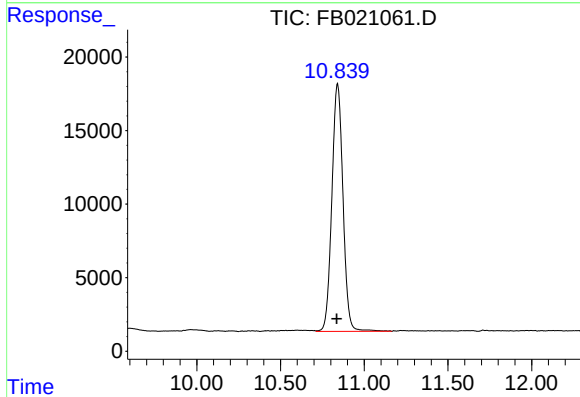


#6 Toluene

R.T.: 10.841 min
Delta R.T.: 0.005 min
Response: 777634
Conc: 28.07 ng/ml

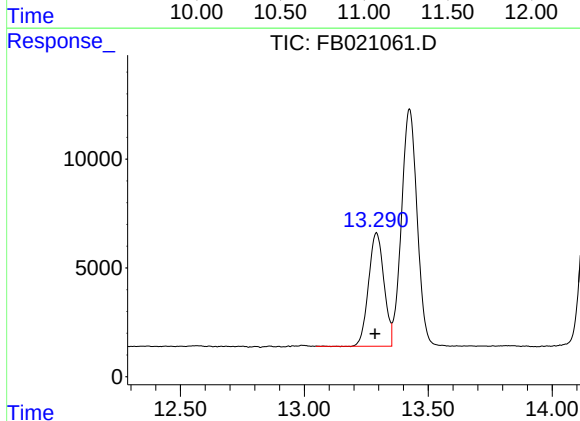


#7 Ethylbenzene

R.T.: 13.291 min
Delta R.T.: 0.006 min
Response: 225246
Conc: 8.03 ng/ml

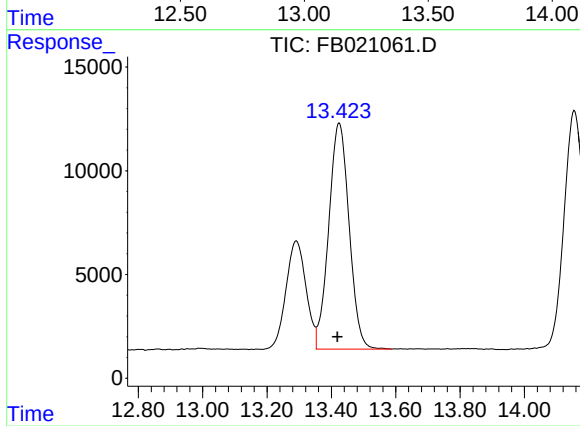

#8 m-Xylene


R.T.: 13.425 min
Delta R.T.: 0.006 min
Response: 479786
Conc: 16.14 ng/ml

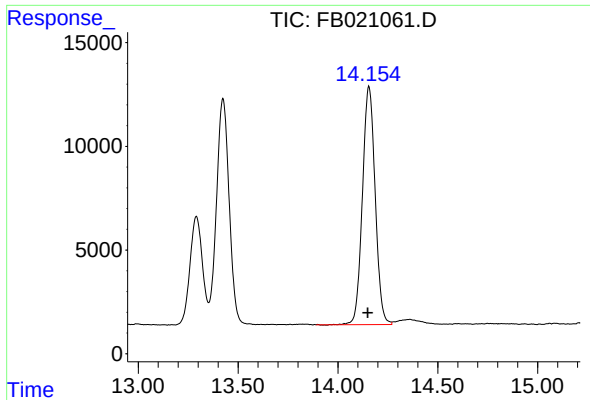

#9 O-Xylene

R.T.: 14.156 min
Delta R.T.: 0.006 min
Response: 508826
Conc: 16.42 ng/ml

Instrument :
FID_B
ClientSampleId :

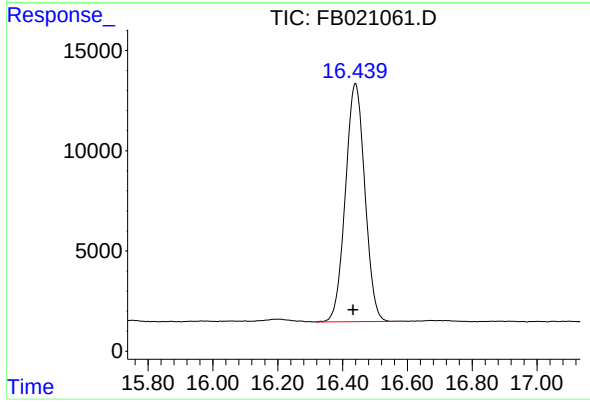

#10 1,2,4-Trimethylbenzene

R.T.: 16.440 min
Delta R.T.: 0.007 min
Response: 494791
Conc: 15.95 ng/ml