

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB051619\
 Data File : FB021062.D
 Signal(s) : FID2B.CH
 Acq On : 16 May 2019 13:44
 Operator : MJ/SJ
 Sample : K2644-01MSD
 Misc : 5.04g/5.00ml DI WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: May 16 23:15:07 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB042919.M
 Quant Title :
 QLast Update : Mon Apr 29 15:53:58 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.996	396337	22.093 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.858	1033943	22.921 ng/ml
2) t 2,2,4-Trimethylpentane	7.612	952168	22.843 ng/ml
3) t n-Heptane	7.952	291365	7.360 ng/ml
4) t Benzene	8.088	390186	9.327 ng/ml
6) t Toluene	10.841	743911	26.854 ng/ml
7) t Ethylbenzene	13.292	223021	7.952 ng/ml
8) t m-Xylene	13.425	473025	15.916 ng/ml
9) t O-Xylene	14.156	504334	16.271 ng/ml
10) t 1,2,4-Trimethylbenzene	16.439	483455	15.588 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB051619\
Data File : FB021062.D
Signal(s) : FID2B.CH
Acq On : 16 May 2019 13:44
Operator : MJ/SJ
Sample : K2644-01MSD
Misc : 5.04g/5.00ml DI WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: May 16 23:15:07 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB042919.M
Quant Title :
QLast Update : Mon Apr 29 15:53:58 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

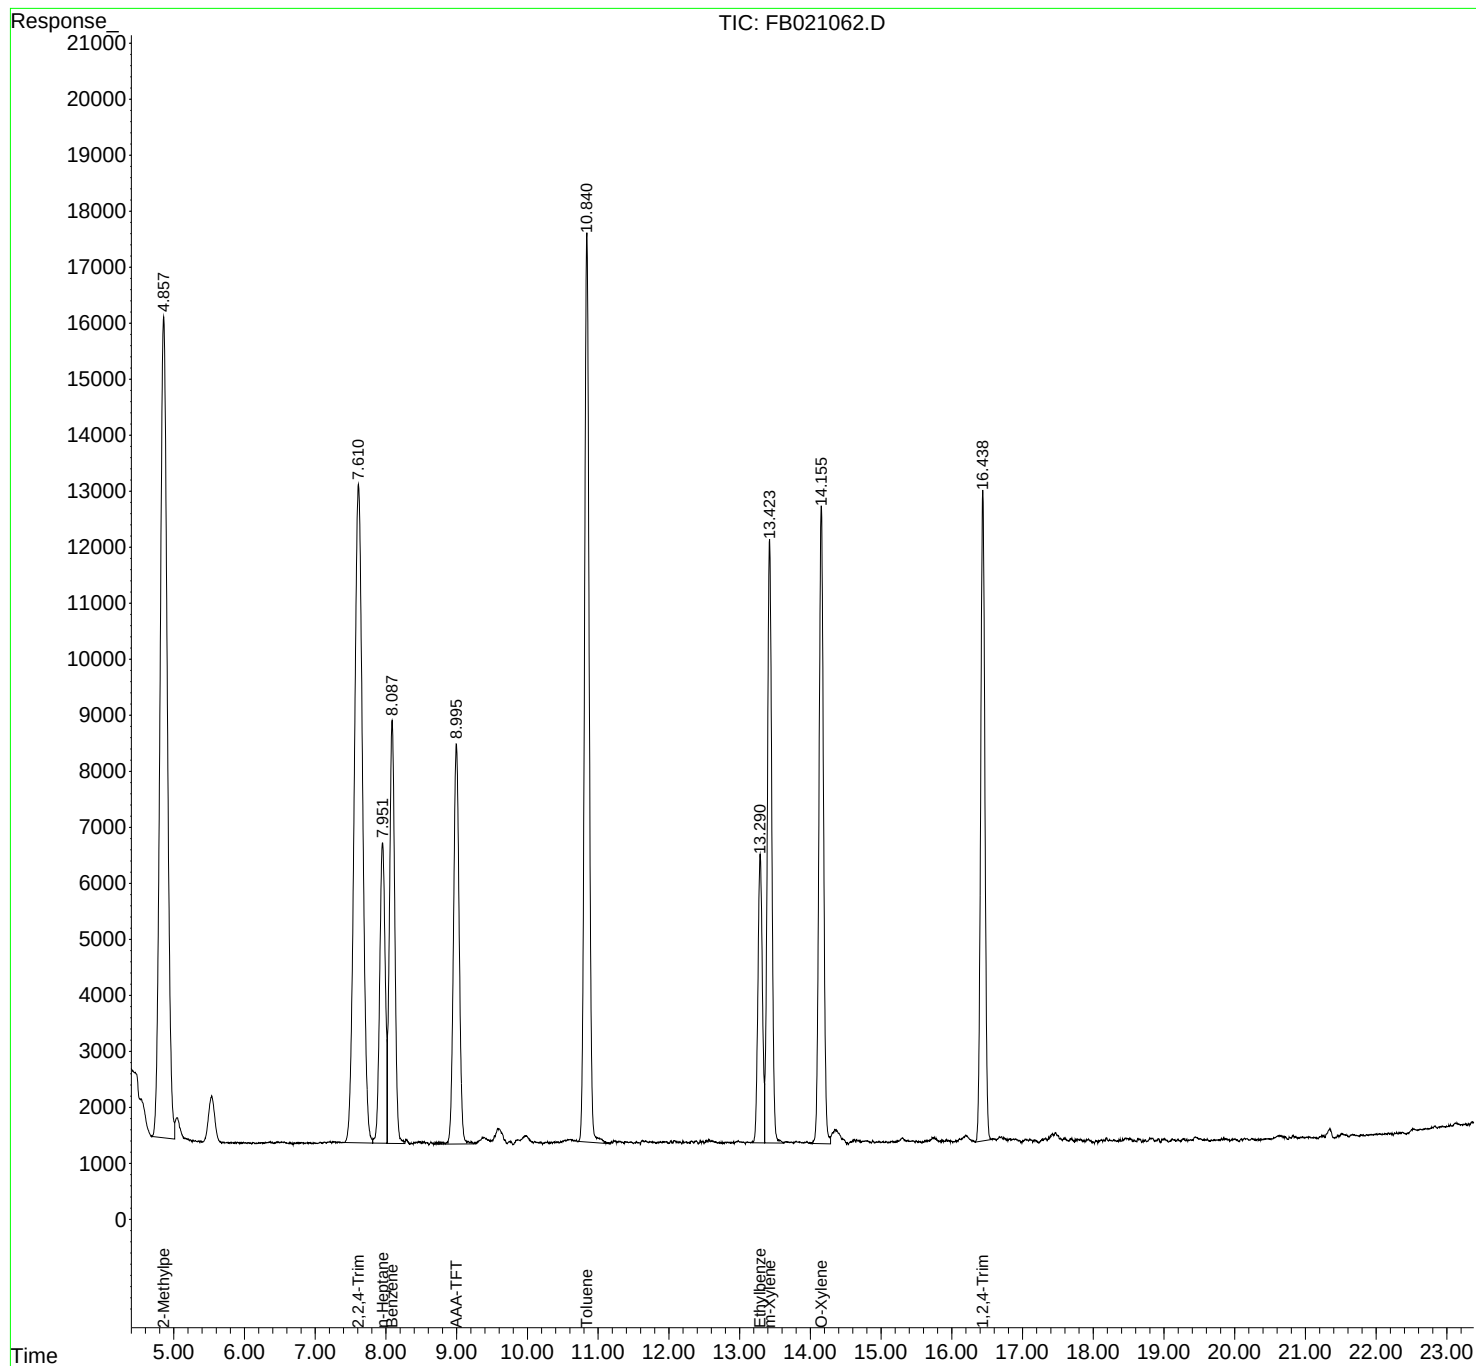


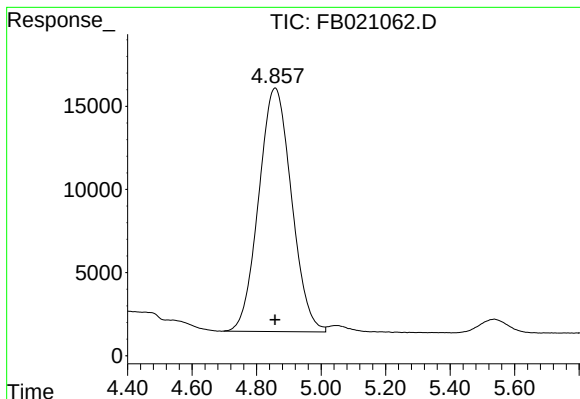

#1 2-Methylpentane


R.T.: 4.858 min
Delta R.T.: 0.001 min
Response: 1033943
Conc: 22.92 ng/ml

Instrument :
FID_B
ClientSampleId :

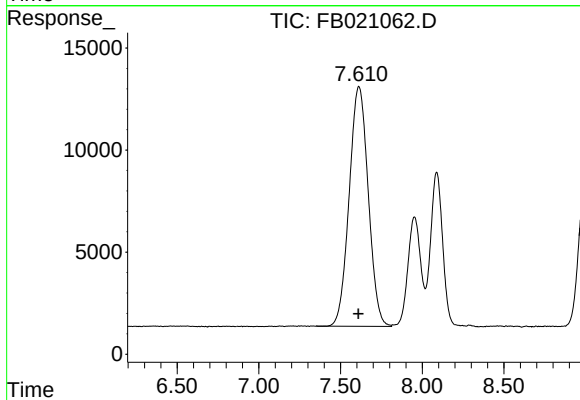


#2 2,2,4-Trimethylpentane

R.T.: 7.612 min
Delta R.T.: 0.003 min
Response: 952168
Conc: 22.84 ng/ml

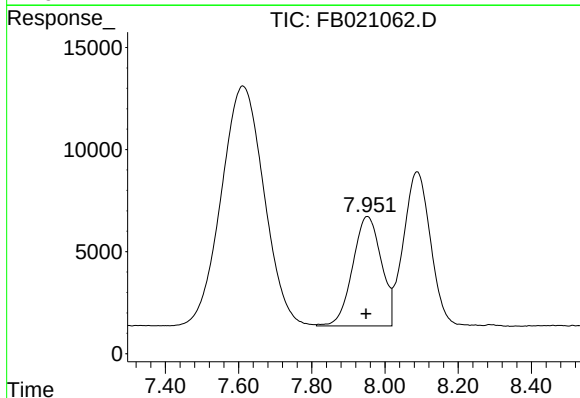


#3 n-Heptane

R.T.: 7.952 min
Delta R.T.: 0.004 min
Response: 291365
Conc: 7.36 ng/ml

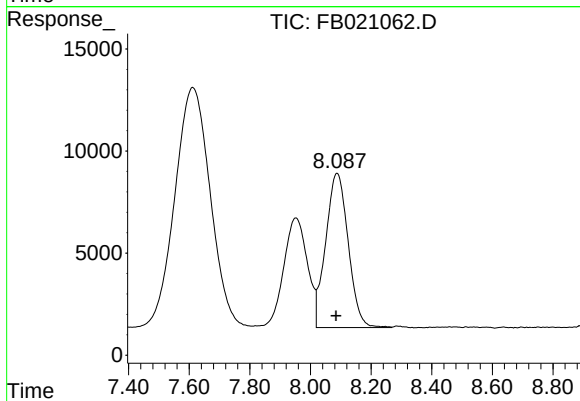


#4 Benzene

R.T.: 8.088 min
Delta R.T.: 0.004 min
Response: 390186
Conc: 9.33 ng/ml

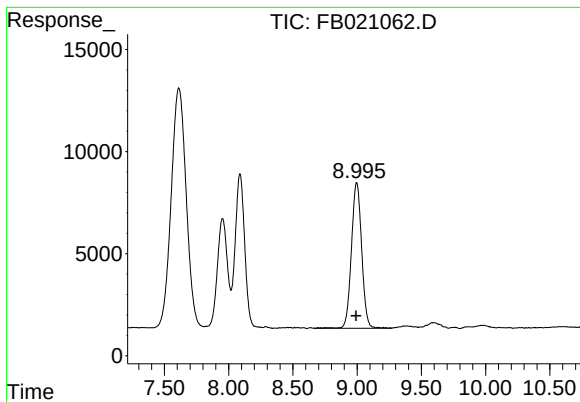


#5 AAA-TFT
 R.T.: 8.996 min
 Delta R.T.: 0.005 min
 Response: 396337
 Conc: 22.09 ng/ml


Instrument :
 FID_B
 ClientSampleId :

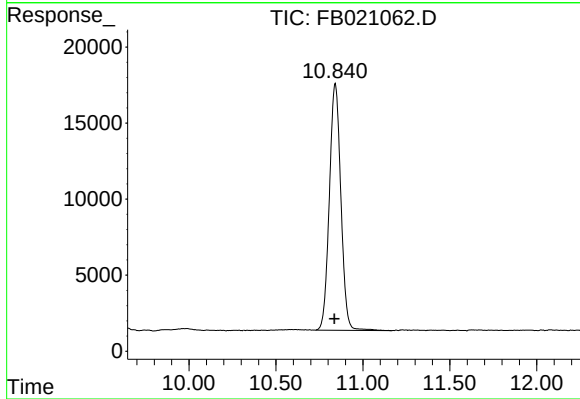


#6 Toluene
 R.T.: 10.841 min
 Delta R.T.: 0.005 min
 Response: 743911
 Conc: 26.85 ng/ml

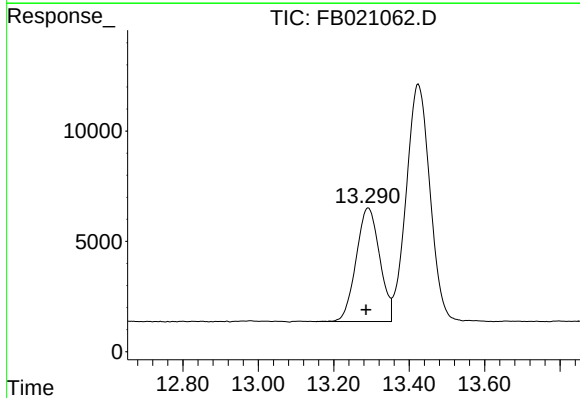

#7 Ethylbenzene
 R.T.: 13.292 min
 Delta R.T.: 0.006 min
 Response: 223021
 Conc: 7.95 ng/ml

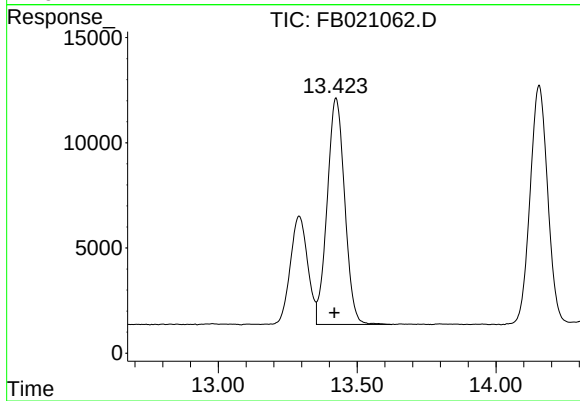


#8 m-Xylene
 R.T.: 13.425 min
 Delta R.T.: 0.006 min
 Response: 473025
 Conc: 15.92 ng/ml

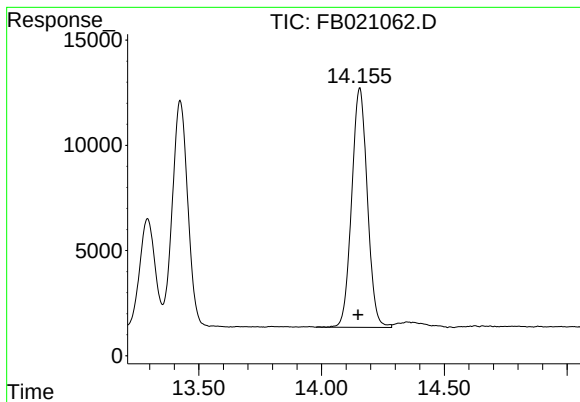

#9 O-Xylene

R.T.: 14.156 min
Delta R.T.: 0.006 min
Response: 504334
Conc: 16.27 ng/ml

Instrument :
FID_B
ClientSampleId :

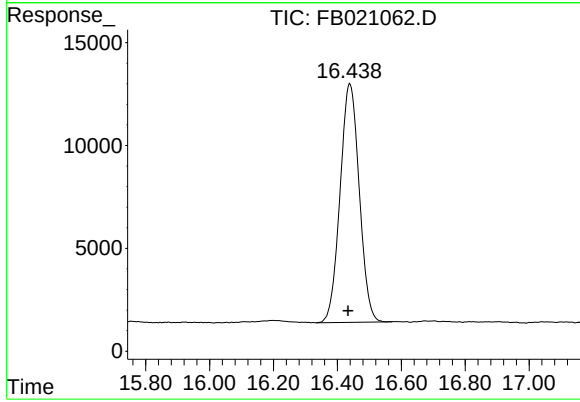

#10 1,2,4-Trimethylbenzene

R.T.: 16.439 min
Delta R.T.: 0.006 min
Response: 483455
Conc: 15.59 ng/ml